

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042619\
 Data File : P0055679.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Apr 2019 13:57
 Operator : SM/SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Manual Integrations
 APPROVED

mohammad
 4/30/2019 3:20:53 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 26 22:36:57 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Apr 25 01:58:33 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.300	3.596	537134	552808	21.199	22.700
2) SA Decachlor...	9.923	8.563	765768	544247	17.845m	17.705

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO042619\
Data File : PO055679.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Apr 2019 13:57
Operator : SM/SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

mohammad
4/30/2019 3:20:53 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 26 22:36:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO042419.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Apr 25 01:58:33 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

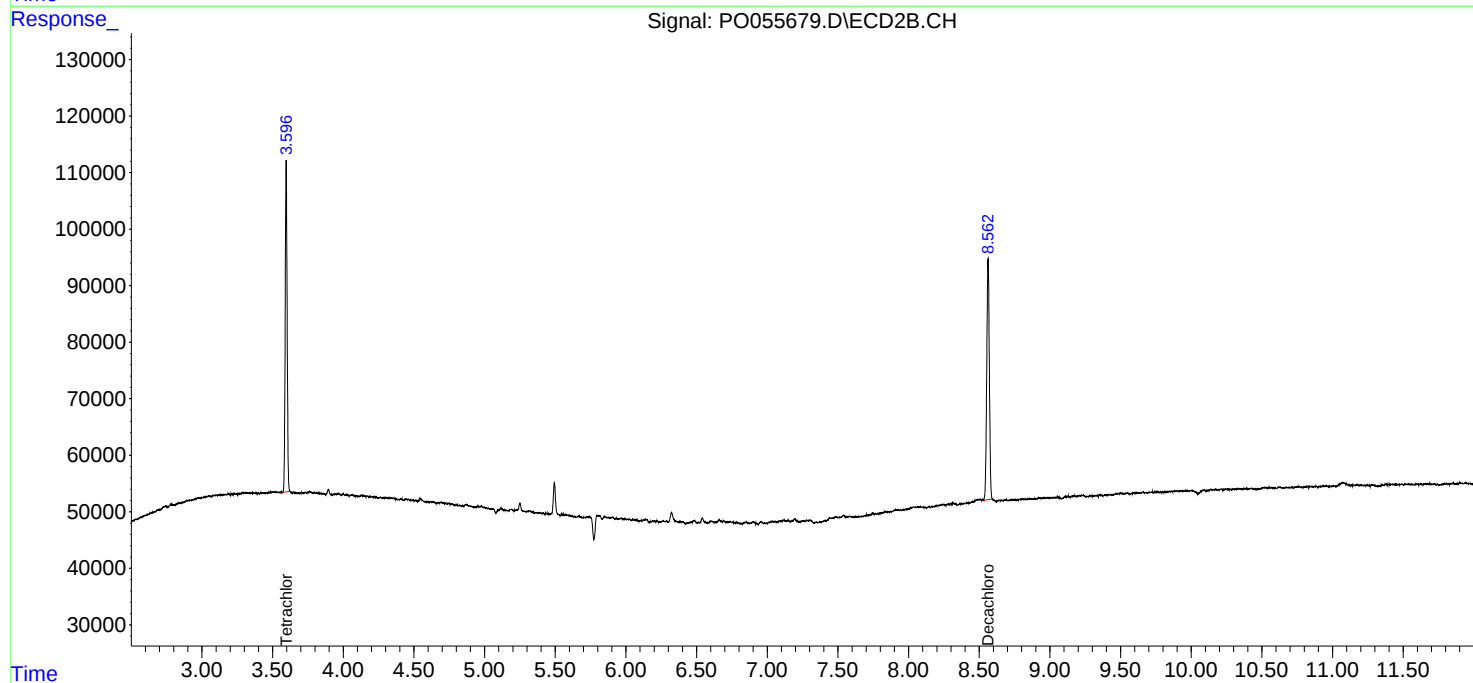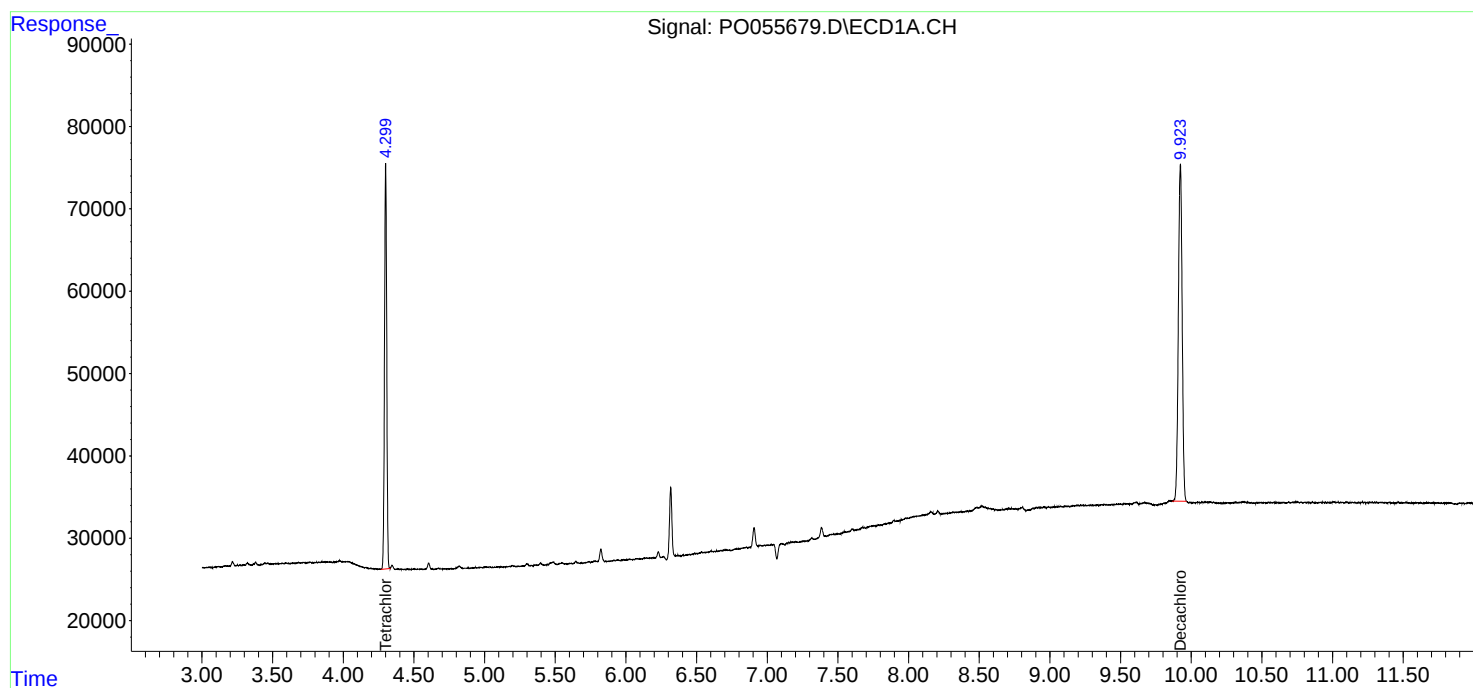

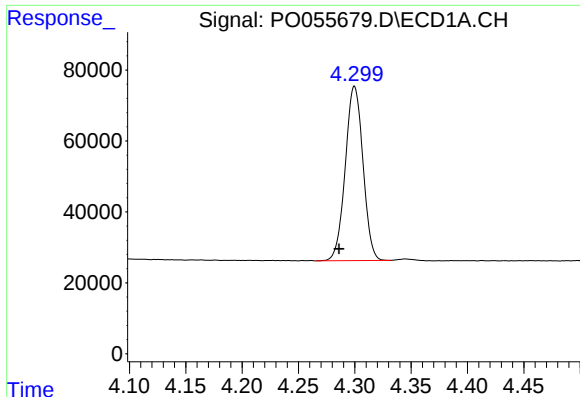


#1 Tetrachloro-m-xylene

R.T.: 4.300 min
Delta R.T.: 0.014 min
Response: 537134
Conc: 21.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

mohammad
4/30/2019 3:20:53 PM

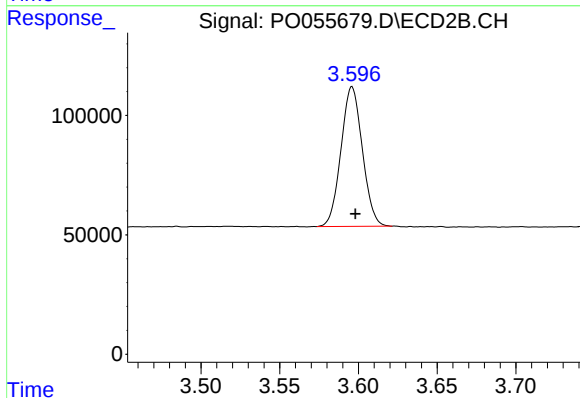


#1 Tetrachloro-m-xylene

R.T.: 3.596 min
Delta R.T.: -0.002 min
Response: 552808
Conc: 22.70 ng/ml

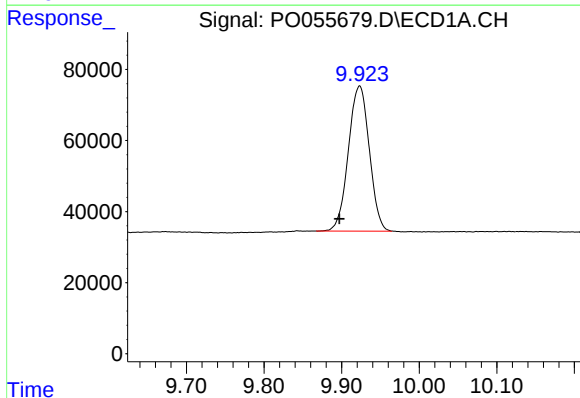

#2 Decachlorobiphenyl

R.T.: 9.923 min
Delta R.T.: 0.026 min
Response: 765768
Conc: 17.84 ng/ml m

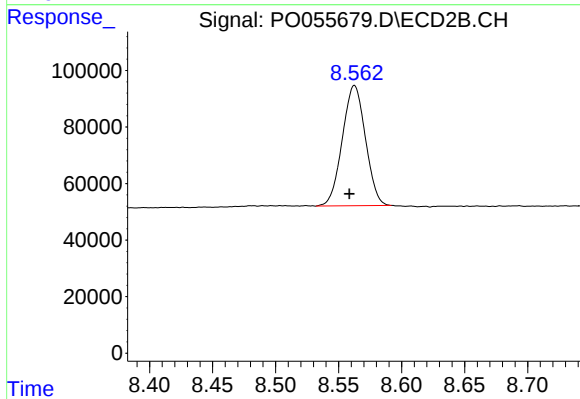

#2 Decachlorobiphenyl

R.T.: 8.563 min
Delta R.T.: 0.004 min
Response: 544247
Conc: 17.71 ng/ml