

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042621\
 Data File : P0077293.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Apr 2021 11:51
 Operator : DD\AJ
 Sample : M2142-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 EO-04-042221

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 26 17:53:03 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 21 09:50:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.894	3.888	2199306	1074934	20.811	20.432
2) SA Decachlor...	10.860	9.126	2135481	704583	20.568	18.673

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042621\
Data File : P0077293.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Apr 2021 11:51
Operator : DD\AJ
Sample : M2142-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
EO-04-042221

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 26 17:53:03 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042121.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 21 09:50:22 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

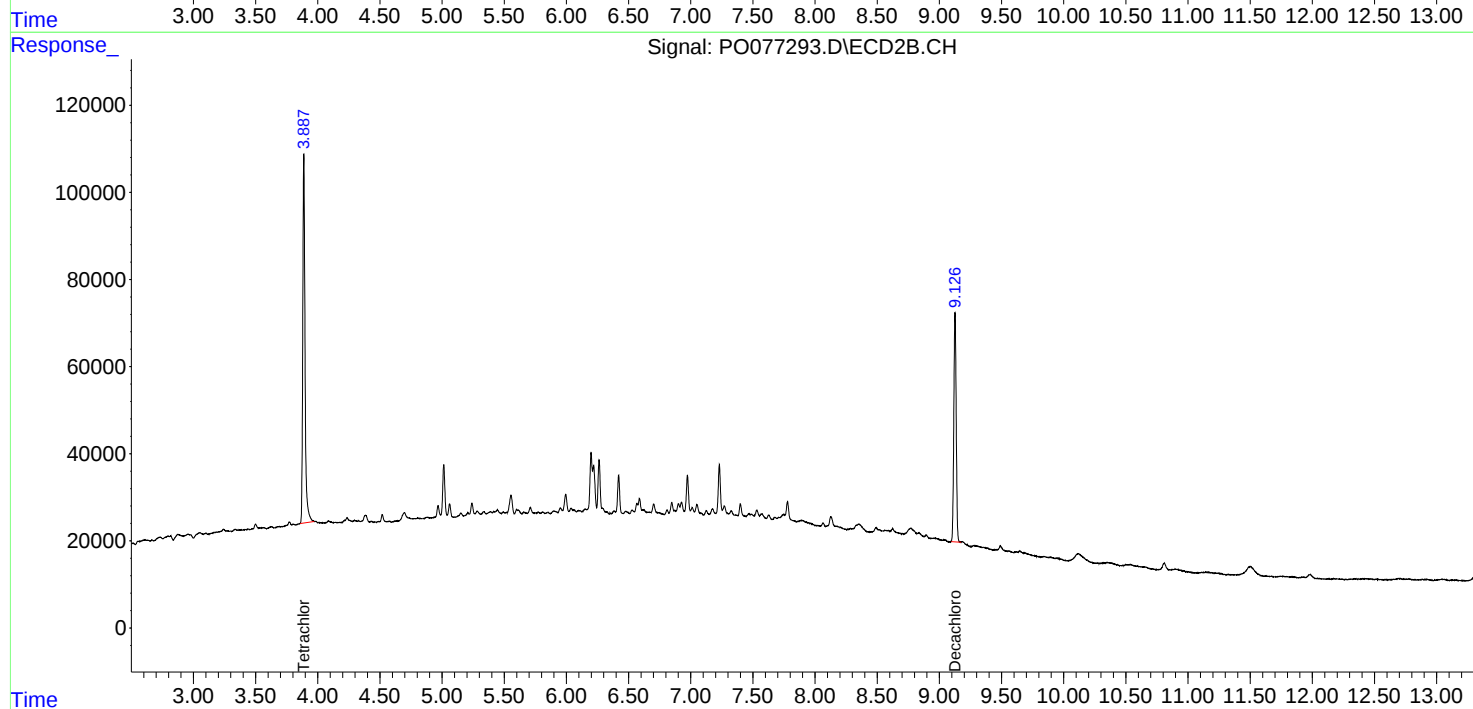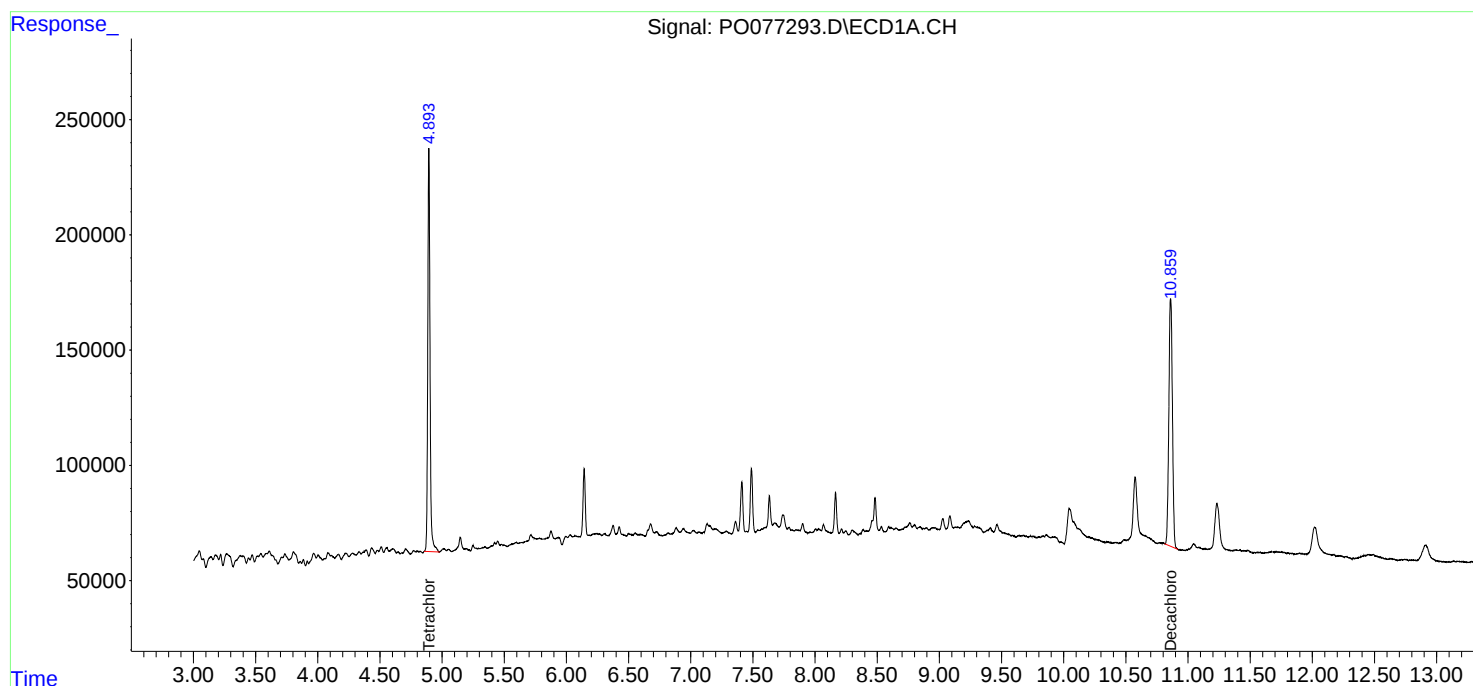


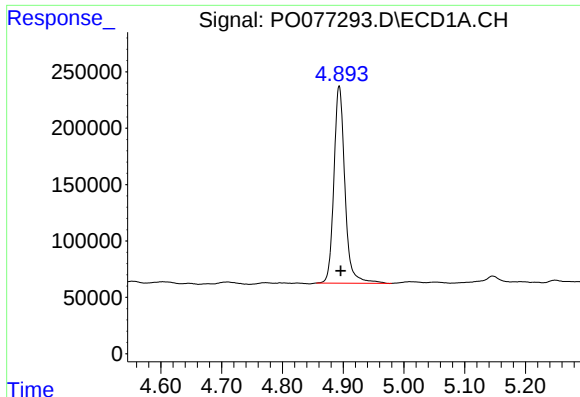

#1 Tetrachloro-m-xylene


R.T.: 4.894 min
Delta R.T.: -0.002 min
Response: 2199306
Conc: 20.81 ng/ml

Instrument :
ECD_O
ClientSampleId :
EO-04-042221

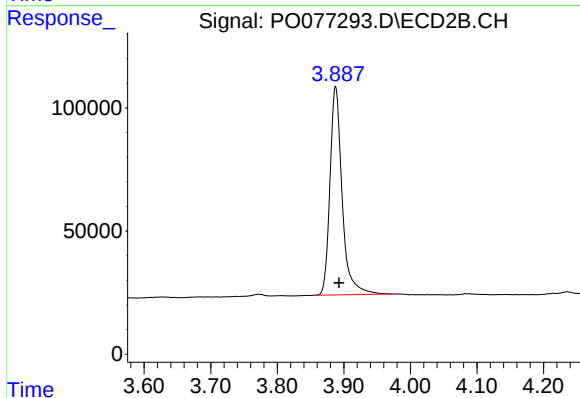


#1 Tetrachloro-m-xylene

R.T.: 3.888 min
Delta R.T.: -0.005 min
Response: 1074934
Conc: 20.43 ng/ml

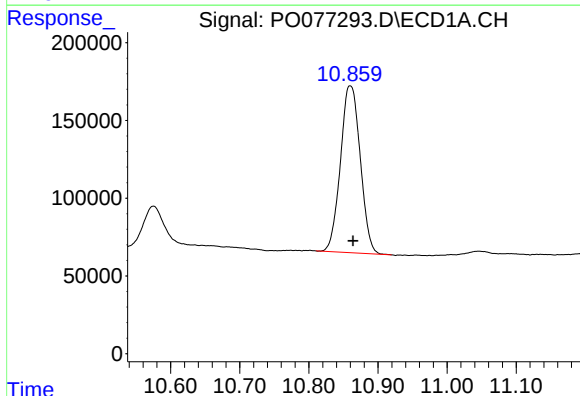

#2 Decachlorobiphenyl

R.T.: 10.860 min
Delta R.T.: -0.004 min
Response: 2135481
Conc: 20.57 ng/ml

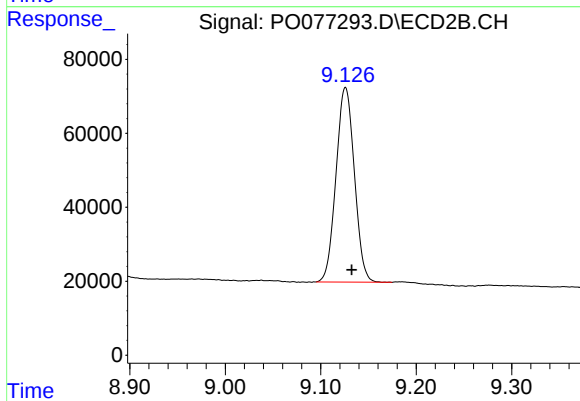

#2 Decachlorobiphenyl

R.T.: 9.126 min
Delta R.T.: -0.006 min
Response: 704583
Conc: 18.67 ng/ml