

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042621\
 Data File : P0077309.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Apr 2021 17:30
 Operator : DD\AJ
 Sample : M2170-11
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CS-1

Manual Integrations
 APPROVED

Ankita
 4/27/2021 12:54:55 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 27 02:02:49 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 21 09:50:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.896	3.891	2172355	1007541	20.556	19.151
2) SA Decachlor...	10.861	9.126	1528694	488882	14.724	12.956
Target Compounds						
26) L6 AR-1254-1	7.127	5.994	177442	104397	43.150	36.166m
27) L6 AR-1254-2	7.359	6.153	168625	45458	26.054	17.607m#
28) L6 AR-1254-3	7.738	6.568	286661	188299	42.362	48.128m
29) L6 AR-1254-4	8.032	6.808	119767	35672	24.354m	15.701m#
30) L6 AR-1254-5	8.459	7.231	224911	481043	40.401m	132.673m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042621\
Data File : P0077309.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Apr 2021 17:30
Operator : DD\AJ
Sample : M2170-11
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
CS-1


Manual Integrations
APPROVED

Ankita
4/27/2021 12:54:55 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 27 02:02:49 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042121.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 21 09:50:22 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

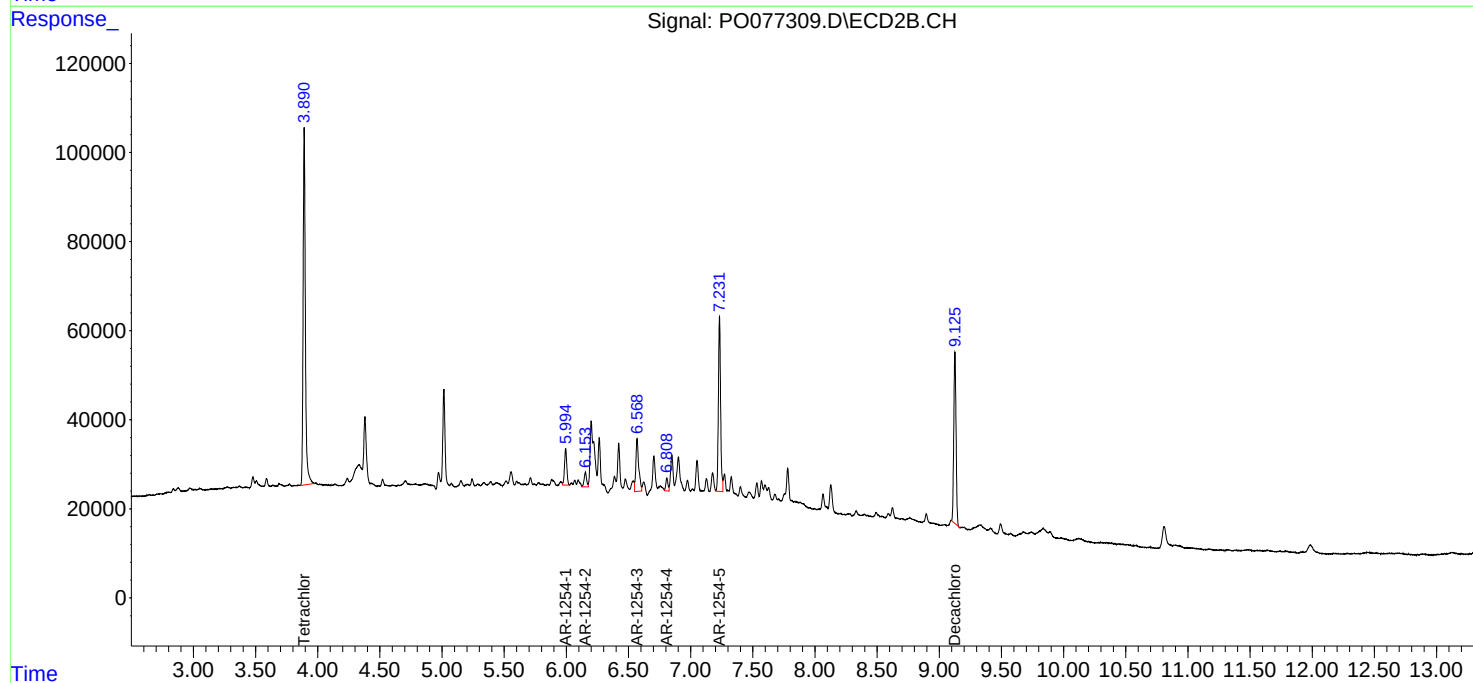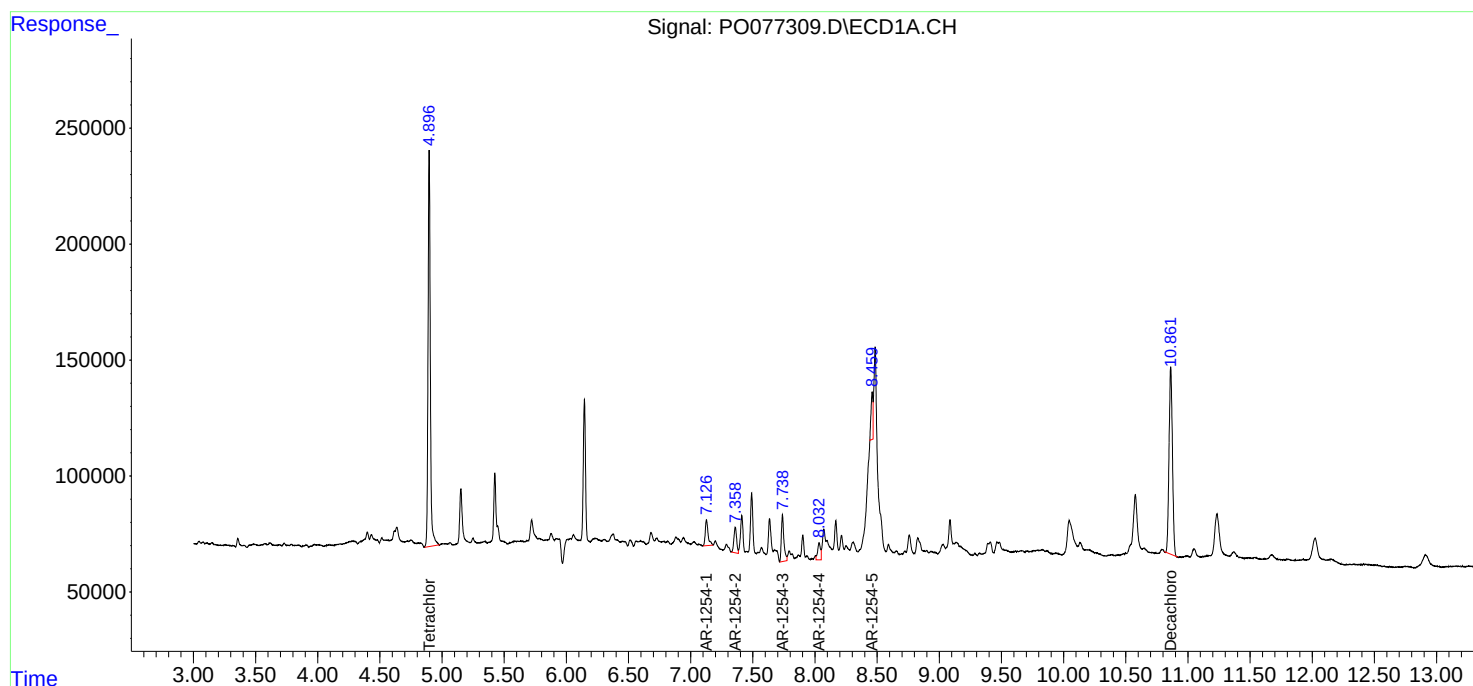

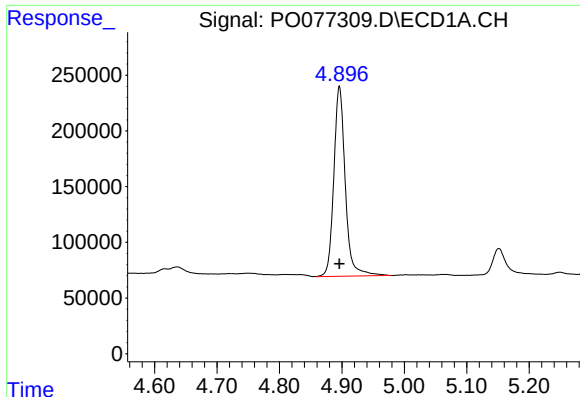


#1 Tetrachloro-m-xylene

R.T.: 4.896 min
Delta R.T.: 0.000 min
Response: 2172355
Conc: 20.56 ng/ml

Instrument :
ECD_O
ClientSampleId :
CS-1


Manual Integrations
APPROVED

Ankita
4/27/2021 12:54:55 PM

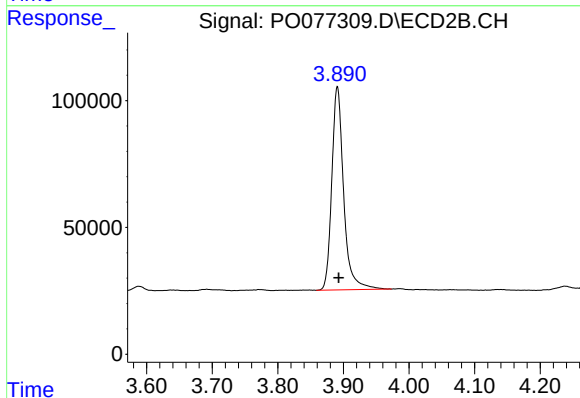


#1 Tetrachloro-m-xylene

R.T.: 3.891 min
Delta R.T.: -0.002 min
Response: 1007541
Conc: 19.15 ng/ml

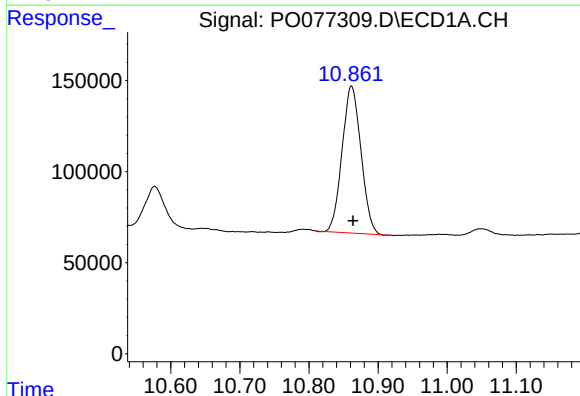


#2 Decachlorobiphenyl

R.T.: 10.861 min
Delta R.T.: -0.002 min
Response: 1528694
Conc: 14.72 ng/ml

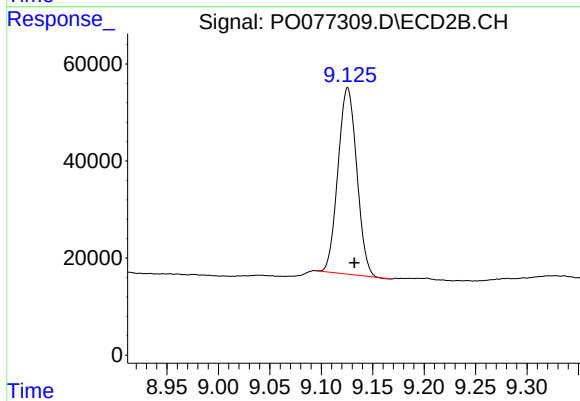

#2 Decachlorobiphenyl

R.T.: 9.126 min
Delta R.T.: -0.007 min
Response: 488882
Conc: 12.96 ng/ml

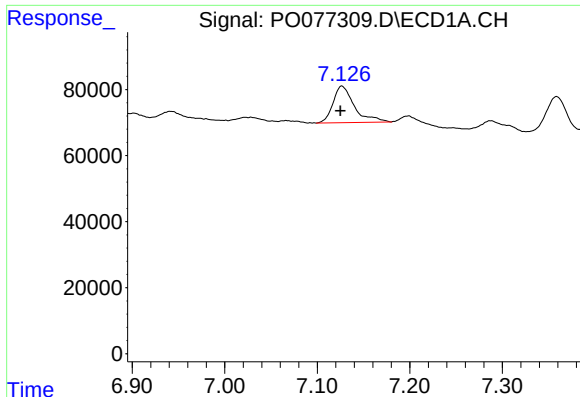


#26 AR-1254-1

R.T.: 7.127 min
Delta R.T.: 0.002 min
Response: 177442
Conc: 43.15 ng/ml

Instrument :
ECD_O
ClientSampleId :
CS-1


Manual Integrations
APPROVED

Ankita
4/27/2021 12:54:55 PM

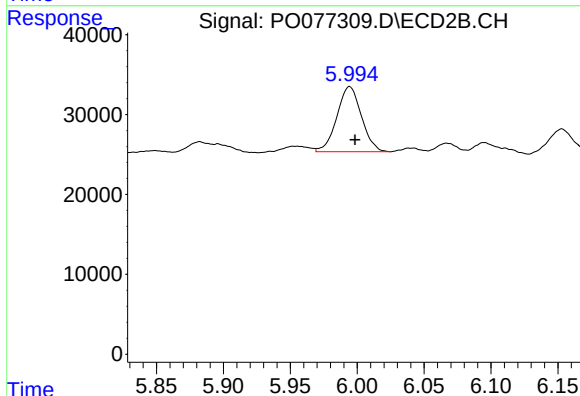


#26 AR-1254-1

R.T.: 5.994 min
Delta R.T.: -0.005 min
Response: 104397
Conc: 36.17 ng/ml m

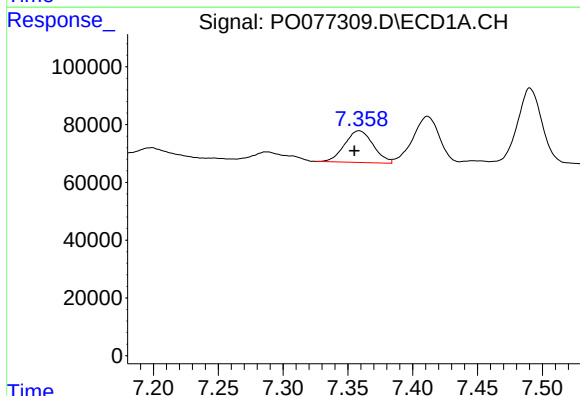


#27 AR-1254-2

R.T.: 7.359 min
Delta R.T.: 0.004 min
Response: 168625
Conc: 26.05 ng/ml

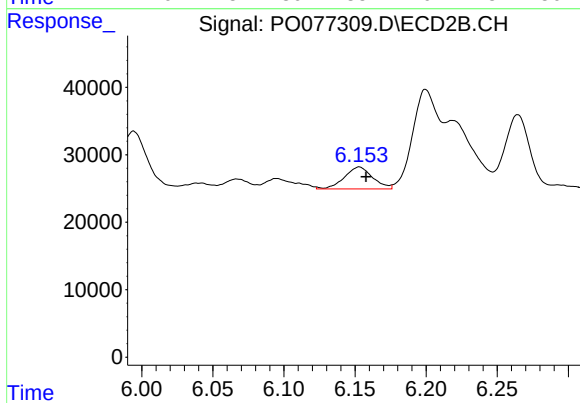

#27 AR-1254-2

R.T.: 6.153 min
Delta R.T.: -0.005 min
Response: 45458
Conc: 17.61 ng/ml m

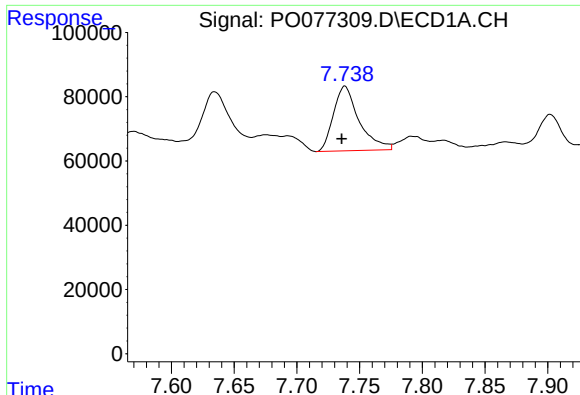


#28 AR-1254-3

R.T.: 7.738 min
Delta R.T.: 0.003 min
Response: 286661
Conc: 42.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
CS-1


Manual Integrations
APPROVED

Ankita
4/27/2021 12:54:55 PM

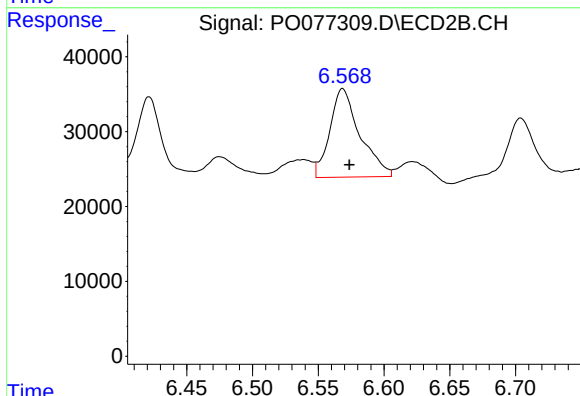


#28 AR-1254-3

R.T.: 6.568 min
Delta R.T.: -0.006 min
Response: 188299
Conc: 48.13 ng/ml m

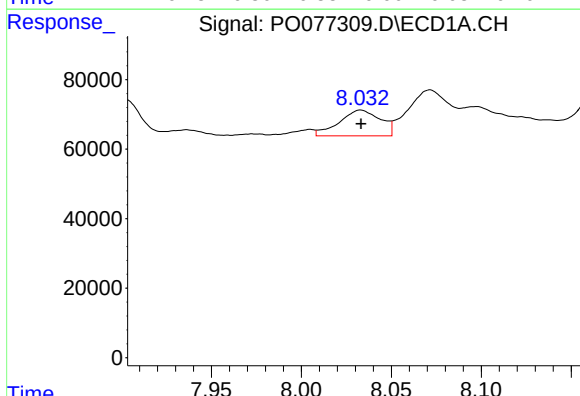


#29 AR-1254-4

R.T.: 8.032 min
Delta R.T.: 0.000 min
Response: 119767
Conc: 24.35 ng/ml m

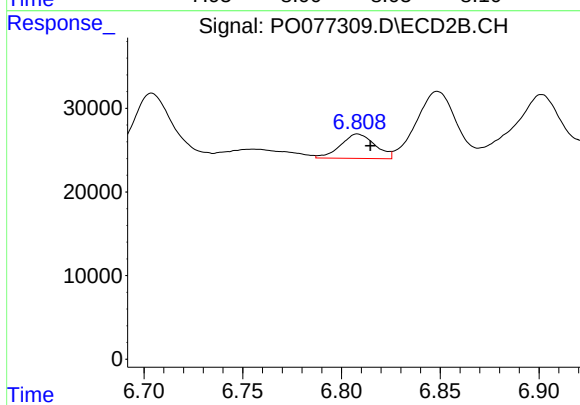

#29 AR-1254-4

R.T.: 6.808 min
Delta R.T.: -0.007 min
Response: 35672
Conc: 15.70 ng/ml m

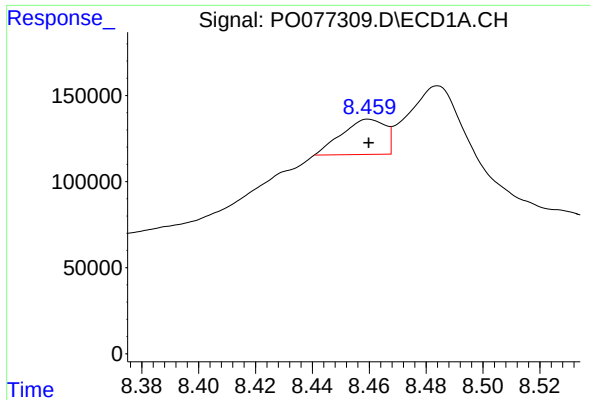


#30 AR-1254-5

R.T.: 8.459 min
Delta R.T.: 0.000 min
Response: 224911
Conc: 40.40 ng/ml m

Instrument :
ECD_O
ClientSampleId :
CS-1

Manual Integrations
APPROVED

Ankita
4/27/2021 12:54:55 PM

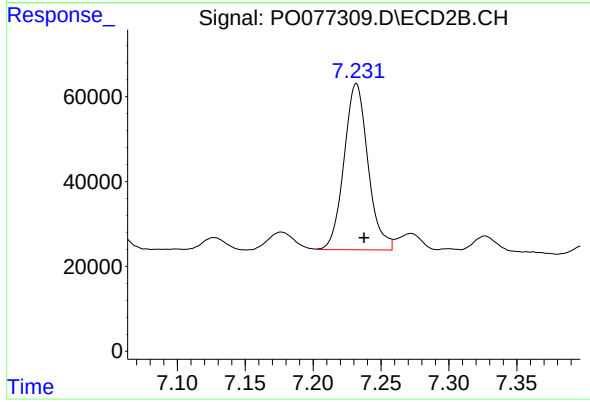

#30 AR-1254-5

R.T.: 7.231 min
Delta R.T.: -0.006 min
Response: 481043
Conc: 132.67 ng/ml m