

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_O\Data\P0042621\  
 Data File : P0077319.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 26 Apr 2021 20:39  
 Operator : DD\AJ  
 Sample : M2160-01  
 Misc :  
 ALS Vial : 28 Sample Multiplier: 1

Instrument :  
 ECD\_O  
 ClientSampleId :  
 OK-03-042321

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 27 02:07:51 2021  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_O\methods\P0042121.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Apr 21 09:50:22 2021  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound                    | RT#1   | RT#2  | Resp#1  | Resp#2 | ng/ml  | ng/ml  |
|-----------------------------|--------|-------|---------|--------|--------|--------|
| -----                       |        |       |         |        |        |        |
| System Monitoring Compounds |        |       |         |        |        |        |
| 1) SA Tetrachlo...          | 4.896  | 3.892 | 2013712 | 956512 | 19.054 | 18.181 |
| 2) SA Decachlor...          | 10.863 | 9.127 | 1732960 | 554924 | 16.692 | 14.706 |

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_O\Data\P0042621\  
Data File : P0077319.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 26 Apr 2021 20:39  
Operator : DD\AJ  
Sample : M2160-01  
Misc :  
ALS Vial : 28 Sample Multiplier: 1

Instrument :  
ECD\_O  
ClientSampleId :  
OK-03-042321

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Apr 27 02:07:51 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_O\methods\P0042121.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Wed Apr 21 09:50:22 2021  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

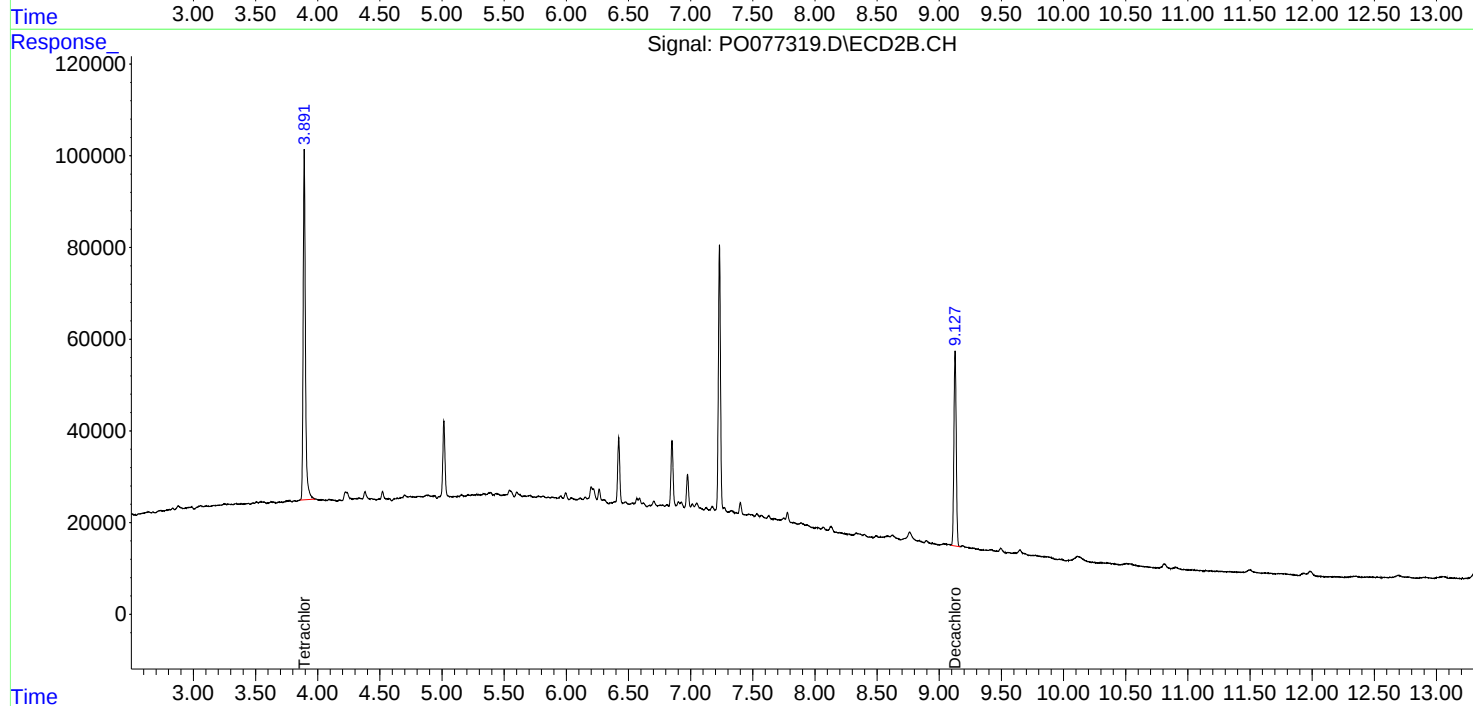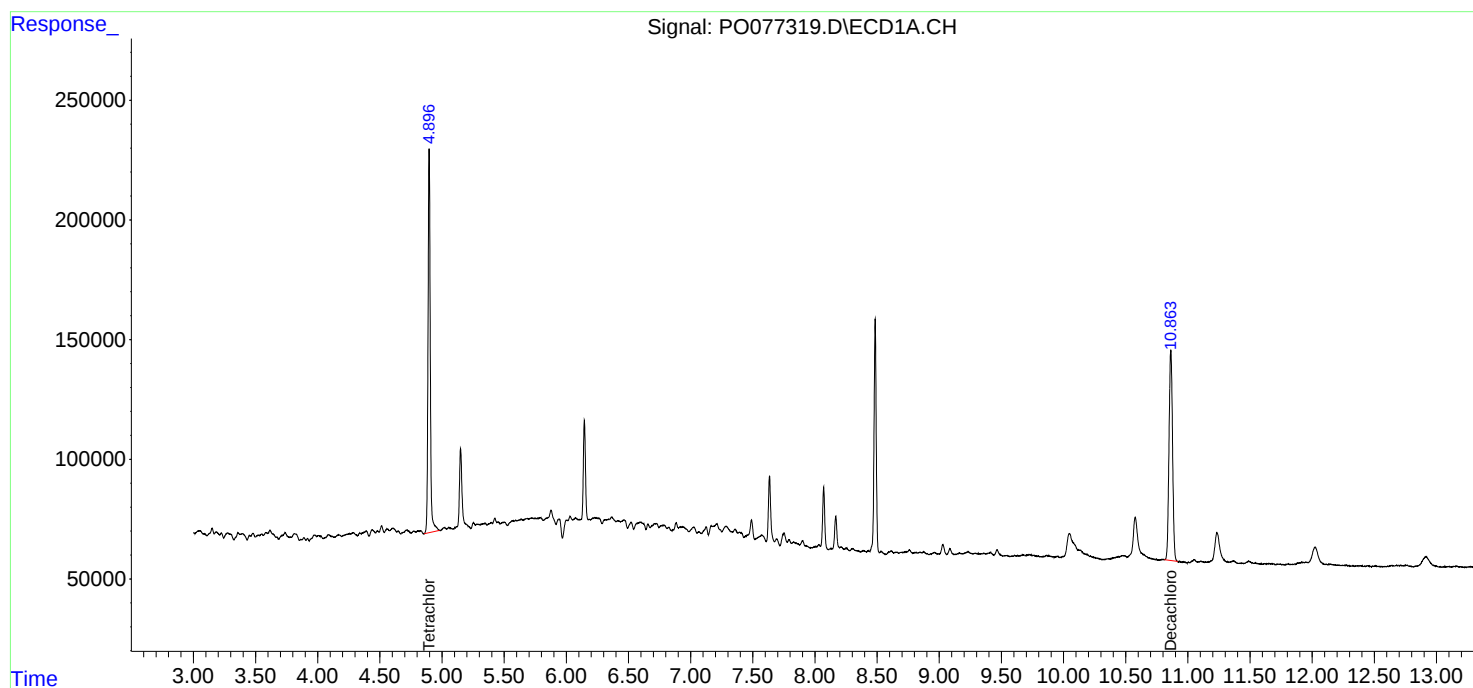


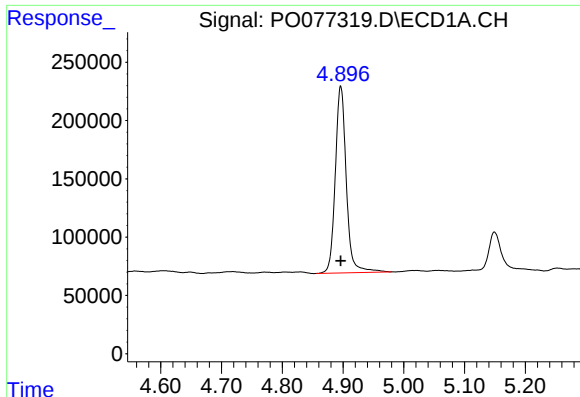

#1 Tetrachloro-m-xylene


R.T.: 4.896 min  
Delta R.T.: 0.000 min  
Response: 2013712  
Conc: 19.05 ng/ml

Instrument :  
ECD\_O  
ClientSampleId :  
OK-03-042321

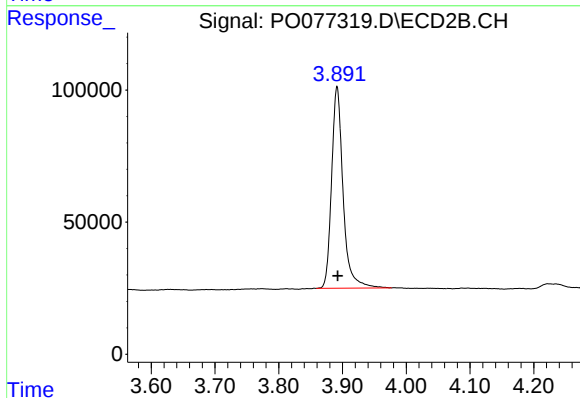


#1 Tetrachloro-m-xylene

R.T.: 3.892 min  
Delta R.T.: -0.001 min  
Response: 956512  
Conc: 18.18 ng/ml

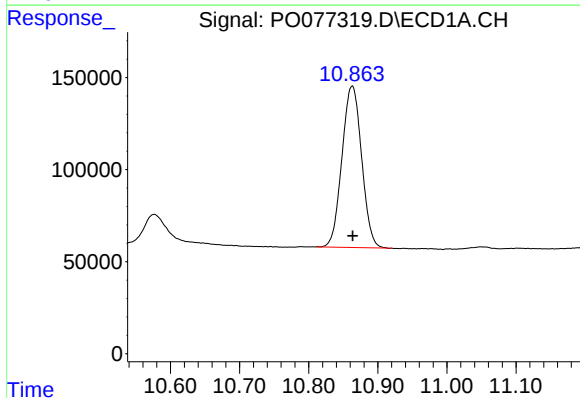

#2 Decachlorobiphenyl

R.T.: 10.863 min  
Delta R.T.: 0.000 min  
Response: 1732960  
Conc: 16.69 ng/ml

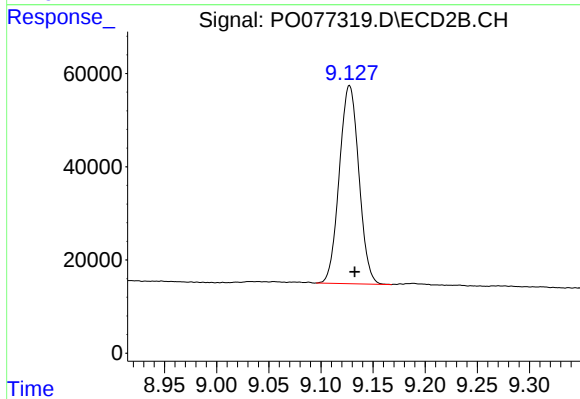

#2 Decachlorobiphenyl

R.T.: 9.127 min  
Delta R.T.: -0.005 min  
Response: 554924  
Conc: 14.71 ng/ml