

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042621\
 Data File : P0077320.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Apr 2021 20:56
 Operator : DD\AJ
 Sample : M2163-01
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TT-059-RW8-IDWSO-202104-1

Manual Integrations
 APPROVED

Ankita
 4/27/2021 12:54:58 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 27 02:08:07 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 21 09:50:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.896	3.891	2234833	968910	21.147	18.416m
2) SA Decachlor...	10.859	9.126	1910996	603025	18.406	15.981

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042621\
Data File : P0077320.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Apr 2021 20:56
Operator : DD\AJ
Sample : M2163-01
Misc :
ALS Vial : 29 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TT-059-RW8-IDWSO-202104-1


Manual Integrations
APPROVED

Ankita
4/27/2021 12:54:58 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 27 02:08:07 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042121.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 21 09:50:22 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

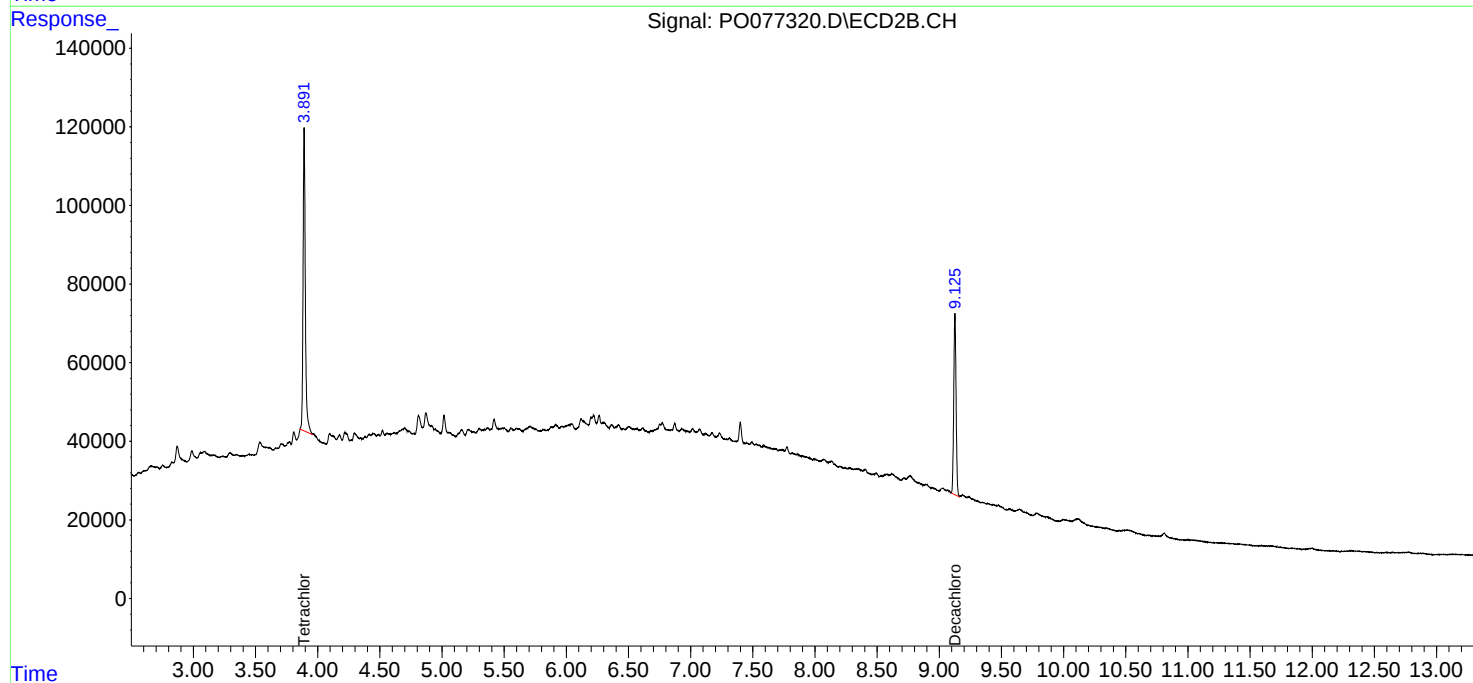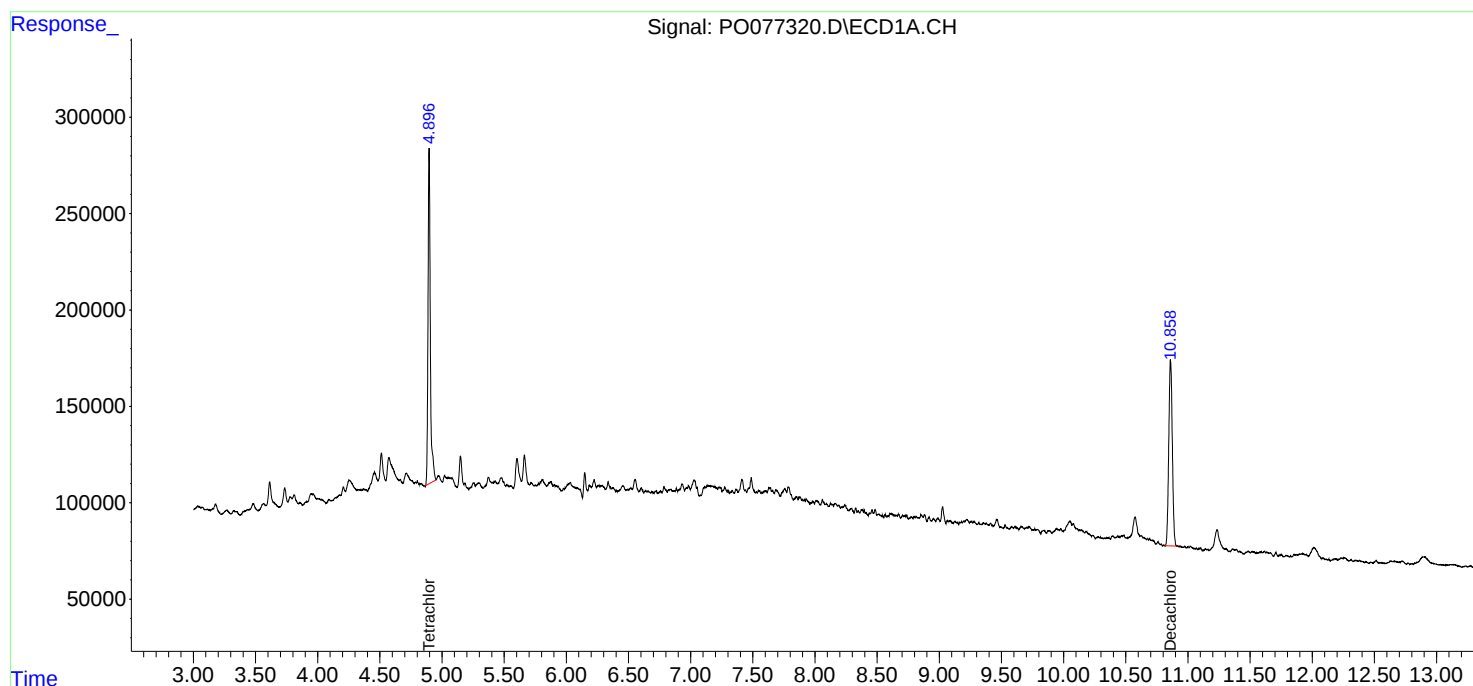

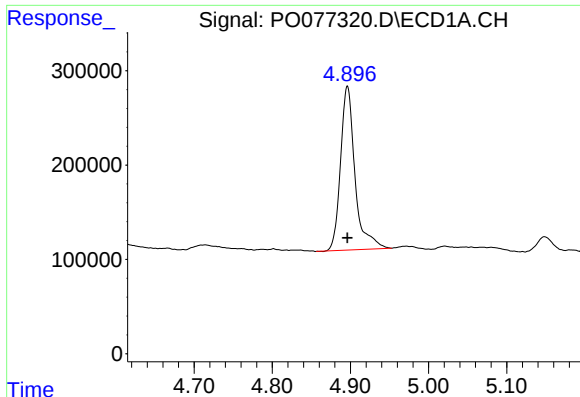


#1 Tetrachloro-m-xylene

R.T.: 4.896 min
Delta R.T.: 0.000 min
Response: 2234833
Conc: 21.15 ng/ml

Instrument :
ECD_O
ClientSampleId :
TT-059-RW8-IDWSO-202104-1


Manual Integrations
APPROVED

Ankita
4/27/2021 12:54:58 PM

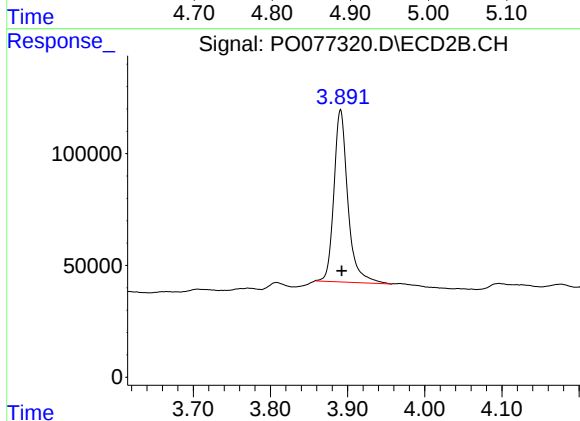


#1 Tetrachloro-m-xylene

R.T.: 3.891 min
Delta R.T.: -0.002 min
Response: 968910
Conc: 18.42 ng/ml m

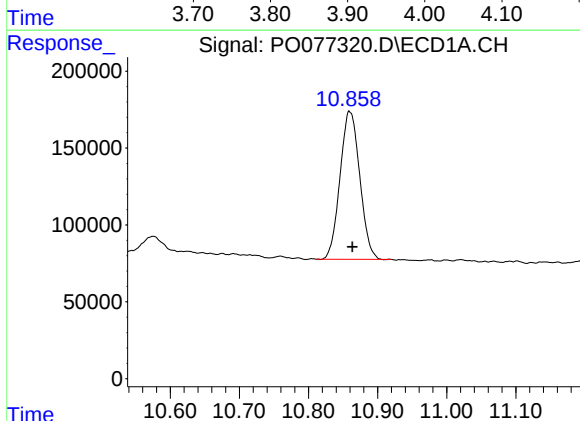

#2 Decachlorobiphenyl

R.T.: 10.859 min
Delta R.T.: -0.004 min
Response: 1910996
Conc: 18.41 ng/ml

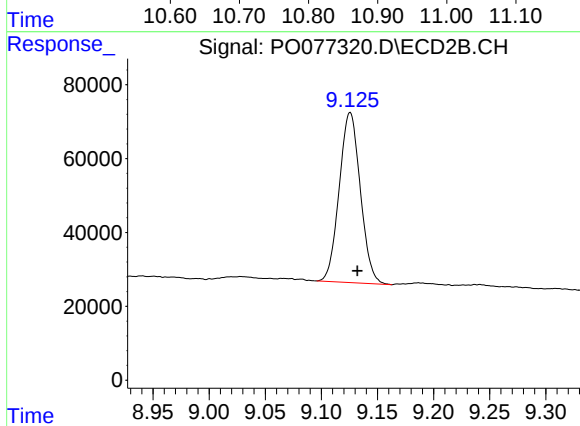

#2 Decachlorobiphenyl

R.T.: 9.126 min
Delta R.T.: -0.007 min
Response: 603025
Conc: 15.98 ng/ml