

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042621\
 Data File : P0077332.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Apr 2021 00:38
 Operator : DD\AJ
 Sample : M2153-03
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PLA-109

Manual Integrations
 APPROVED

Ankita
 4/27/2021 12:55:05 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 27 02:14:22 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 21 09:50:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.896	3.891	2051402	973304	19.411	18.500
2) SA Decachlor...	10.859	9.125	1812693	618981	17.459	16.404
Target Compounds						
16) L4 AR-1242-1	6.218	5.133	130626	63920	48.086	58.349
17) L4 AR-1242-2	6.242	5.153	197212	105054	44.706	46.238
18) L4 AR-1242-3	6.307	5.340	126001	55629	45.431	54.449
19) L4 AR-1242-4	6.414	5.435	89550	53075	41.737m	46.717
20) L4 AR-1242-5	7.196	5.994	120194	80949	51.982	57.692

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO042621\
Data File : PO077332.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Apr 2021 00:38
Operator : DD\AJ
Sample : M2153-03
Misc :
ALS Vial : 38 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
PLA-109


Manual Integrations
APPROVED

Ankita
4/27/2021 12:55:05 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 27 02:14:22 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO042121.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 21 09:50:22 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

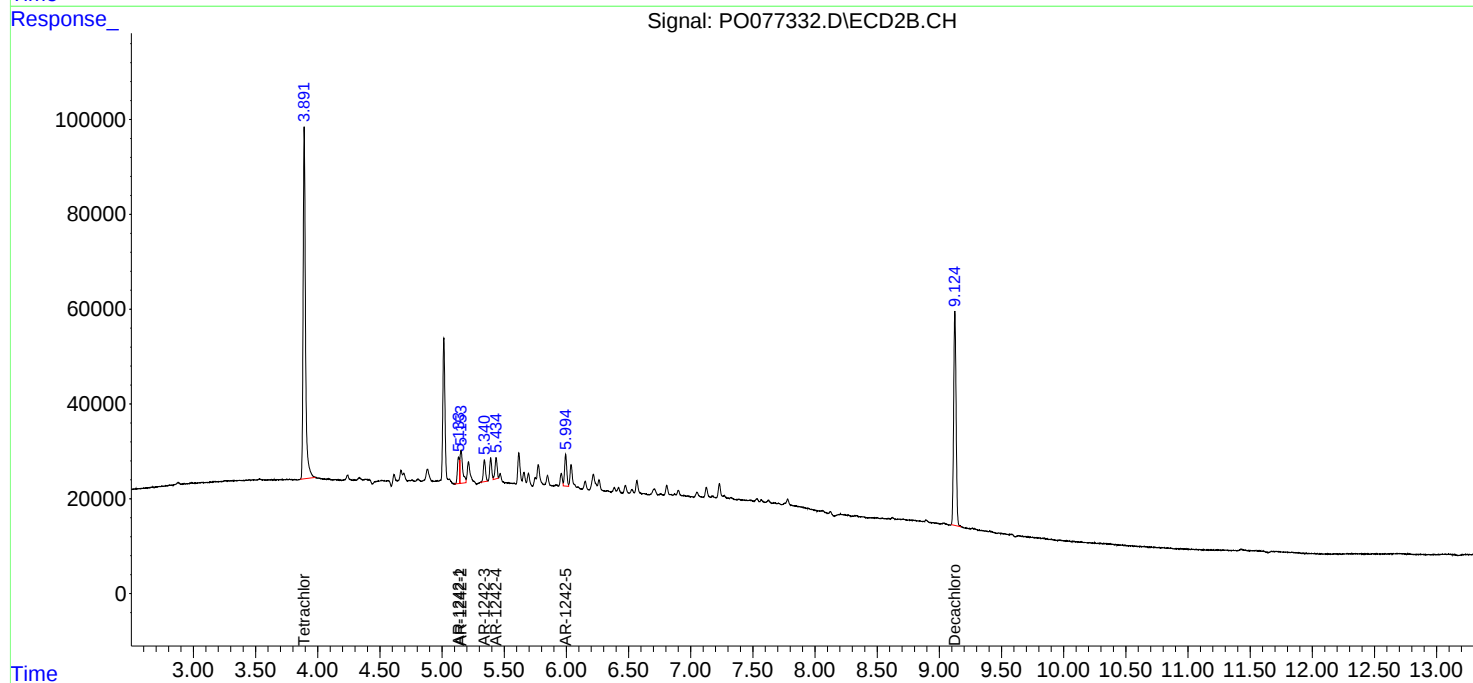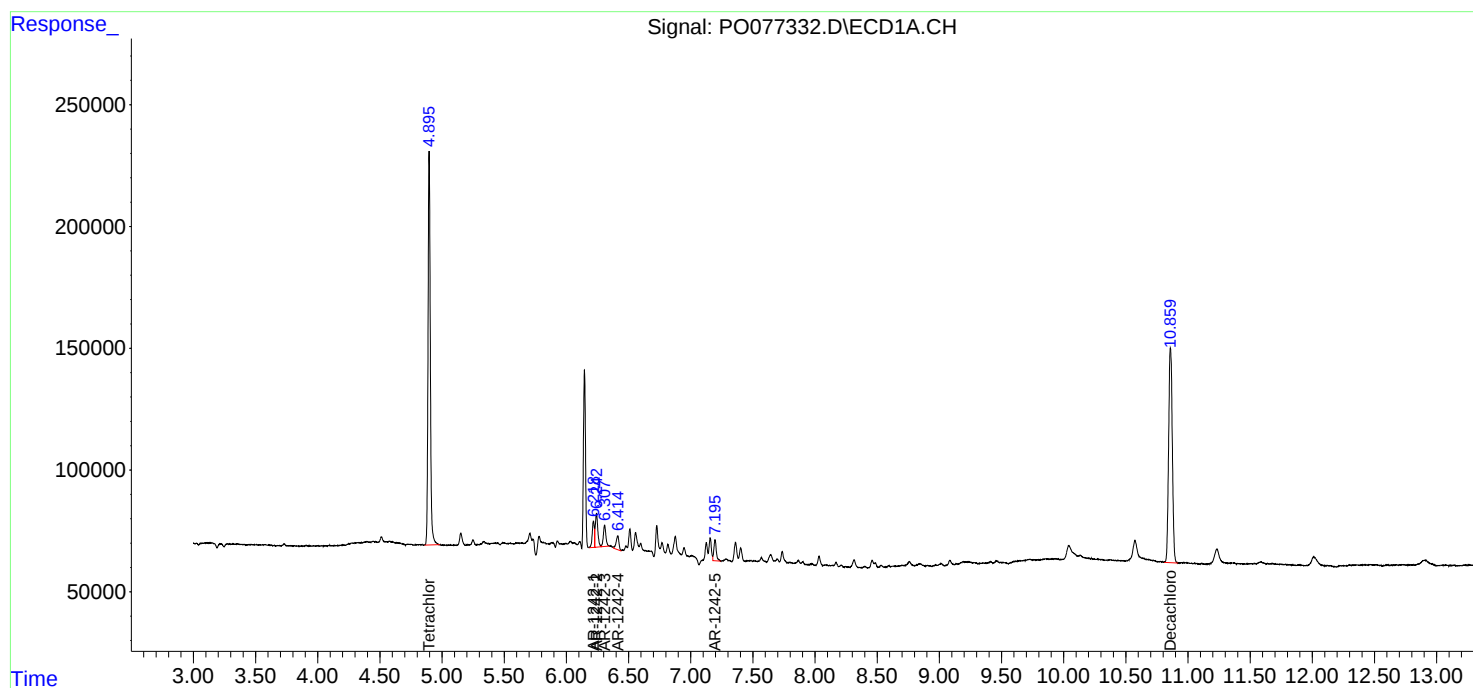

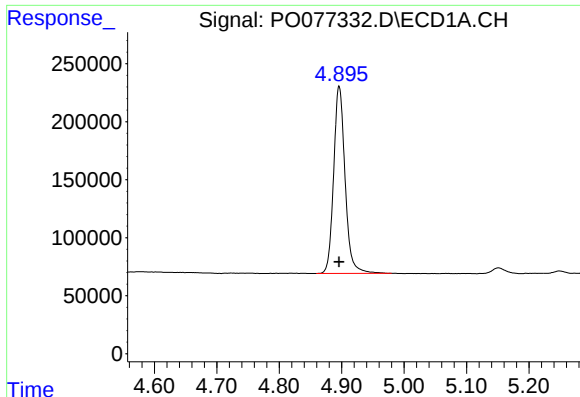


#1 Tetrachloro-m-xylene

R.T.: 4.896 min
Delta R.T.: 0.000 min
Response: 2051402
Conc: 19.41 ng/ml

Instrument :
ECD_O
ClientSampleId :
PLA-109


Manual Integrations
APPROVED

Ankita
4/27/2021 12:55:05 PM

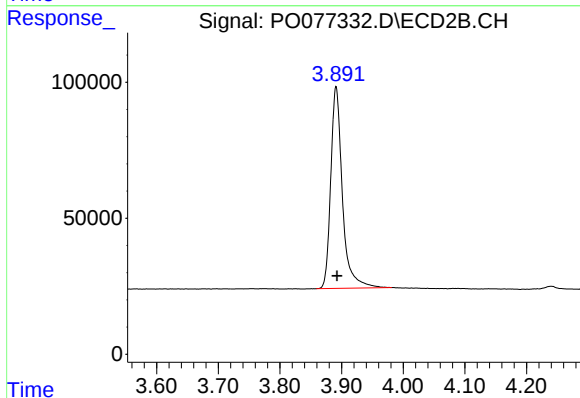


#1 Tetrachloro-m-xylene

R.T.: 3.891 min
Delta R.T.: -0.002 min
Response: 973304
Conc: 18.50 ng/ml

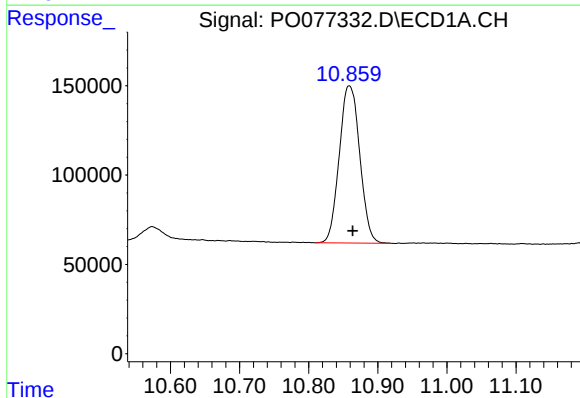


#2 Decachlorobiphenyl

R.T.: 10.859 min
Delta R.T.: -0.005 min
Response: 1812693
Conc: 17.46 ng/ml

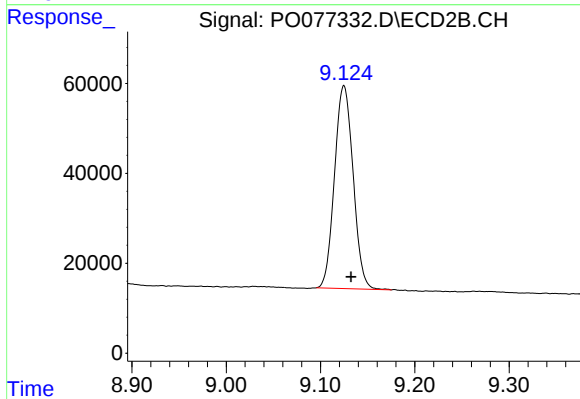

#2 Decachlorobiphenyl

R.T.: 9.125 min
Delta R.T.: -0.007 min
Response: 618981
Conc: 16.40 ng/ml

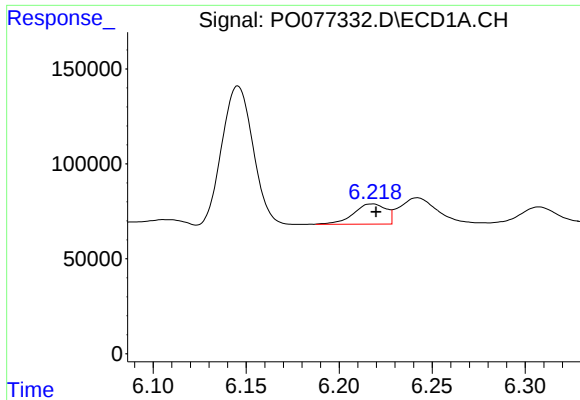


#16 AR-1242-1

R.T.: 6.218 min
Delta R.T.: -0.002 min
Response: 130626
Conc: 48.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
PLA-109


Manual Integrations
APPROVED

Ankita
4/27/2021 12:55:05 PM

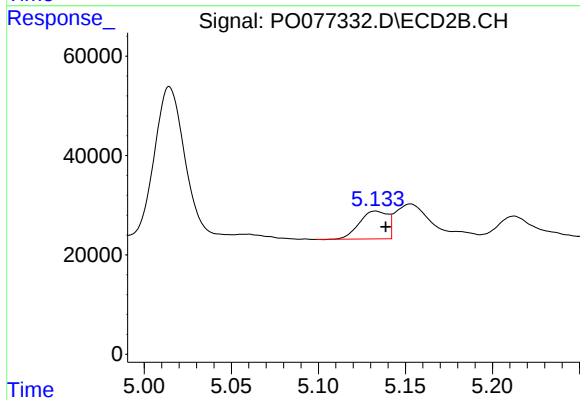


#16 AR-1242-1

R.T.: 5.133 min
Delta R.T.: -0.006 min
Response: 63920
Conc: 58.35 ng/ml

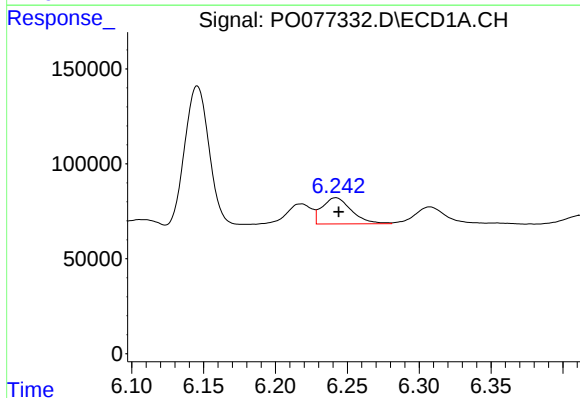


#17 AR-1242-2

R.T.: 6.242 min
Delta R.T.: -0.002 min
Response: 197212
Conc: 44.71 ng/ml

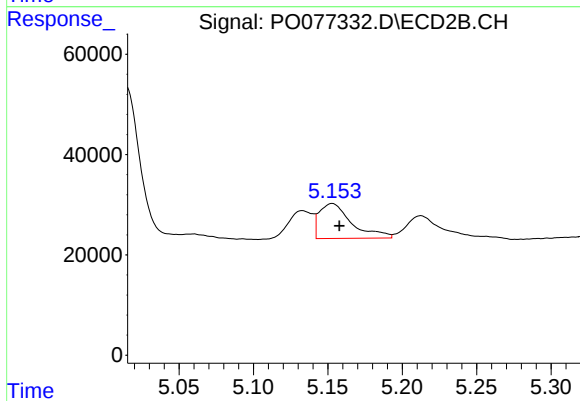

#17 AR-1242-2

R.T.: 5.153 min
Delta R.T.: -0.005 min
Response: 105054
Conc: 46.24 ng/ml

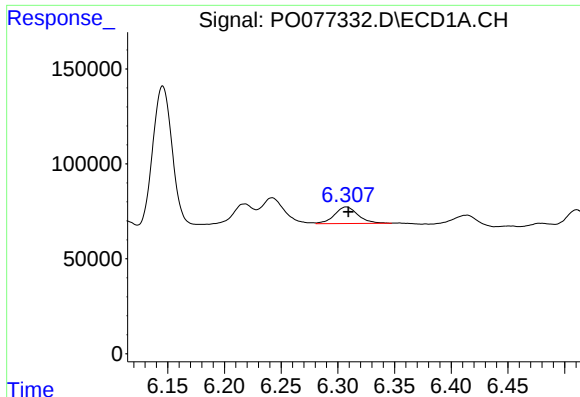


#18 AR-1242-3

R.T.: 6.307 min
Delta R.T.: -0.002 min
Response: 126001
Conc: 45.43 ng/ml

Instrument :
ECD_O
ClientSampleId :
PLA-109


Manual Integrations
APPROVED

Ankita
4/27/2021 12:55:05 PM

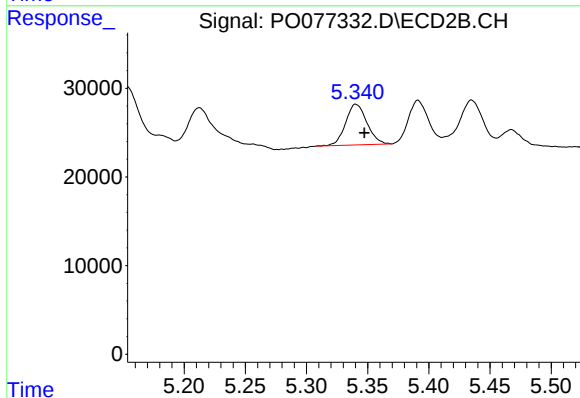


#18 AR-1242-3

R.T.: 5.340 min
Delta R.T.: -0.007 min
Response: 55629
Conc: 54.45 ng/ml

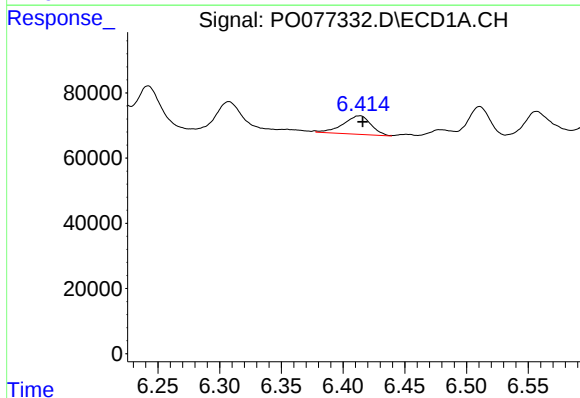


#19 AR-1242-4

R.T.: 6.414 min
Delta R.T.: -0.002 min
Response: 89550
Conc: 41.74 ng/ml m

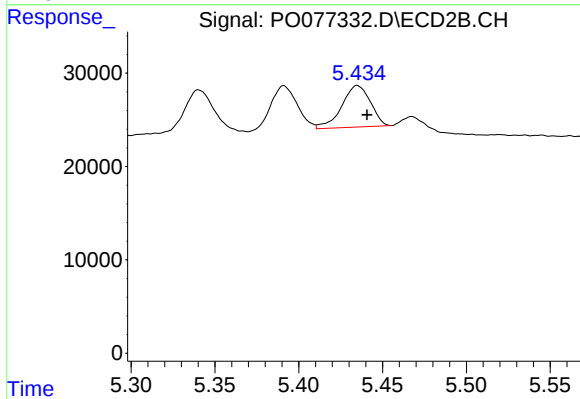

#19 AR-1242-4

R.T.: 5.435 min
Delta R.T.: -0.006 min
Response: 53075
Conc: 46.72 ng/ml

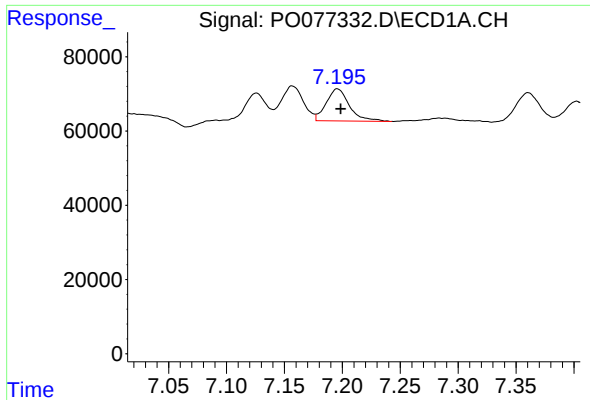


#20 AR-1242-5

R.T.: 7.196 min
Delta R.T.: -0.003 min
Response: 120194
Conc: 51.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
PLA-109

Manual Integrations
APPROVED

Ankita
4/27/2021 12:55:05 PM

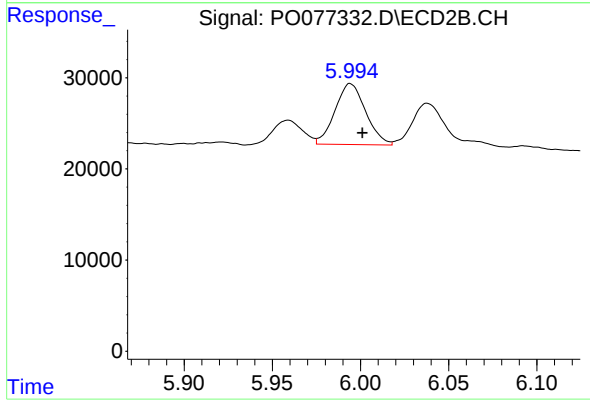

#20 AR-1242-5

R.T.: 5.994 min
Delta R.T.: -0.007 min
Response: 80949
Conc: 57.69 ng/ml