

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042623\
 Data File : P0094597.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Apr 2023 04:41
 Operator : YP/AJ
 Sample : 02485-02
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 33994

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/27/2023
 Supervised By :Ankita Jodhani 04/27/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 27 05:39:58 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042623.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Apr 27 03:04:50 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.416	3.619	40356488	23237043	11.716m	17.366 #
2) SA Decachlor...	10.253	8.632	30021566	14322378	12.371	12.724

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042623\
Data File : P0094597.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Apr 2023 04:41
Operator : YP/AJ
Sample : 02485-02
Misc :
ALS Vial : 44 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
33994


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/27/2023
Supervised By :Ankita Jodhani 04/27/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 27 05:39:58 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042623.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Apr 27 03:04:50 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

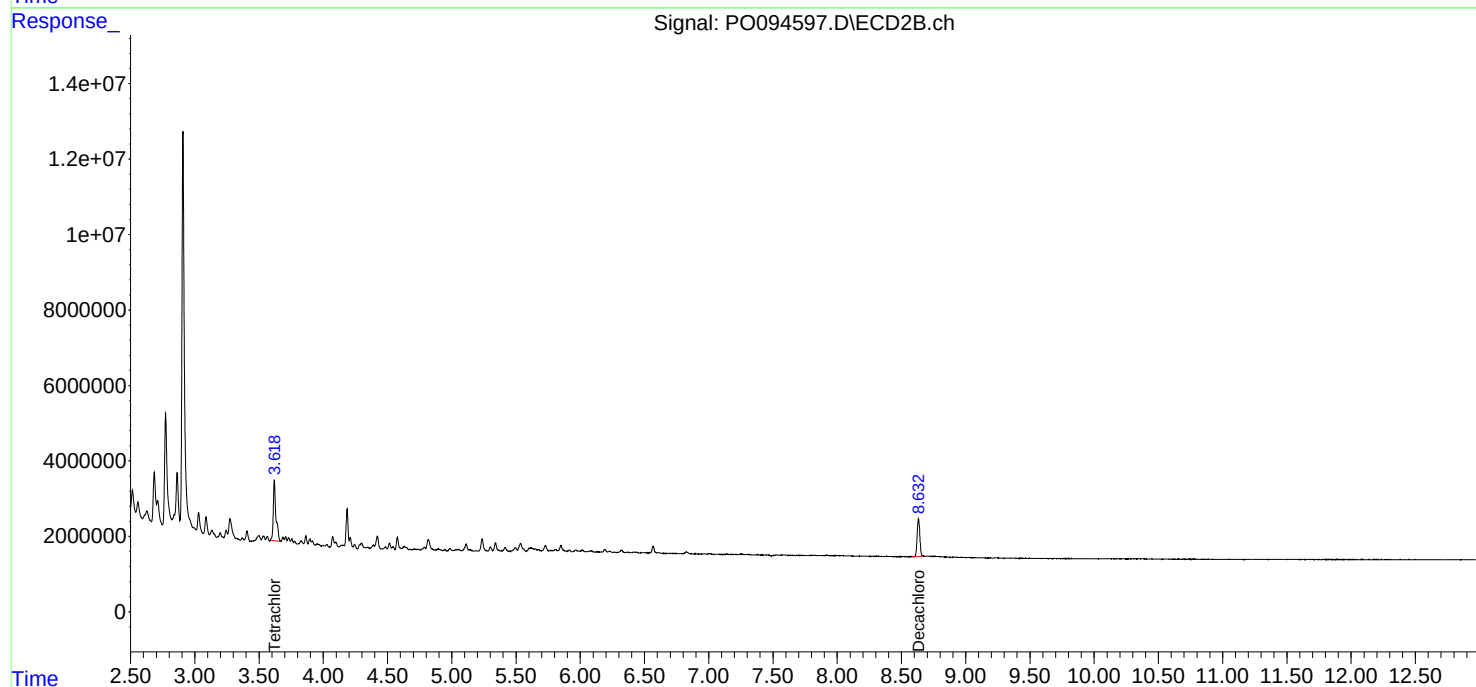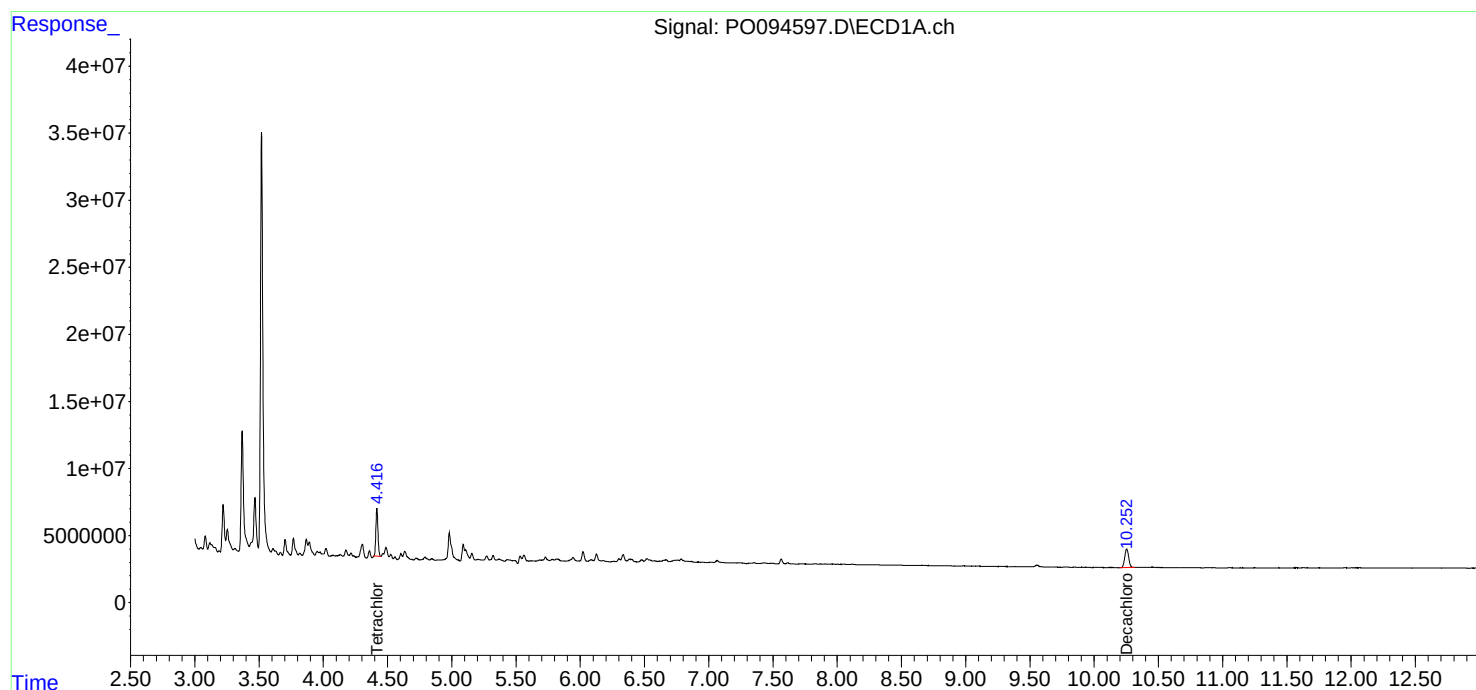

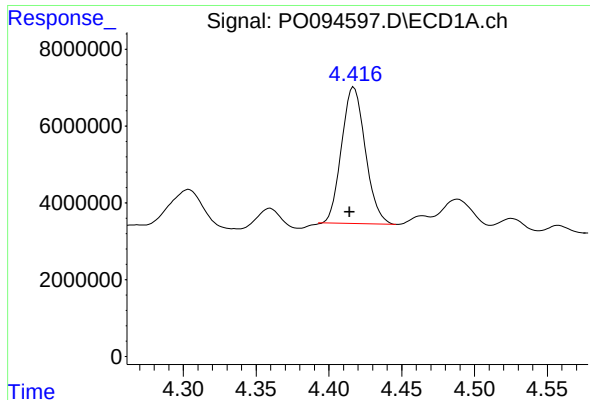


#1 Tetrachloro-m-xylene

R.T.: 4.416 min
Delta R.T.: 0.002 min
Response: 40356488
Conc: 11.72 ng/ml

Instrument :
ECD_O
ClientSampleId :
33994


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/27/2023
Supervised By :Ankita Jodhani 04/27/2023

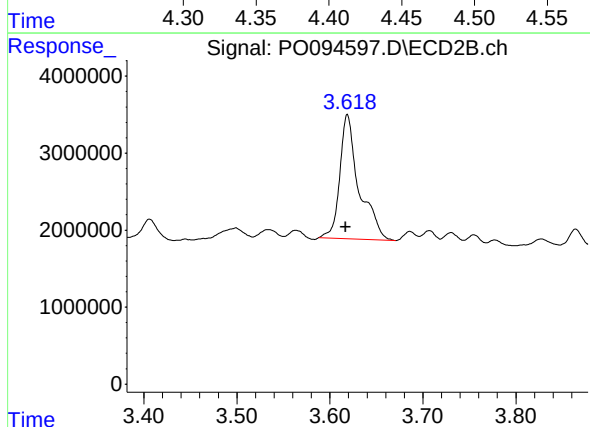


#1 Tetrachloro-m-xylene

R.T.: 3.619 min
Delta R.T.: 0.002 min
Response: 23237043
Conc: 17.37 ng/ml

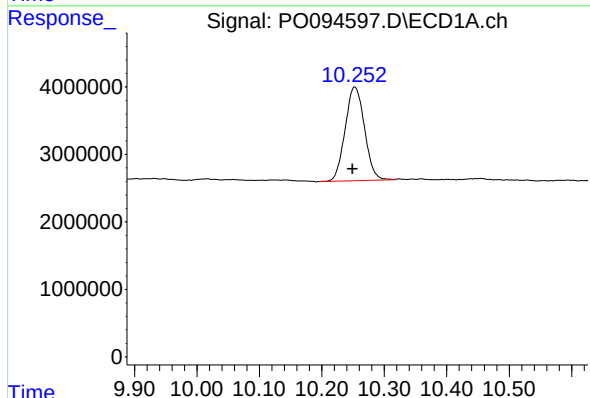

#2 Decachlorobiphenyl

R.T.: 10.253 min
Delta R.T.: 0.003 min
Response: 30021566
Conc: 12.37 ng/ml

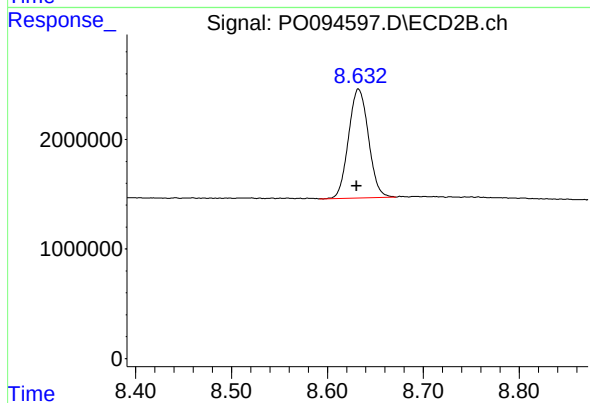

#2 Decachlorobiphenyl

R.T.: 8.632 min
Delta R.T.: 0.002 min
Response: 14322378
Conc: 12.72 ng/ml