

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042623\
 Data File : P0094598.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Apr 2023 07:13
 Operator : YP/AJ
 Sample : 02496-01
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TOTE-4-25-2023

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/27/2023
 Supervised By :Ankita Jodhani 04/27/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 27 07:43:28 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042623.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Apr 27 03:04:50 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.421	3.624	29912224	10541435	8.684m	7.878
2) SA Decachlor...	10.257	8.631	13066583	6490664	5.384	5.767

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO042623\
Data File : PO094598.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Apr 2023 07:13
Operator : YP/AJ
Sample : 02496-01
Misc :
ALS Vial : 46 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TOTE-4-25-2023


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/27/2023
Supervised By :Ankita Jodhani 04/27/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 27 07:43:28 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO042623.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Apr 27 03:04:50 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

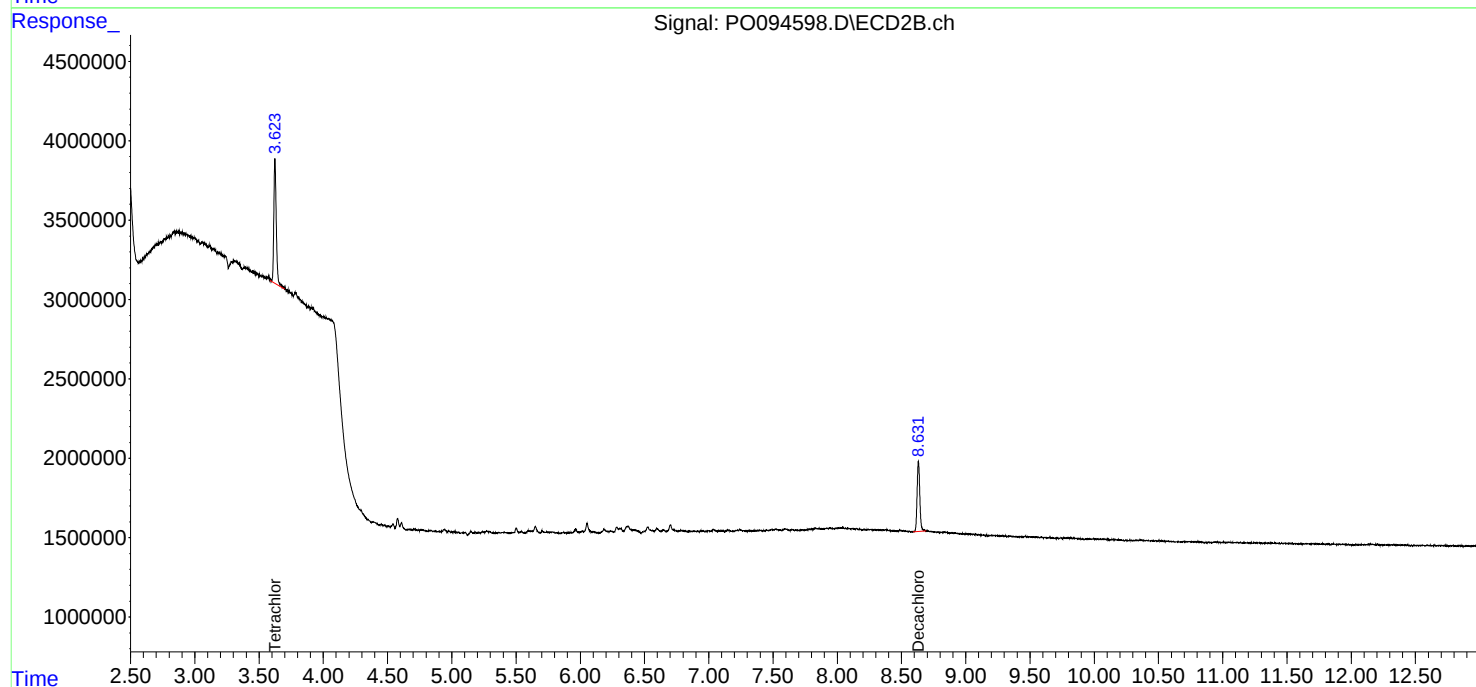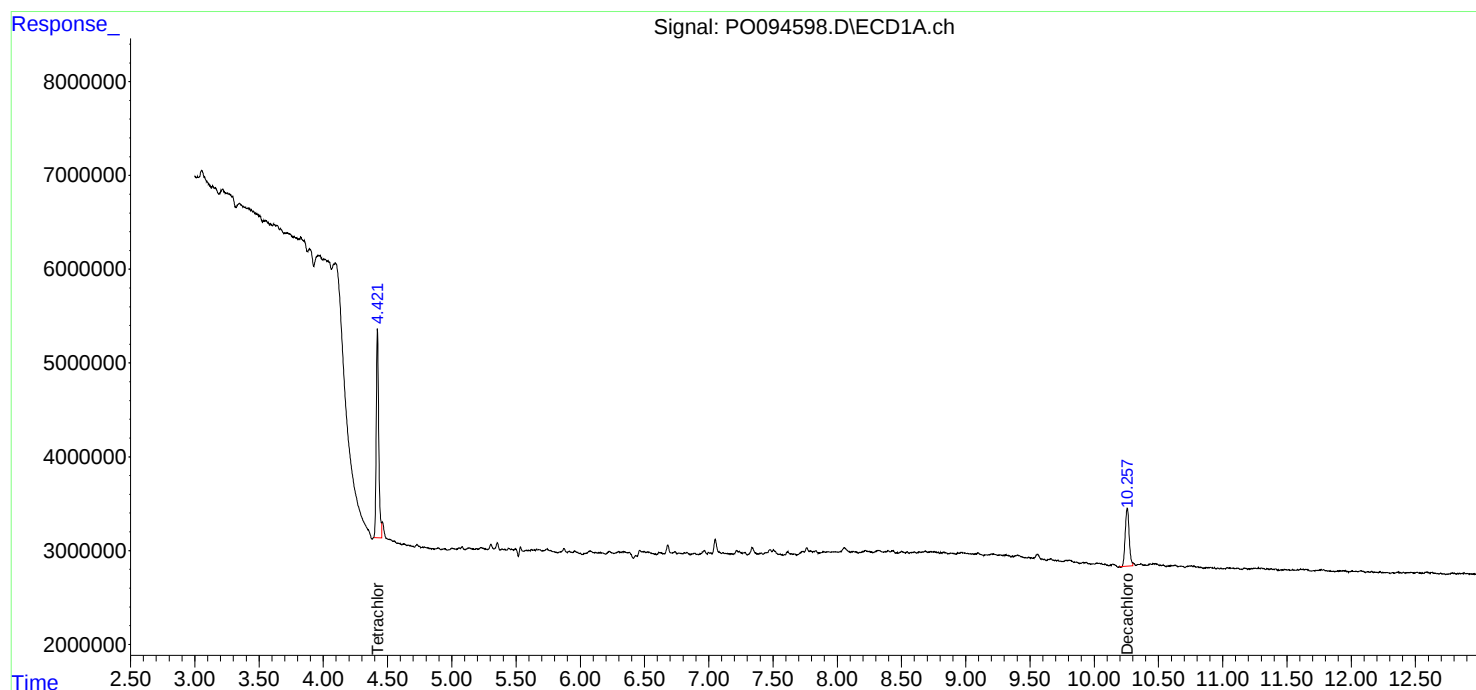

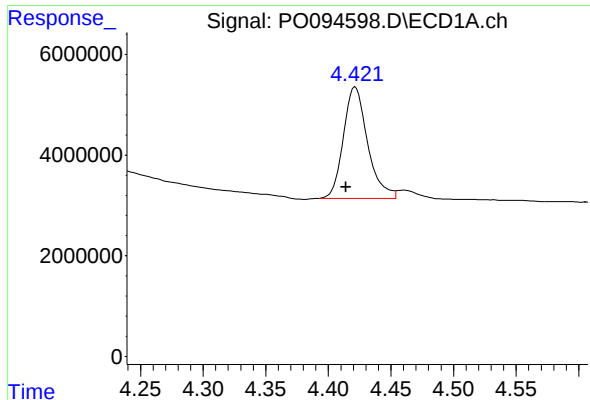


#1 Tetrachloro-m-xylene

R.T.: 4.421 min
Delta R.T.: 0.007 min
Response: 29912224
Conc: 8.68 ng/ml

Instrument :
ECD_O
ClientSampleId :
TOTE-4-25-2023


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/27/2023
Supervised By :Ankita Jodhani 04/27/2023

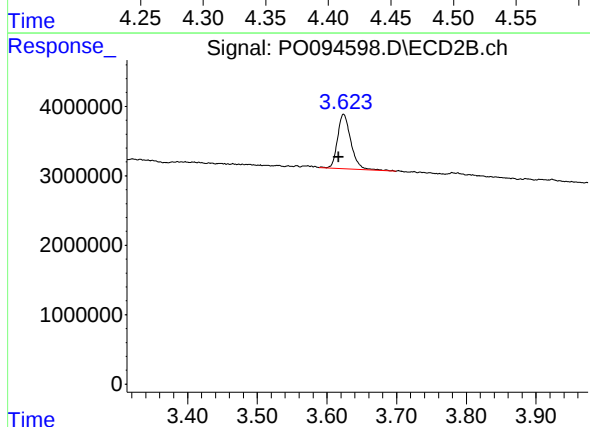


#1 Tetrachloro-m-xylene

R.T.: 3.624 min
Delta R.T.: 0.007 min
Response: 10541435
Conc: 7.88 ng/ml

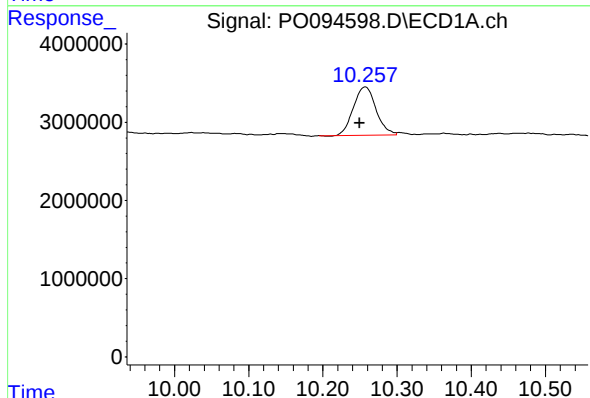

#2 Decachlorobiphenyl

R.T.: 10.257 min
Delta R.T.: 0.008 min
Response: 13066583
Conc: 5.38 ng/ml

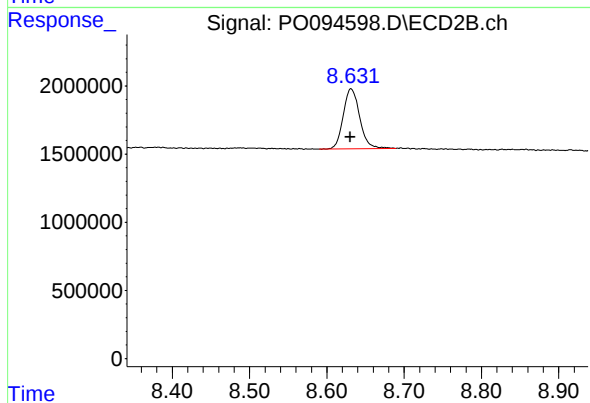

#2 Decachlorobiphenyl

R.T.: 8.631 min
Delta R.T.: 0.000 min
Response: 6490664
Conc: 5.77 ng/ml