

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042721\
 Data File : P0077344.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Apr 2021 12:21
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 27 16:28:43 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 21 09:50:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.895	3.890	2424350	1145926	22.940	21.781
2) SA Decachlor...	10.859	9.123	2338879	744968	22.528	19.743
Target Compounds						
24) L5 AR-1248-4	7.156	0.000	543592	0	134.505	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042721\
Data File : P0077344.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Apr 2021 12:21
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 27 16:28:43 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042121.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 21 09:50:22 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

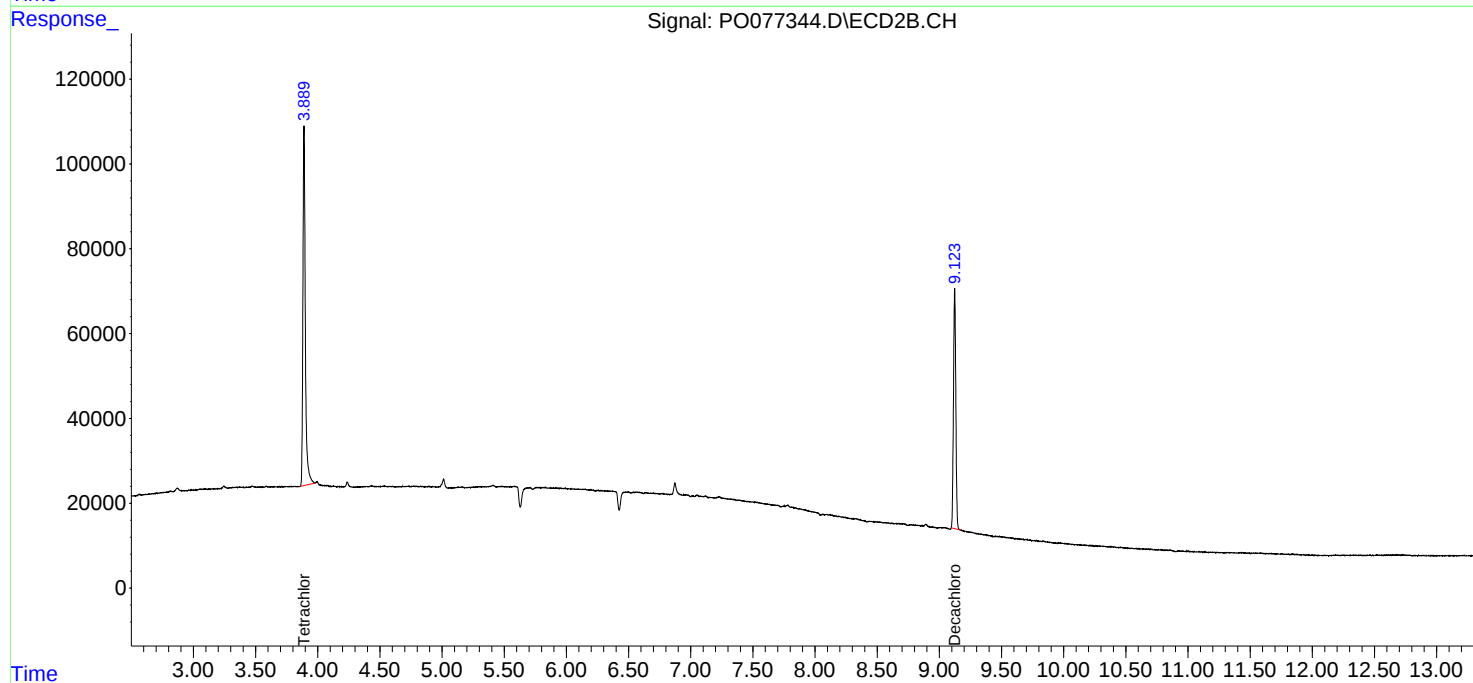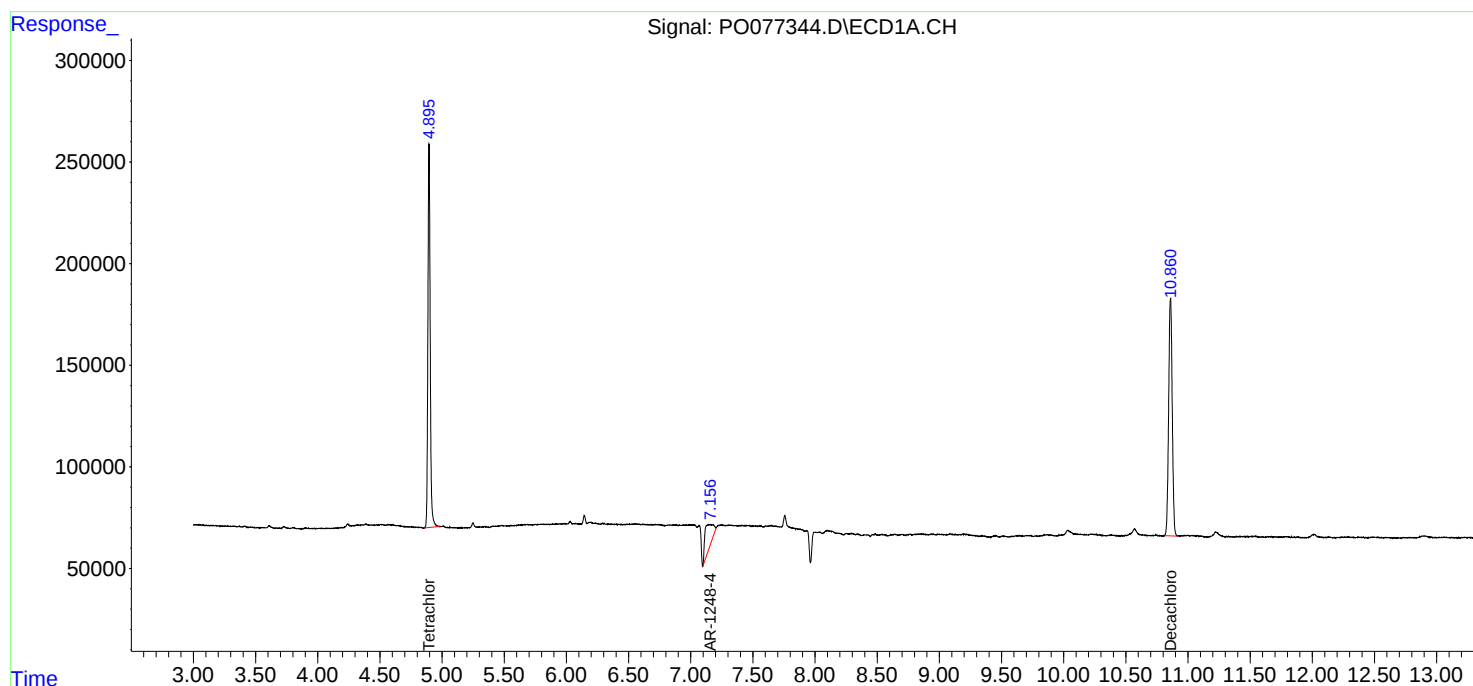


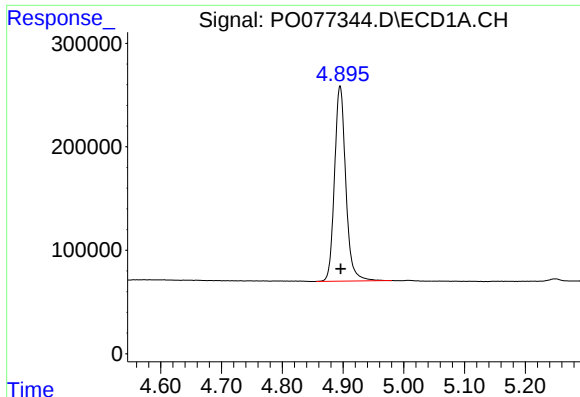

#1 Tetrachloro-m-xylene


R.T.: 4.895 min
Delta R.T.: 0.000 min
Response: 2424350
Conc: 22.94 ng/ml

Instrument :
ECD_O
ClientSampleId :

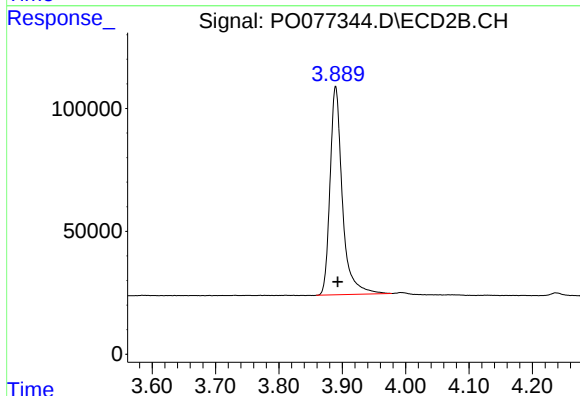


#1 Tetrachloro-m-xylene

R.T.: 3.890 min
Delta R.T.: -0.003 min
Response: 1145926
Conc: 21.78 ng/ml

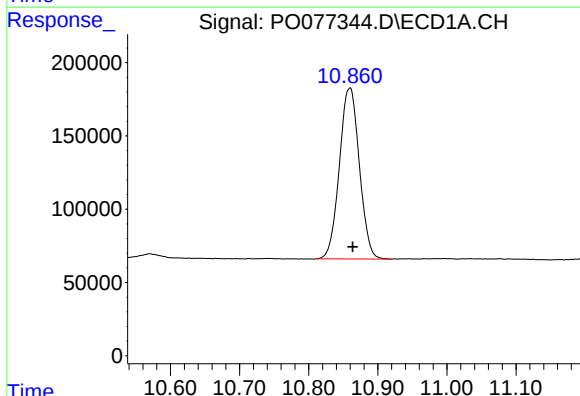


#2 Decachlorobiphenyl

R.T.: 10.859 min
Delta R.T.: -0.004 min
Response: 2338879
Conc: 22.53 ng/ml

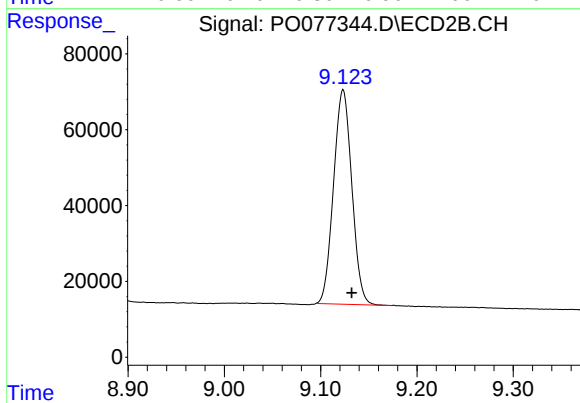

#2 Decachlorobiphenyl


R.T.: 9.123 min
Delta R.T.: -0.009 min
Response: 744968
Conc: 19.74 ng/ml

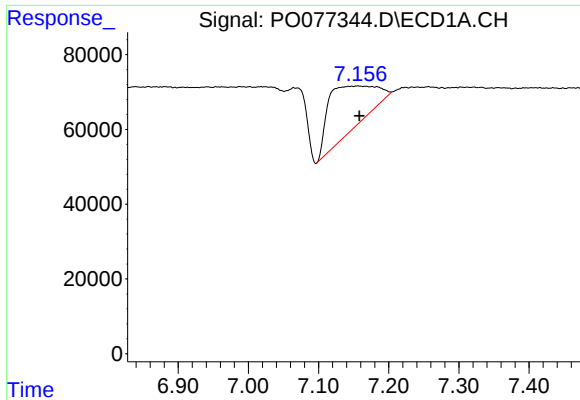

#24 AR-1248-4

R.T.: 7.156 min
Delta R.T.: -0.002 min
Response: 543592
Conc: 134.51 ng/ml

Instrument :
ECD_O
ClientSampleId :

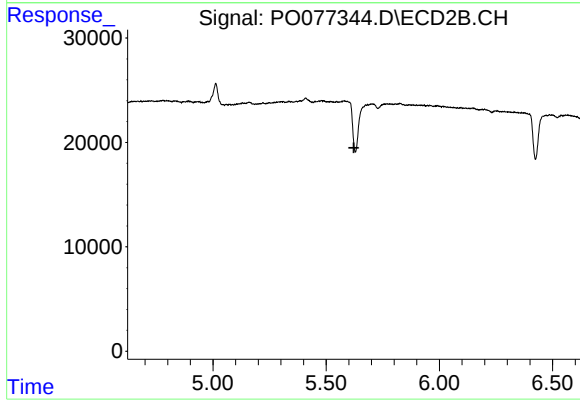

#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.622 min
Response: 0
Conc: N.D.