

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0042721\
 Data File : P0077345.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Apr 2021 12:38
 Operator : DD\AJ
 Sample : M2170-11
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 CS-1

Manual Integrations
 APPROVED

Ankita
 4/28/2021 3:40:22 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 27 16:28:56 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0042121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 21 09:50:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.894	3.889	2284784	1046269	21.619	19.887
2) SA Decachlor...	10.856	9.123	1716082	557148	16.529	14.765m
Target Compounds						
26) L6 AR-1254-1	7.125	5.990	129974	104822	31.607m	36.313m
27) L6 AR-1254-2	7.356	6.149	207548	40031	32.067	15.505m#
28) L6 AR-1254-3	7.736	6.566	274364	204766	40.545m	52.337 #
29) L6 AR-1254-4	8.030	6.805	80309	33303	16.330m	14.658m
30) L6 AR-1254-5	8.458	7.229	255726	489835	45.937	135.098 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042721\
Data File : P0077345.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Apr 2021 12:38
Operator : DD\AJ
Sample : M2170-11
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
CS-1


Manual Integrations
APPROVED

Ankita
4/28/2021 3:40:22 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 27 16:28:56 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042121.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 21 09:50:22 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

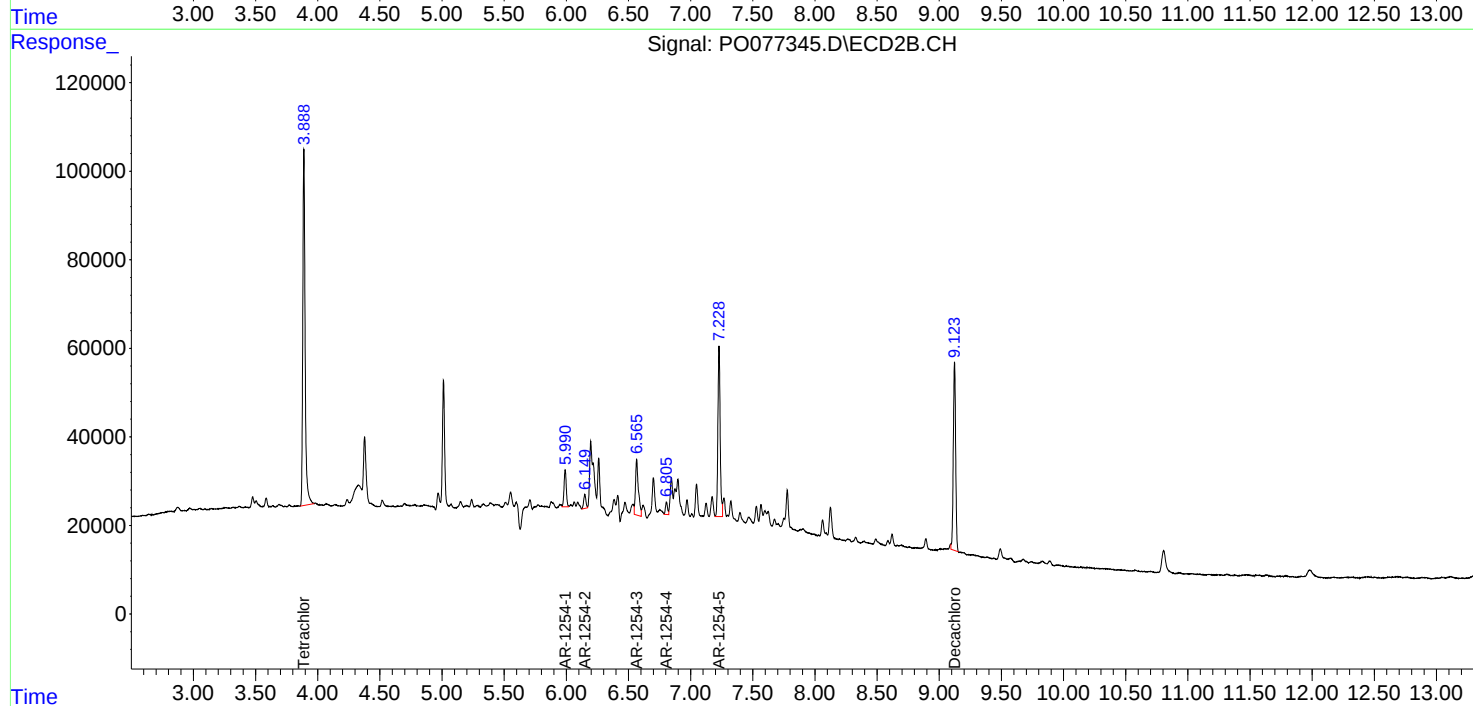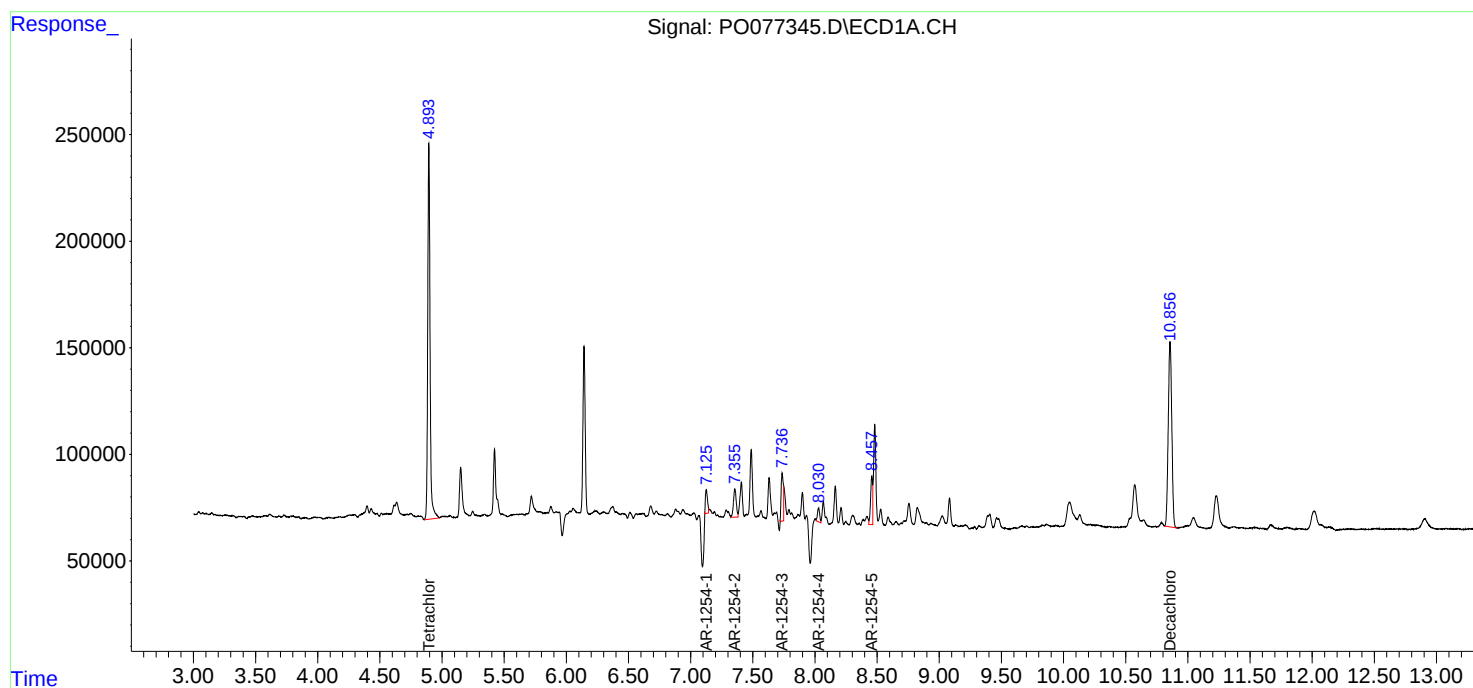

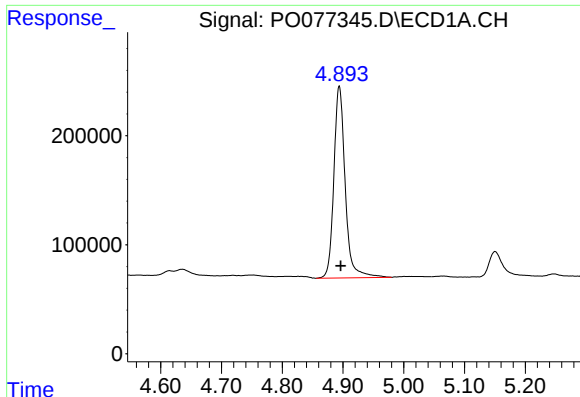


#1 Tetrachloro-m-xylene

R.T.: 4.894 min
Delta R.T.: -0.002 min
Response: 2284784
Conc: 21.62 ng/ml

Instrument :
ECD_O
ClientSampleId :
CS-1


Manual Integrations
APPROVED

Ankita
4/28/2021 3:40:22 PM

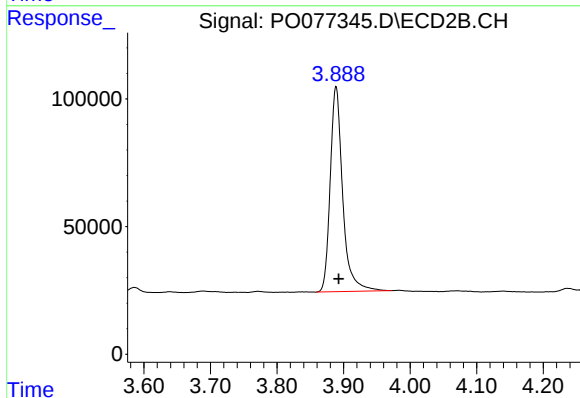


#1 Tetrachloro-m-xylene

R.T.: 3.889 min
Delta R.T.: -0.004 min
Response: 1046269
Conc: 19.89 ng/ml

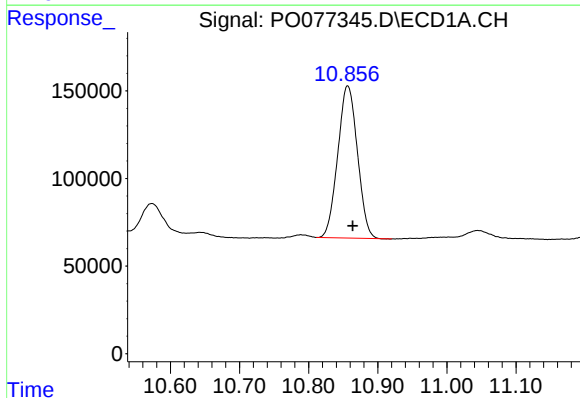


#2 Decachlorobiphenyl

R.T.: 10.856 min
Delta R.T.: -0.007 min
Response: 1716082
Conc: 16.53 ng/ml

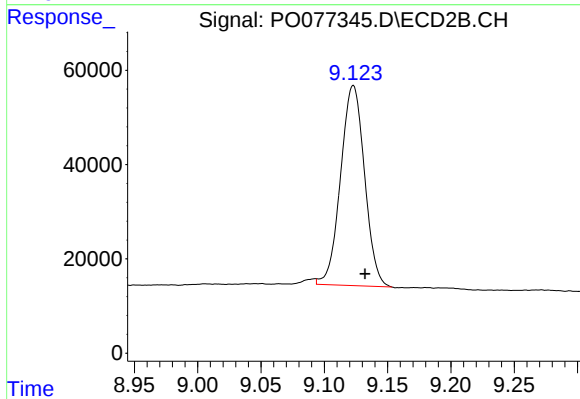

#2 Decachlorobiphenyl

R.T.: 9.123 min
Delta R.T.: -0.010 min
Response: 557148
Conc: 14.77 ng/ml m

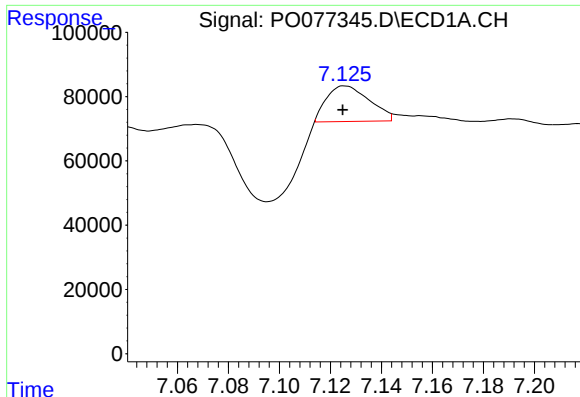


#26 AR-1254-1

R.T.: 7.125 min
Delta R.T.: 0.000 min
Response: 129974
Conc: 31.61 ng/ml m

Instrument :
ECD_O
ClientSampleId :
CS-1


Manual Integrations
APPROVED

Ankita
4/28/2021 3:40:22 PM

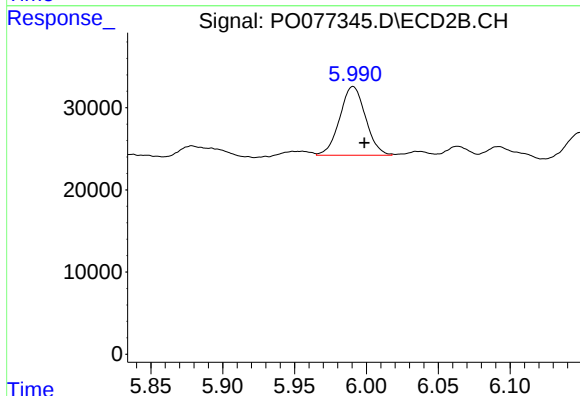


#26 AR-1254-1

R.T.: 5.990 min
Delta R.T.: -0.008 min
Response: 104822
Conc: 36.31 ng/ml m

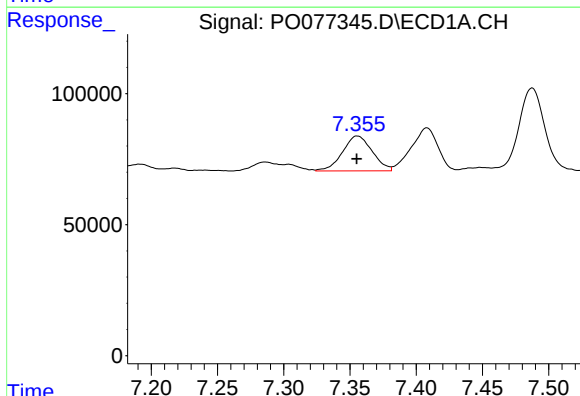


#27 AR-1254-2

R.T.: 7.356 min
Delta R.T.: 0.000 min
Response: 207548
Conc: 32.07 ng/ml

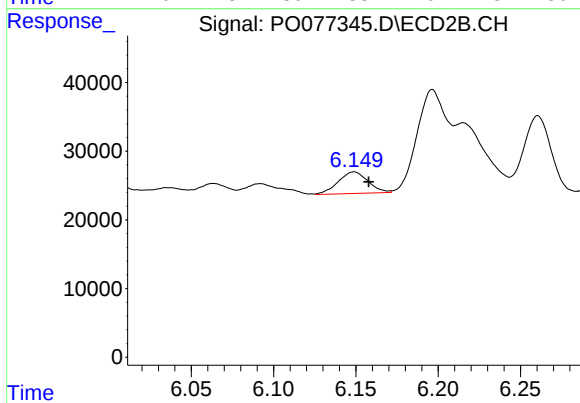

#27 AR-1254-2

R.T.: 6.149 min
Delta R.T.: -0.009 min
Response: 40031
Conc: 15.51 ng/ml m

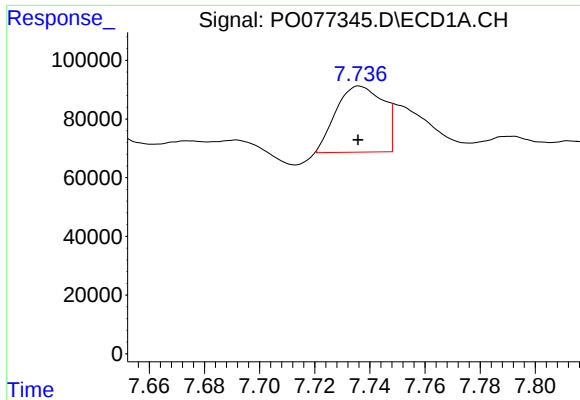


#28 AR-1254-3

R.T.: 7.736 min
Delta R.T.: 0.000 min
Response: 274364
Conc: 40.55 ng/ml m

Instrument :
ECD_O
ClientSampleId :
CS-1


Manual Integrations
APPROVED

Ankita
4/28/2021 3:40:22 PM

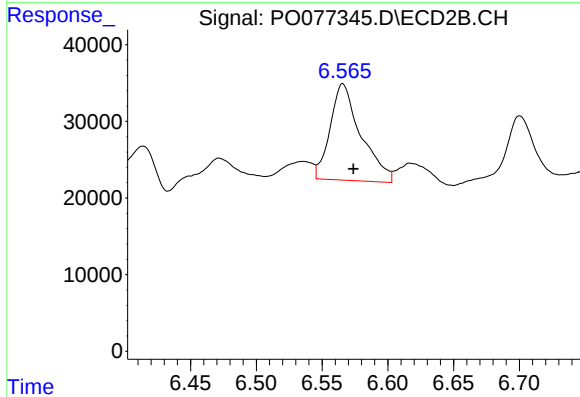


#28 AR-1254-3

R.T.: 6.566 min
Delta R.T.: -0.008 min
Response: 204766
Conc: 52.34 ng/ml

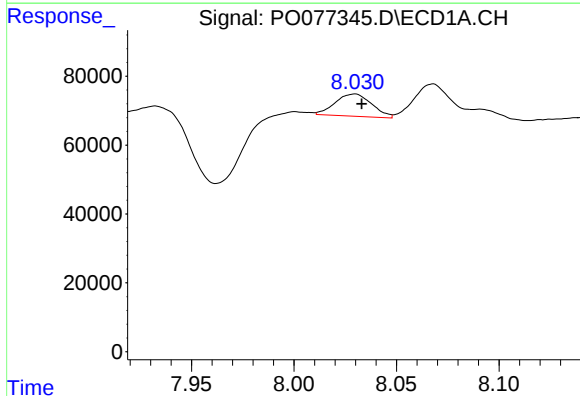


#29 AR-1254-4

R.T.: 8.030 min
Delta R.T.: -0.003 min
Response: 80309
Conc: 16.33 ng/ml m

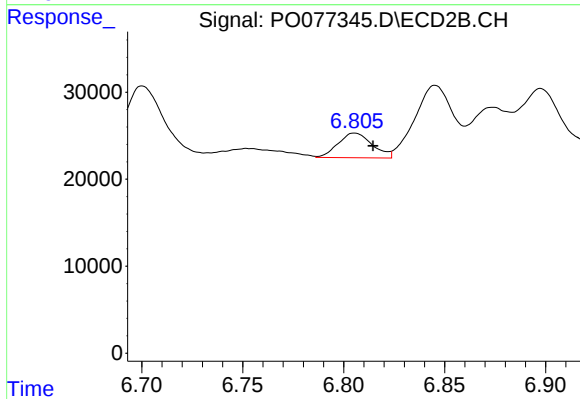

#29 AR-1254-4

R.T.: 6.805 min
Delta R.T.: -0.009 min
Response: 33303
Conc: 14.66 ng/ml m

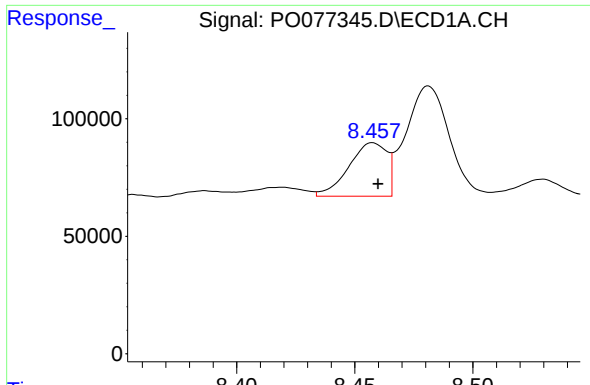


#30 AR-1254-5

R.T.: 8.458 min
Delta R.T.: -0.002 min
Response: 255726
Conc: 45.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
CS-1

Manual Integrations
APPROVED

Ankita
4/28/2021 3:40:22 PM

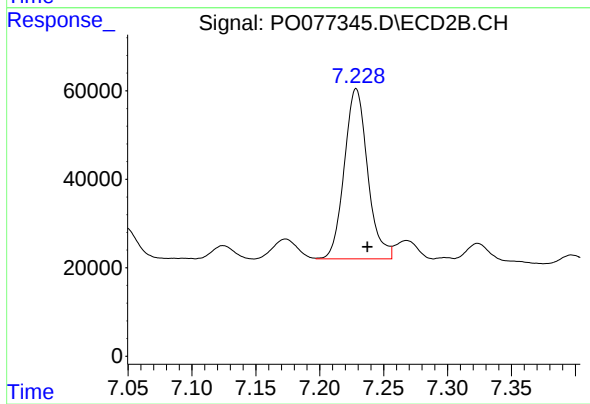

#30 AR-1254-5

R.T.: 7.229 min
Delta R.T.: -0.009 min
Response: 489835
Conc: 135.10 ng/ml