

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042721\
 Data File : P0077346.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Apr 2021 12:55
 Operator : DD\AJ
 Sample : M2170-09DL 2X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 DN-1DL

Manual Integrations
 APPROVED

Ankita
 4/28/2021 3:40:24 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 27 16:29:18 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 21 09:50:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.894	3.889	946735	471874	8.958m	8.969
2) SA Decachlor...	10.857	9.123	821536	267316	7.913	7.084
Target Compounds						
26) L6 AR-1254-1	7.122	5.991	1910593	1307126	464.619m	452.827
27) L6 AR-1254-2	7.351	6.150	3367415	1234226	520.286m	478.054
28) L6 AR-1254-3	7.734	6.566	3420366	1998435	505.457m	510.790
29) L6 AR-1254-4	8.029	6.806	2869596	1255735	583.514m	552.690
30) L6 AR-1254-5	8.458	7.230	3451470	3028338	619.994	835.224 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO042721\
Data File : PO077346.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Apr 2021 12:55
Operator : DD\AJ
Sample : M2170-09DL 2X
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
DN-1DL


Manual Integrations
APPROVED

Ankita
4/28/2021 3:40:24 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 27 16:29:18 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO042121.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 21 09:50:22 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

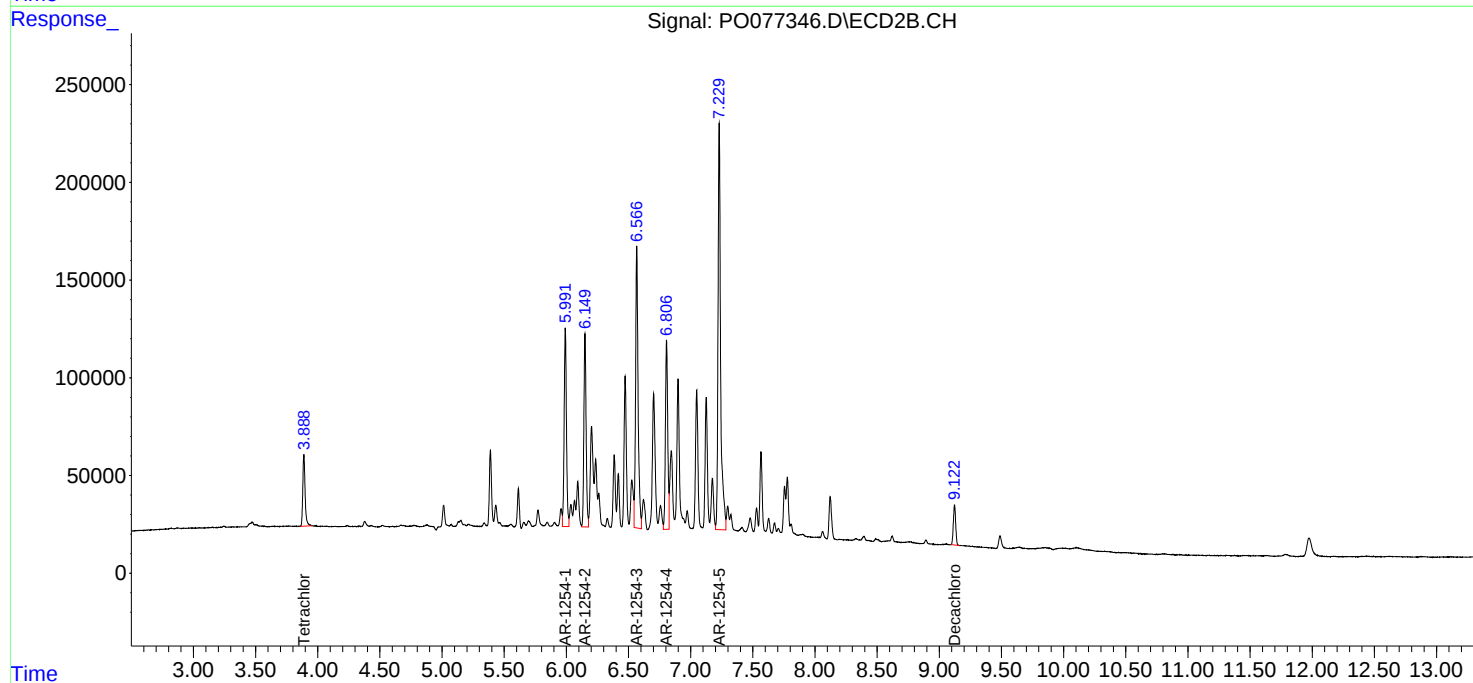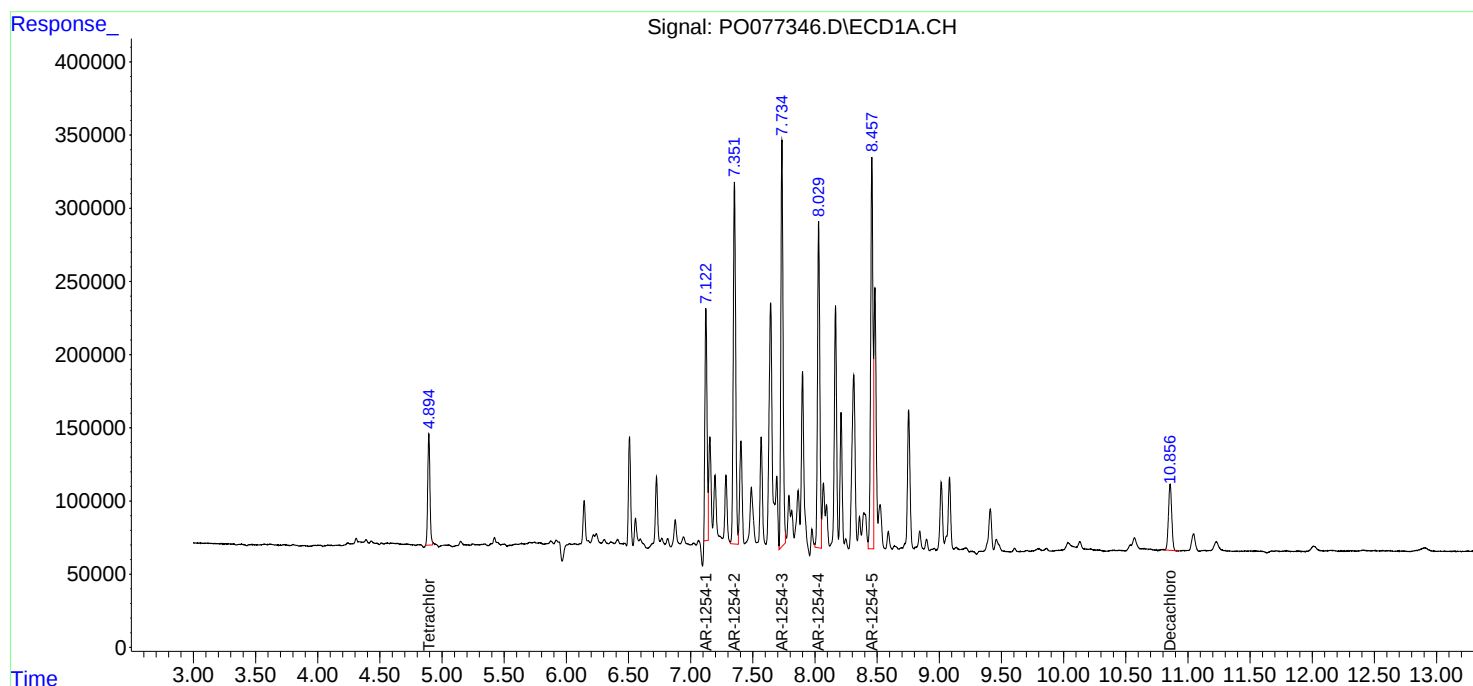

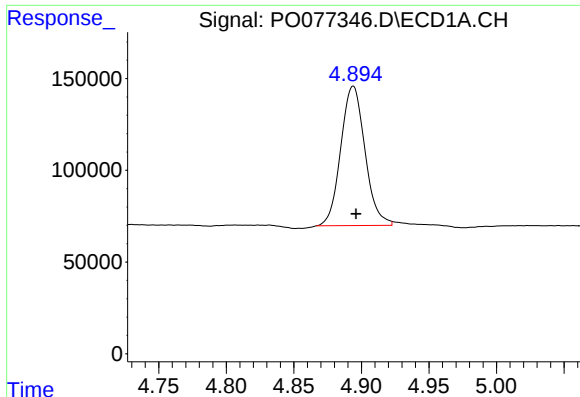


#1 Tetrachloro-m-xylene

R.T.: 4.894 min
Delta R.T.: -0.002 min
Response: 946735
Conc: 8.96 ng/ml m

Instrument :
ECD_O
ClientSampleId :
DN-1DL


Manual Integrations
APPROVED

Ankita
4/28/2021 3:40:24 PM

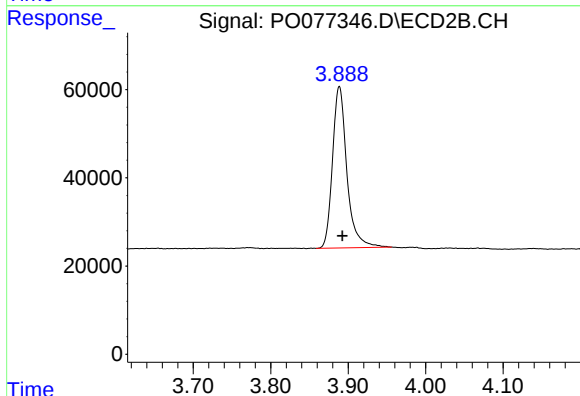


#1 Tetrachloro-m-xylene

R.T.: 3.889 min
Delta R.T.: -0.004 min
Response: 471874
Conc: 8.97 ng/ml

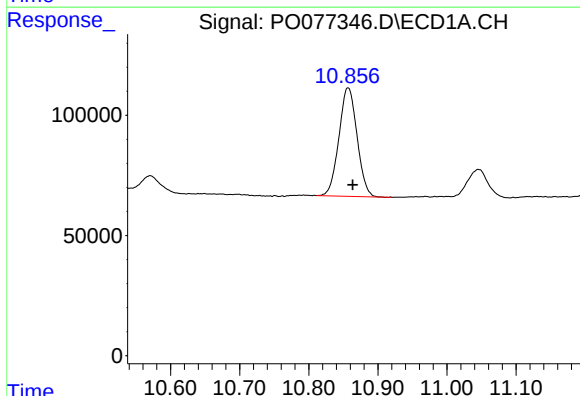


#2 Decachlorobiphenyl

R.T.: 10.857 min
Delta R.T.: -0.007 min
Response: 821536
Conc: 7.91 ng/ml

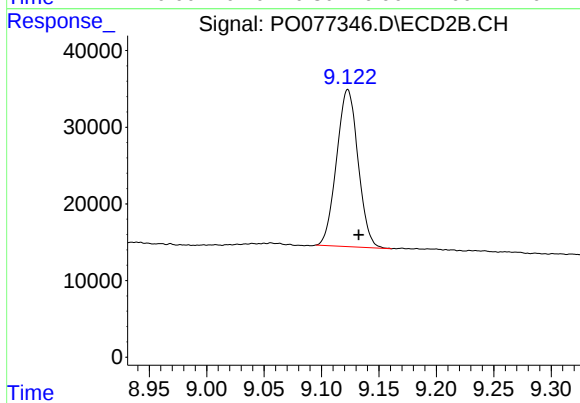

#2 Decachlorobiphenyl

R.T.: 9.123 min
Delta R.T.: -0.009 min
Response: 267316
Conc: 7.08 ng/ml

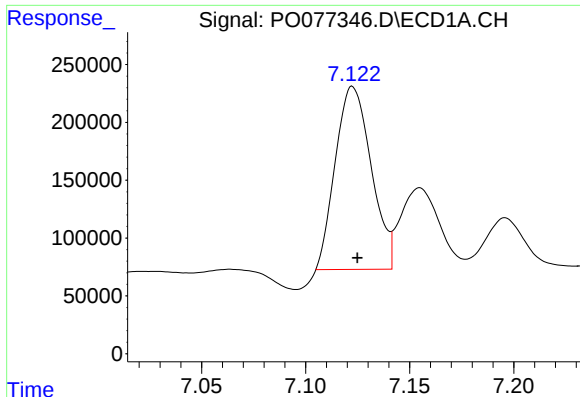


#26 AR-1254-1

R.T.: 7.122 min
Delta R.T.: -0.003 min
Response: 1910593
Conc: 464.62 ng/ml m

Instrument :
ECD_O
ClientSampleId :
DN-1DL


Manual Integrations
APPROVED

Ankita
4/28/2021 3:40:24 PM

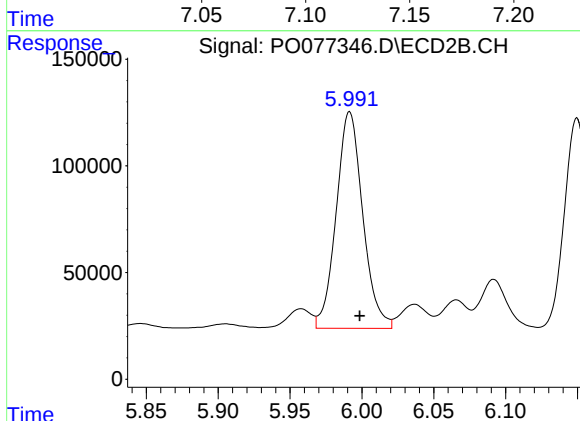


#26 AR-1254-1

R.T.: 5.991 min
Delta R.T.: -0.007 min
Response: 1307126
Conc: 452.83 ng/ml

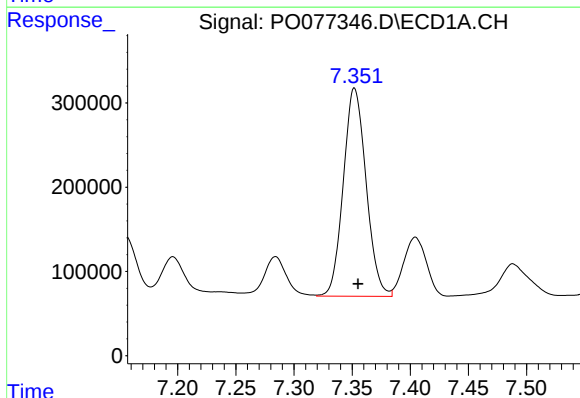


#27 AR-1254-2

R.T.: 7.351 min
Delta R.T.: -0.004 min
Response: 3367415
Conc: 520.29 ng/ml m

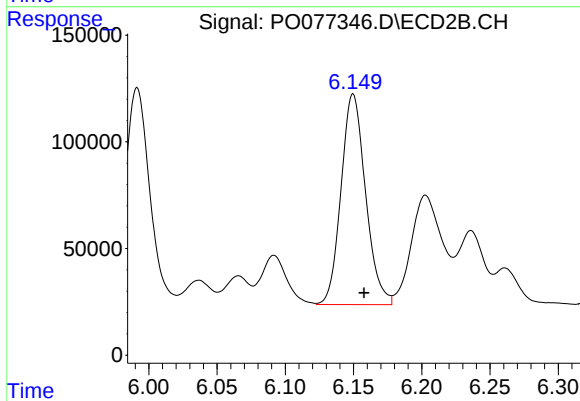

#27 AR-1254-2

R.T.: 6.150 min
Delta R.T.: -0.008 min
Response: 1234226
Conc: 478.05 ng/ml

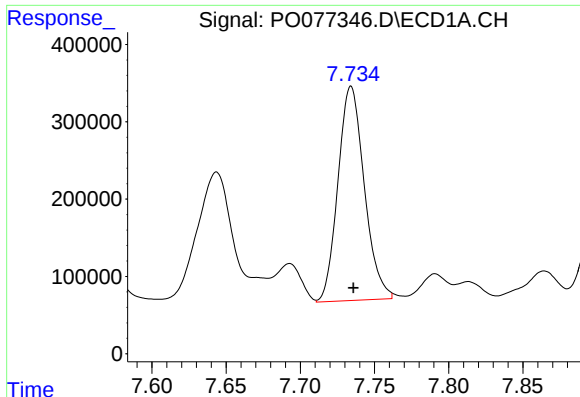


#28 AR-1254-3

R.T.: 7.734 min
Delta R.T.: -0.002 min
Response: 3420366
Conc: 505.46 ng/ml m

Instrument :
ECD_O
ClientSampleId :
DN-1DL


Manual Integrations
APPROVED

Ankita
4/28/2021 3:40:24 PM

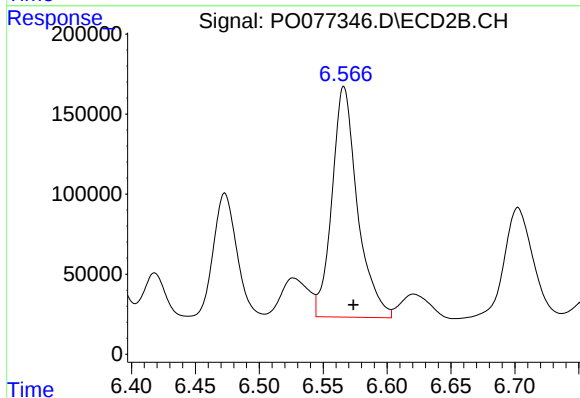


#28 AR-1254-3

R.T.: 6.566 min
Delta R.T.: -0.008 min
Response: 1998435
Conc: 510.79 ng/ml

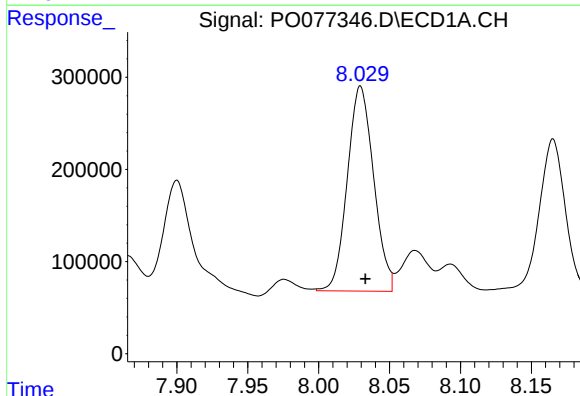


#29 AR-1254-4

R.T.: 8.029 min
Delta R.T.: -0.004 min
Response: 2869596
Conc: 583.51 ng/ml m

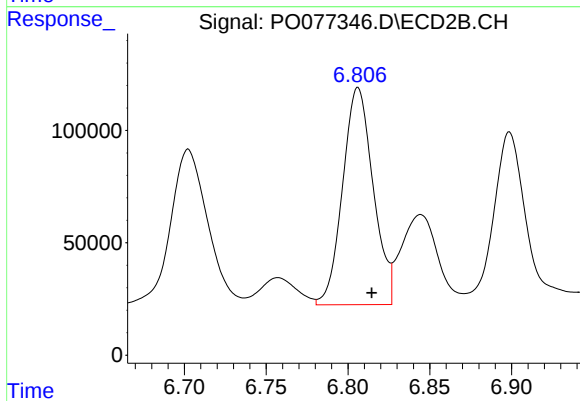

#29 AR-1254-4

R.T.: 6.806 min
Delta R.T.: -0.008 min
Response: 1255735
Conc: 552.69 ng/ml

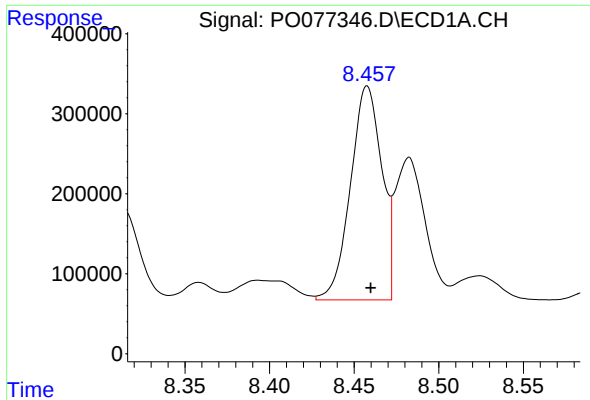


#30 AR-1254-5

R.T.: 8.458 min
Delta R.T.: -0.002 min
Response: 3451470
Conc: 619.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
DN-1DL

Manual Integrations
APPROVED

Ankita
4/28/2021 3:40:24 PM

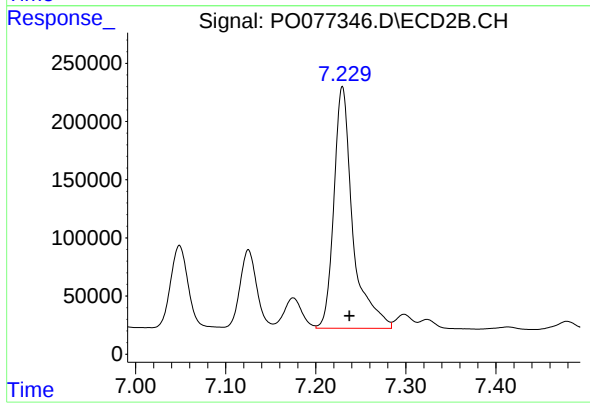

#30 AR-1254-5

R.T.: 7.230 min
Delta R.T.: -0.008 min
Response: 3028338
Conc: 835.22 ng/ml