

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042723\
 Data File : P0094608.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Apr 2023 11:25
 Operator : YP/AJ
 Sample : 02496-01 (Sig #1); 02496-01RE (Sig #2)
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TOTE-4-25-2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 27 15:25:17 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042623.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Apr 27 03:04:50 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.416	3.619	60400650	21983464	17.535	16.429
2) SA Decachlor...	10.250	8.630	35091068	16639680	14.460	14.783

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO042723\
Data File : PO094608.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Apr 2023 11:25
Operator : YP/AJ
Sample : 02496-01 (Sig #1); 02496-01RE (Sig #2)
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TOTE-4-25-2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 27 15:25:17 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO042623.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Apr 27 03:04:50 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

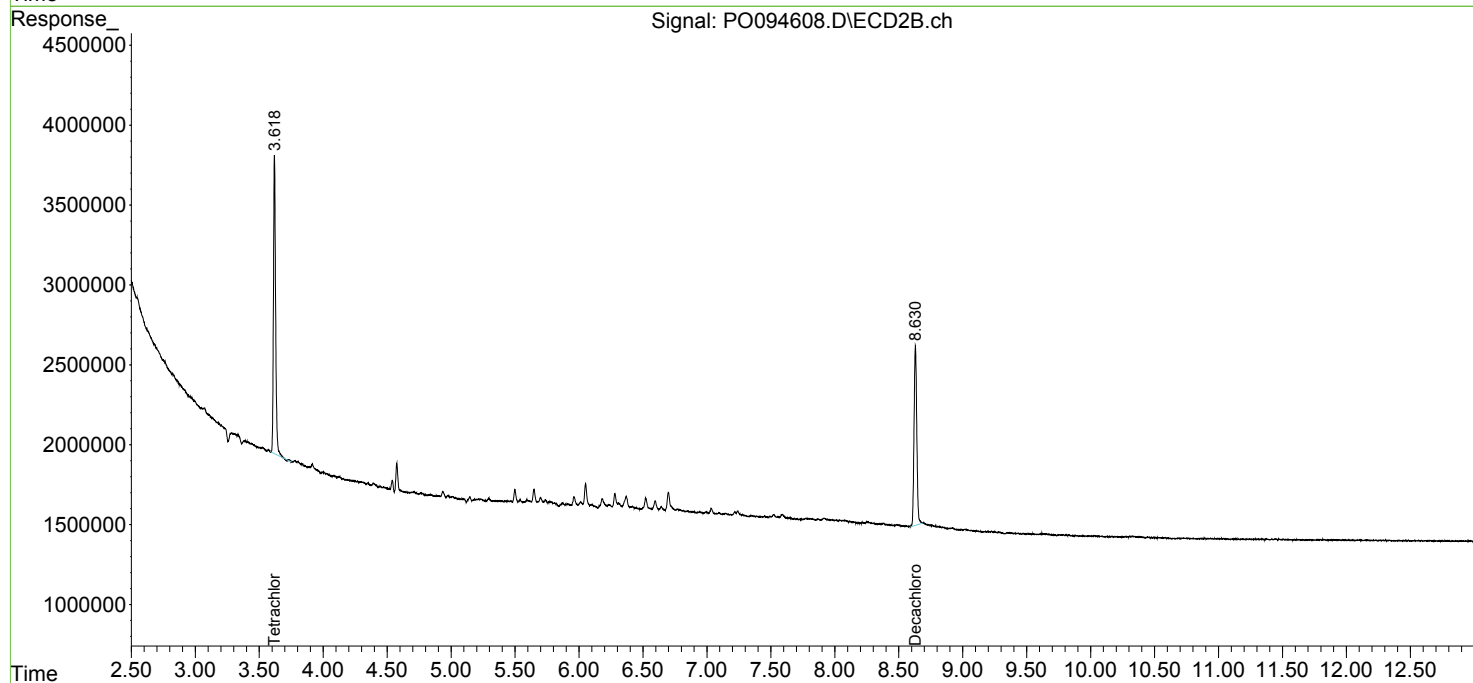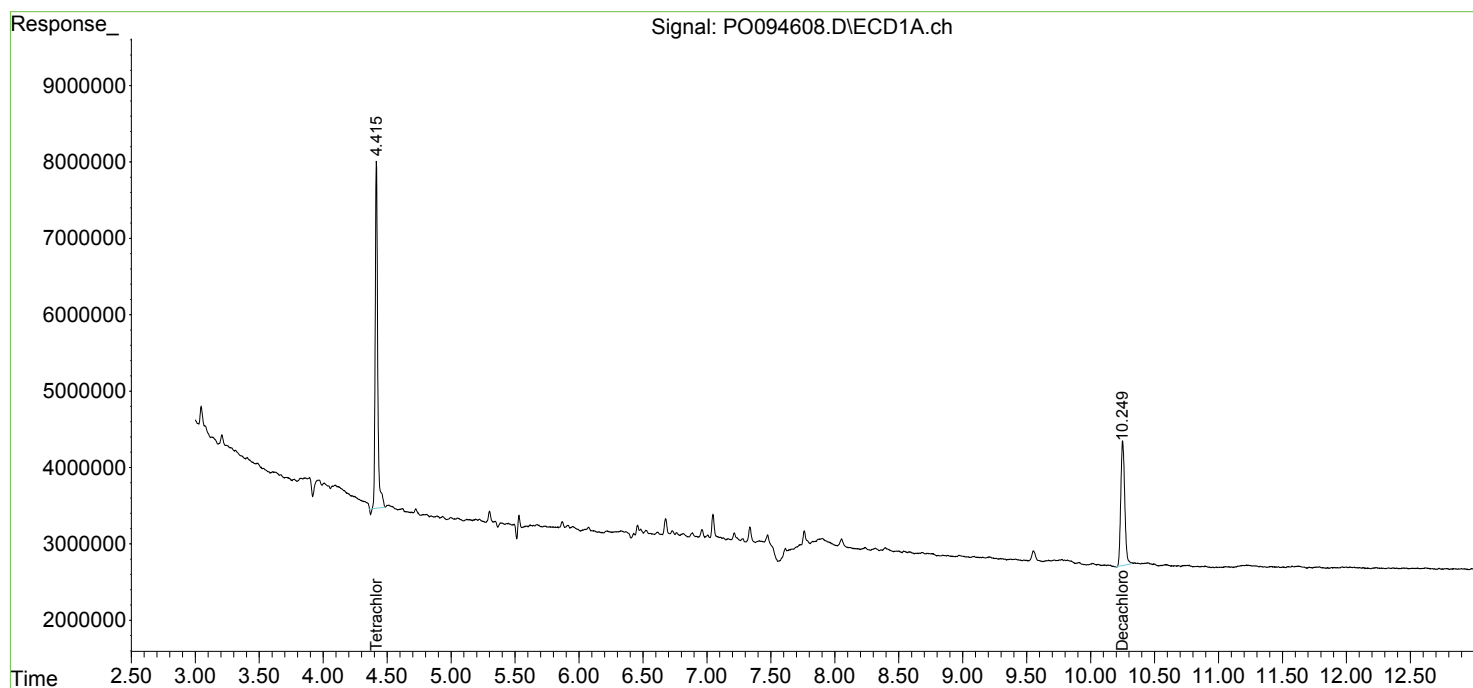


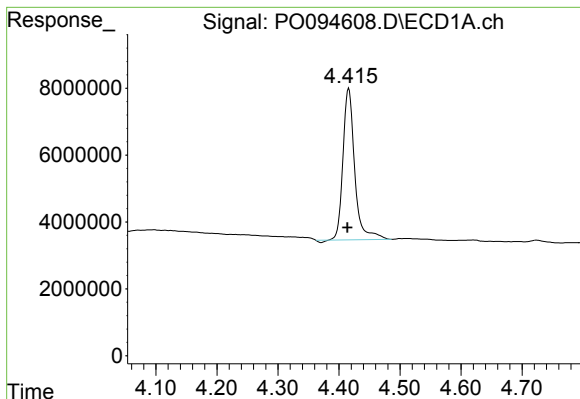

#1 Tetrachloro-m-xylene


R.T.: 4.416 min
Delta R.T.: 0.002 min
Response: 60400650
Conc: 17.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
TOTE-4-25-2023

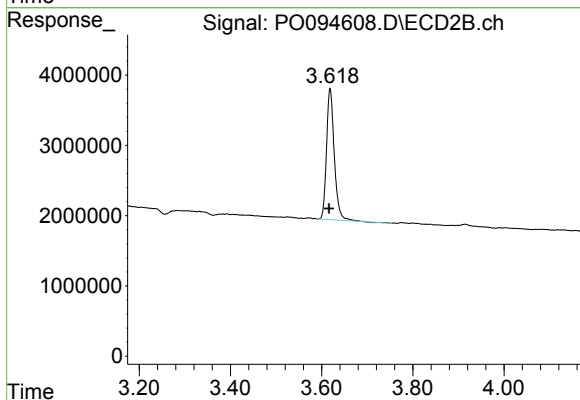


#1 Tetrachloro-m-xylene

R.T.: 3.619 min
Delta R.T.: 0.002 min
Response: 21983464
Conc: 16.43 ng/ml

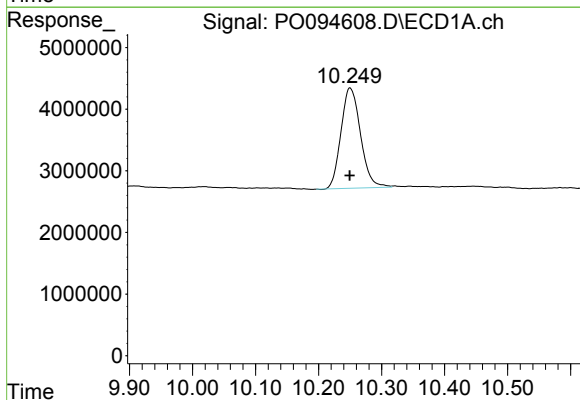

#2 Decachlorobiphenyl

R.T.: 10.250 min
Delta R.T.: 0.000 min
Response: 35091068
Conc: 14.46 ng/ml

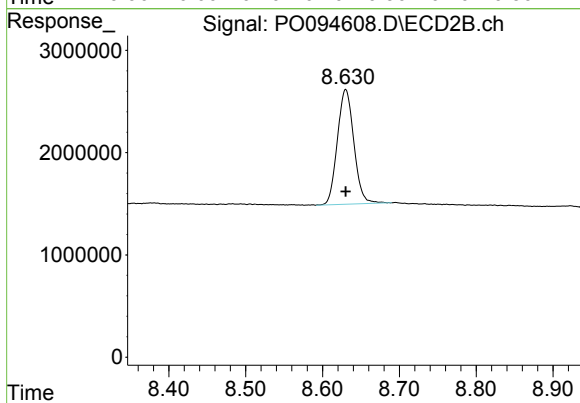

#2 Decachlorobiphenyl

R.T.: 8.630 min
Delta R.T.: 0.000 min
Response: 16639680
Conc: 14.78 ng/ml