

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042825\
 Data File : P0110834.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Apr 2025 04:02
 Operator : YP/AJ
 Sample : Q1900-01
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 WC-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/29/2025
 Supervised By :mohammad ahmed 05/02/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 29 06:10:19 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0041025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 11 02:12:41 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.686	3.683	165.2E6	87028306	18.882	17.441
2) SA Decachlor...	8.726	8.678	112.1E6	26881236	14.204m	13.964m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO042825\
Data File : PO110834.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Apr 2025 04:02
Operator : YP/AJ
Sample : Q1900-01
Misc :
ALS Vial : 38 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
WC-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/29/2025
Supervised By :mohammad ahmed 05/02/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 29 06:10:19 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO041025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 11 02:12:41 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

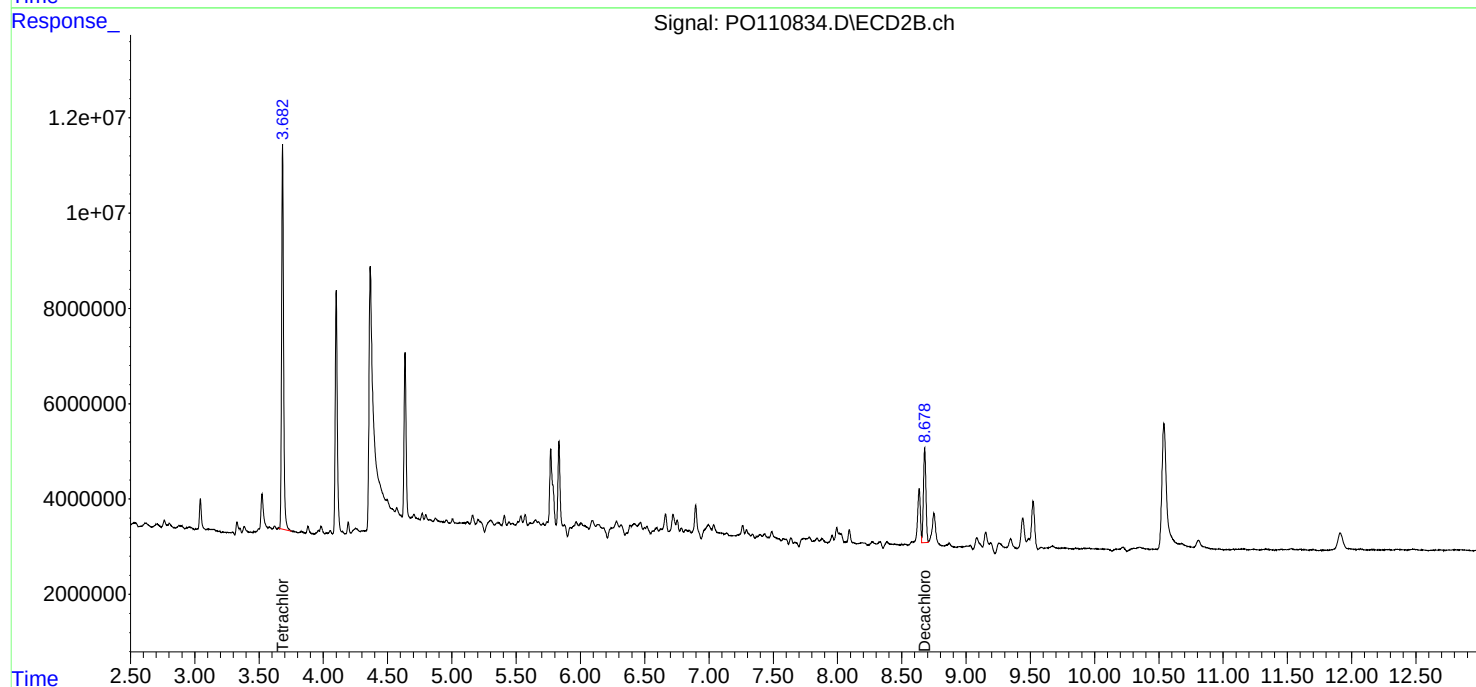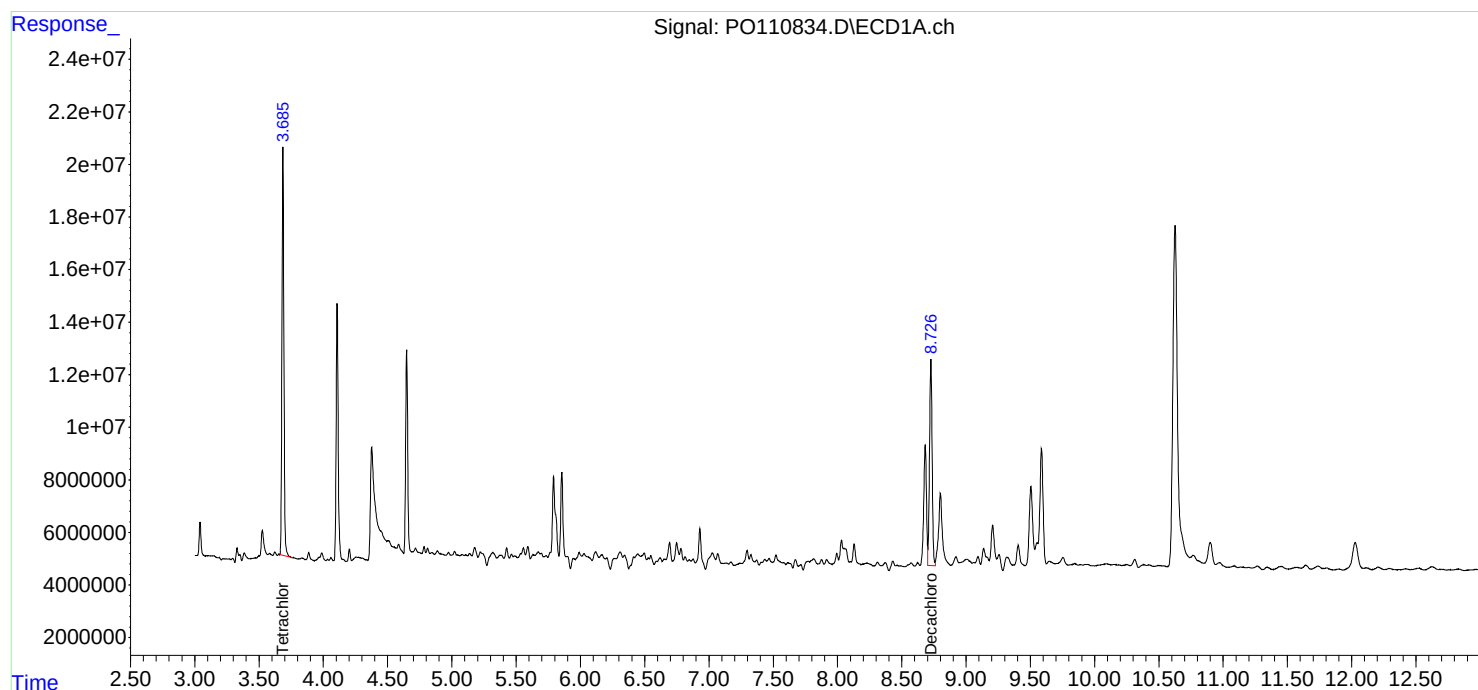

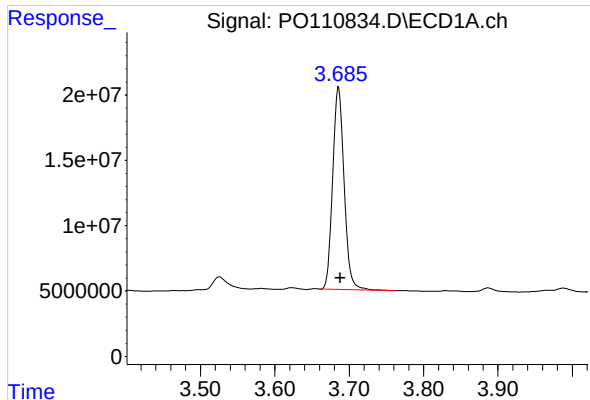


#1 Tetrachloro-m-xylene

R.T.: 3.686 min
Delta R.T.: -0.002 min
Response: 165195409
Conc: 18.88 ng/ml

Instrument :
ECD_O
ClientSampleId :
WC-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/29/2025
Supervised By :mohammad ahmed 05/02/2025

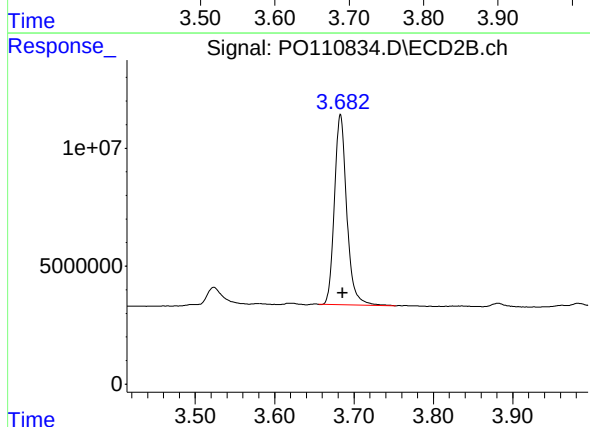


#1 Tetrachloro-m-xylene

R.T.: 3.683 min
Delta R.T.: -0.003 min
Response: 87028306
Conc: 17.44 ng/ml

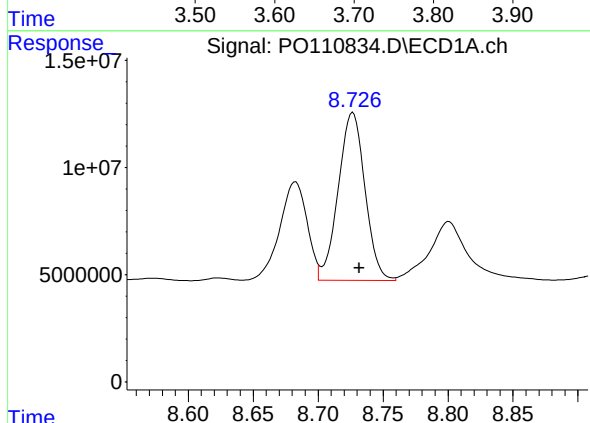

#2 Decachlorobiphenyl

R.T.: 8.726 min
Delta R.T.: -0.006 min
Response: 112141312
Conc: 14.20 ng/ml m

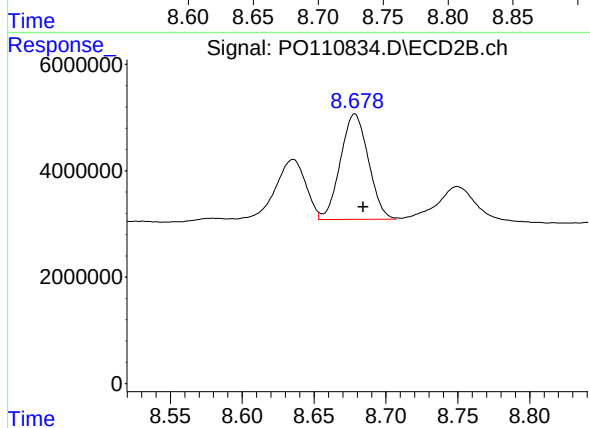

#2 Decachlorobiphenyl

R.T.: 8.678 min
Delta R.T.: -0.006 min
Response: 26881236
Conc: 13.96 ng/ml m