

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042921\
 Data File : P0077435.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Apr 2021 21:35
 Operator : DD\AJ
 Sample : M2217-23
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 30 01:26:05 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Apr 29 05:54:04 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.898	3.894	2691778	1313984	24.530	23.538
2)	SA Decachlor...	10.865	9.125	2069838	686158	18.823	20.170
Target Compounds							
7)	L1 AR-1016-5	0.000	5.615	0	30088	N.D.	18.849 #
9)	L2 AR-1221-2	5.249	0.000	27235	0	31.350	N.D. #
15)	L3 AR-1232-5	0.000	5.615	0	30088	N.D.	51.166 #
24)	L5 AR-1248-4	0.000	5.615	0	30088	N.D.	14.920 #
29)	L6 AR-1254-4	0.000	6.833f	0	195210	N.D.	85.451 #
30)	L6 AR-1254-5	8.464	0.000	95728	0	15.272	N.D. #
32)	L7 AR-1260-2	0.000	6.924f	0	56590	N.D.	15.218 #
34)	L7 AR-1260-4	8.737f	0.000	23732	0	4.334	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042921\
Data File : P0077435.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Apr 2021 21:35
Operator : DD\AJ
Sample : M2217-23
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 30 01:26:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042821.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Apr 29 05:54:04 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

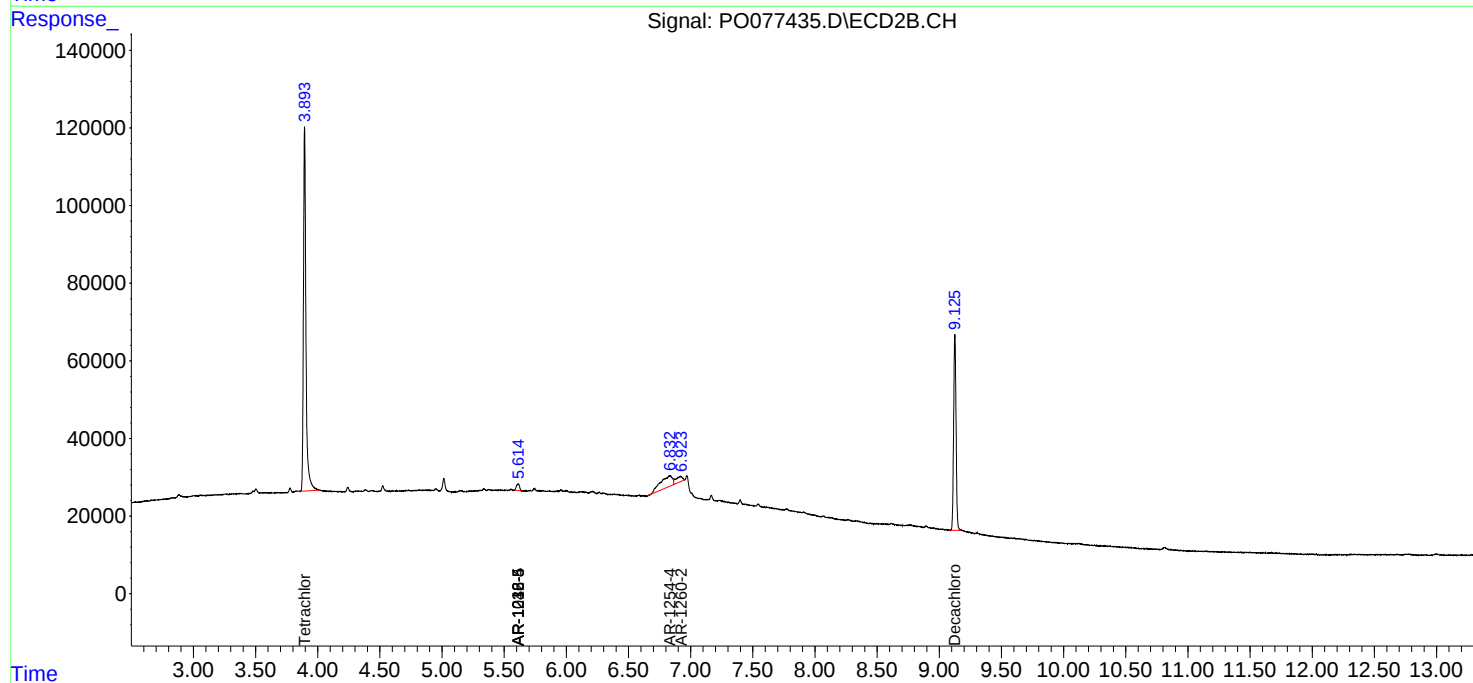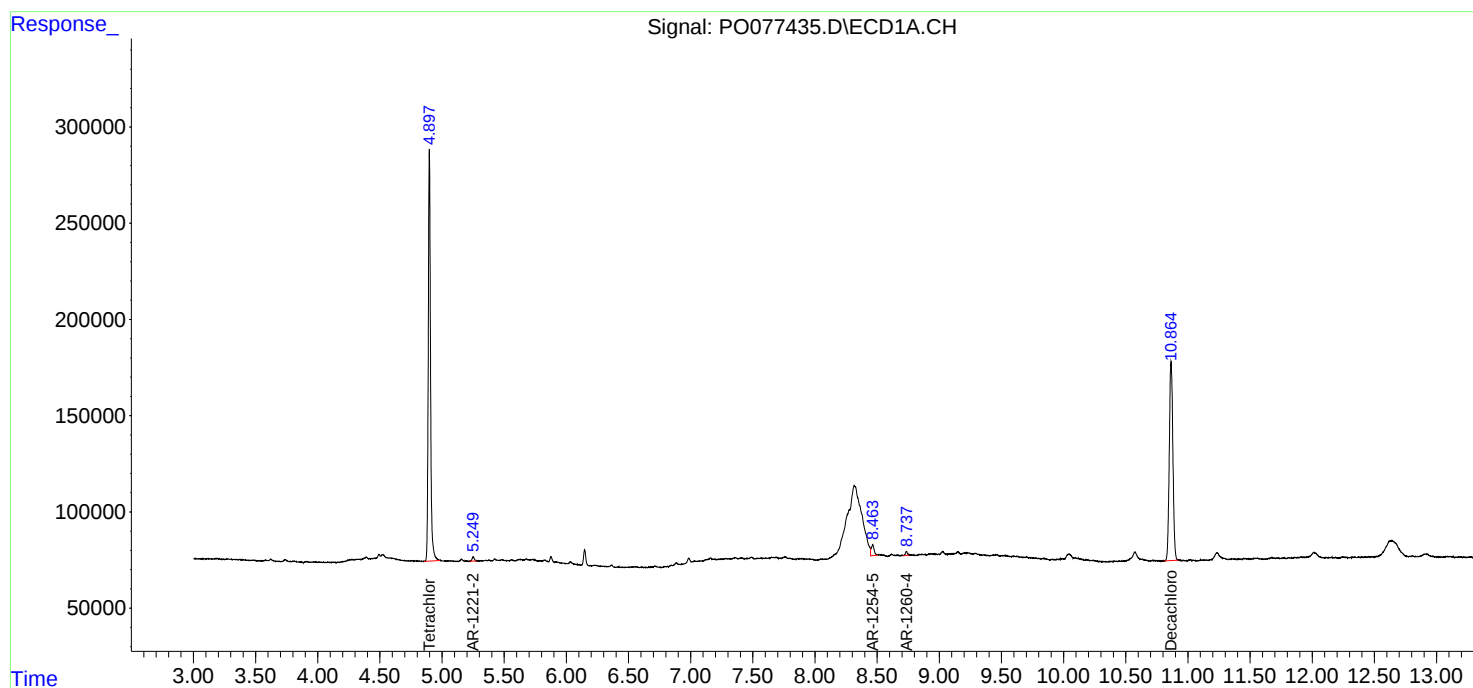


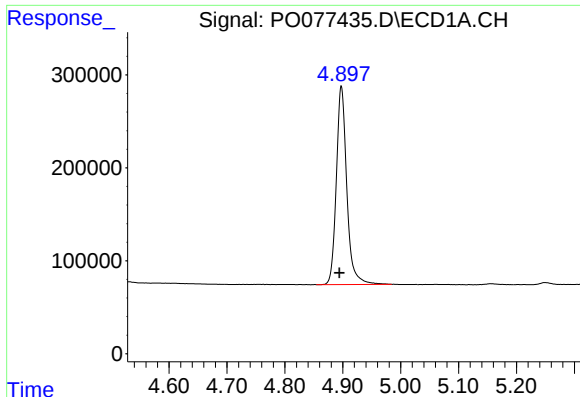

#1 Tetrachloro-m-xylene


R.T.: 4.898 min
Delta R.T.: 0.004 min
Response: 2691778
Conc: 24.53 ng/ml

Instrument :
ECD_O
ClientSampleId :

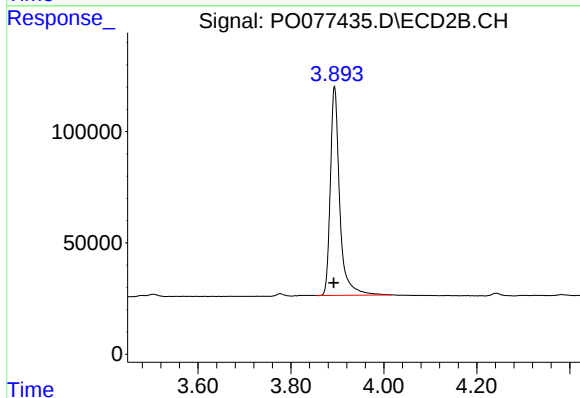


#1 Tetrachloro-m-xylene

R.T.: 3.894 min
Delta R.T.: 0.001 min
Response: 1313984
Conc: 23.54 ng/ml

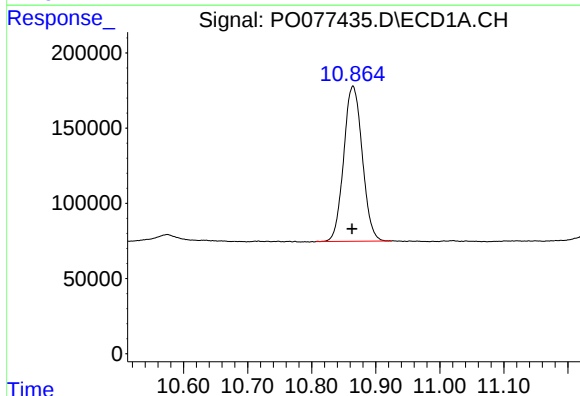


#2 Decachlorobiphenyl

R.T.: 10.865 min
Delta R.T.: 0.002 min
Response: 2069838
Conc: 18.82 ng/ml

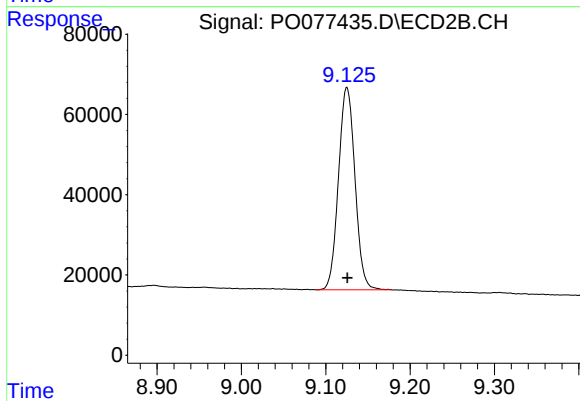

#2 Decachlorobiphenyl


R.T.: 9.125 min
Delta R.T.: 0.000 min
Response: 686158
Conc: 20.17 ng/ml

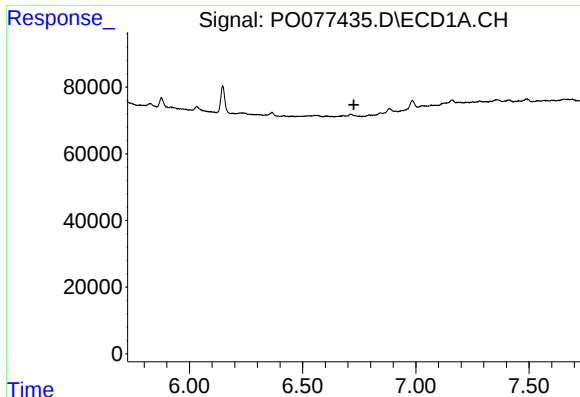

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T.: 6.726 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

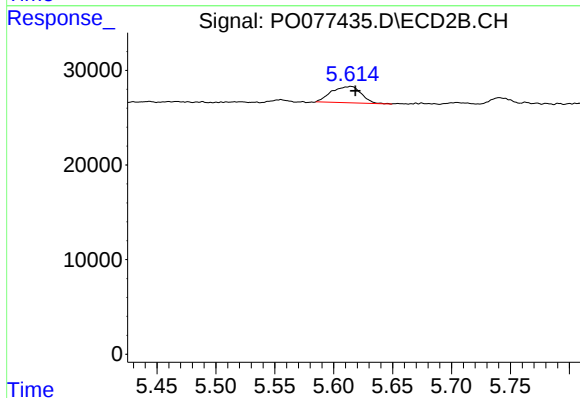


#7 AR-1016-5

R.T.: 5.615 min
Delta R.T.: -0.004 min
Response: 30088
Conc: 18.85 ng/ml

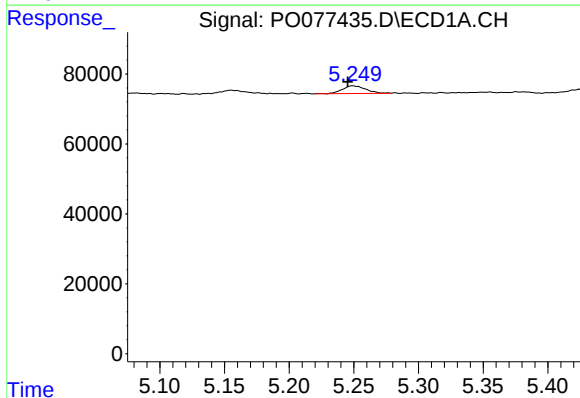


#9 AR-1221-2

R.T.: 5.249 min
Delta R.T.: 0.004 min
Response: 27235
Conc: 31.35 ng/ml

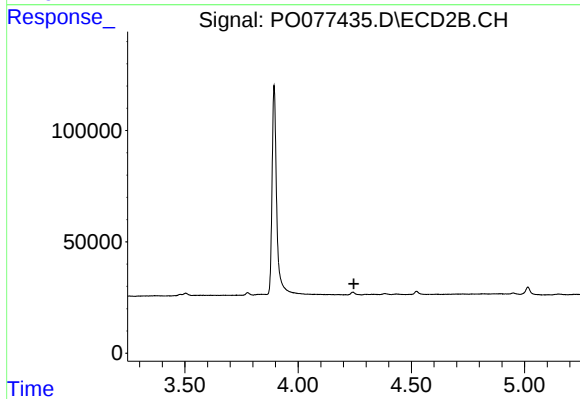

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T.: 4.247 min
Response: 0
Conc: N.D.

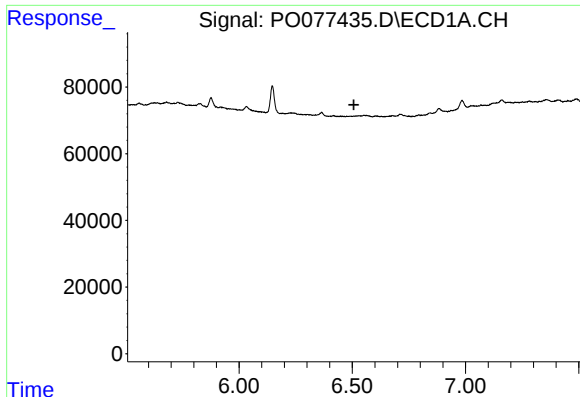

#15 AR-1232-5


R.T.: 0.000 min
Exp R.T. : 6.507 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

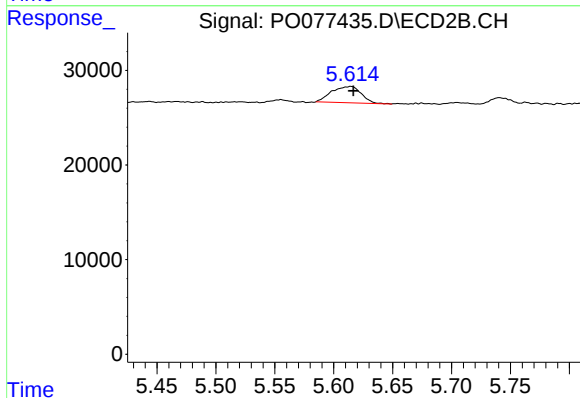


#15 AR-1232-5

R.T.: 5.615 min
Delta R.T.: -0.002 min
Response: 30088
Conc: 51.17 ng/ml

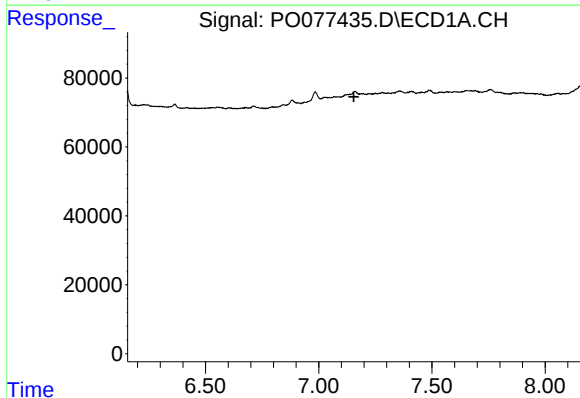


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 7.155 min
Response: 0
Conc: N.D.

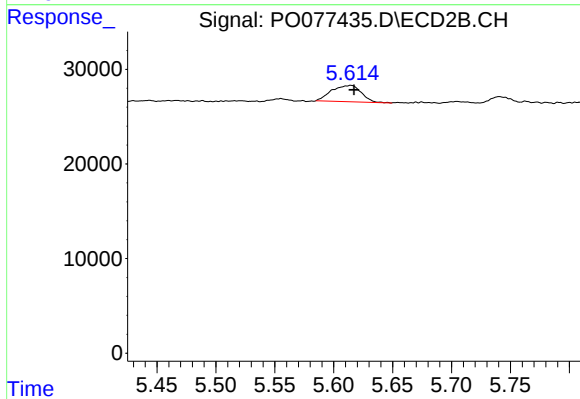

#24 AR-1248-4


R.T.: 5.615 min
Delta R.T.: -0.003 min
Response: 30088
Conc: 14.92 ng/ml

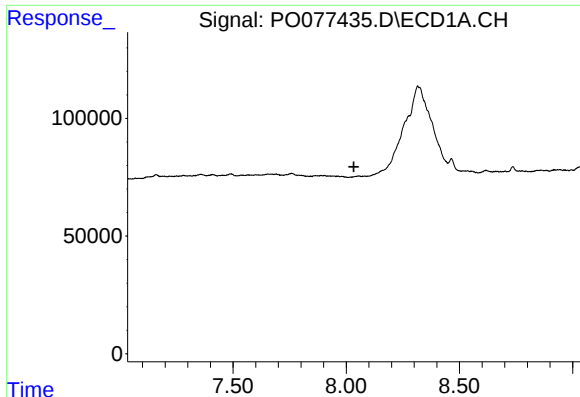

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T.: 8.033 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

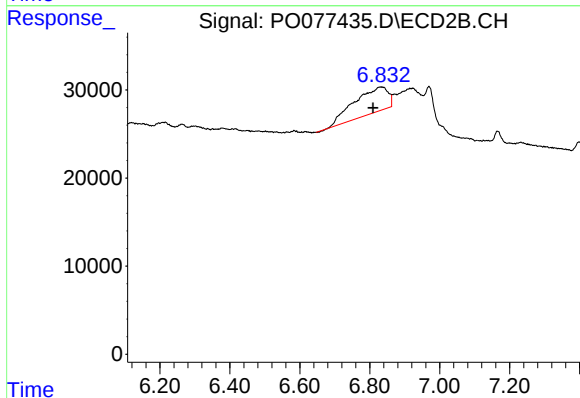


#29 AR-1254-4

R.T.: 6.833 min
Delta R.T.: 0.023 min
Response: 195210
Conc: 85.45 ng/ml

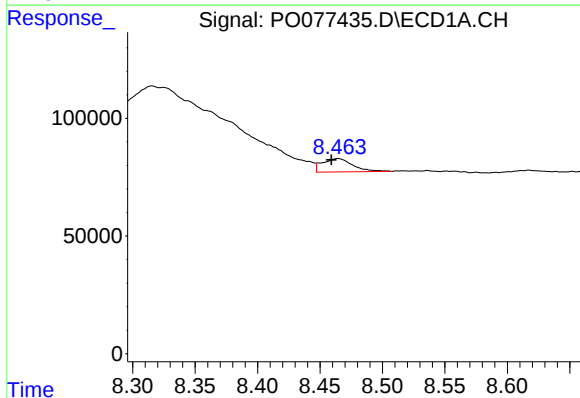


#30 AR-1254-5

R.T.: 8.464 min
Delta R.T.: 0.005 min
Response: 95728
Conc: 15.27 ng/ml

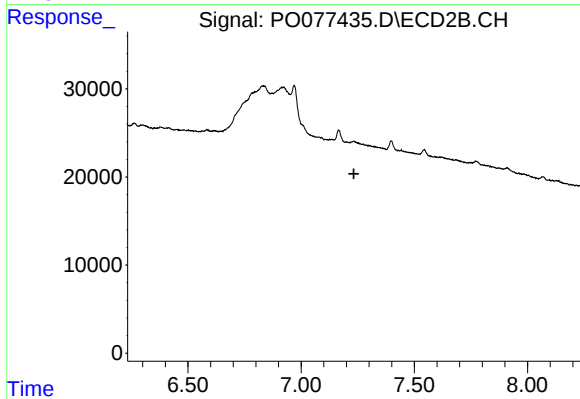

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T.: 7.233 min
Response: 0
Conc: N.D.

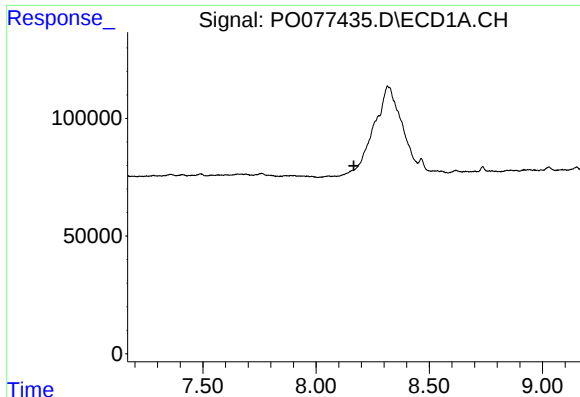

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T.: 8.167 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

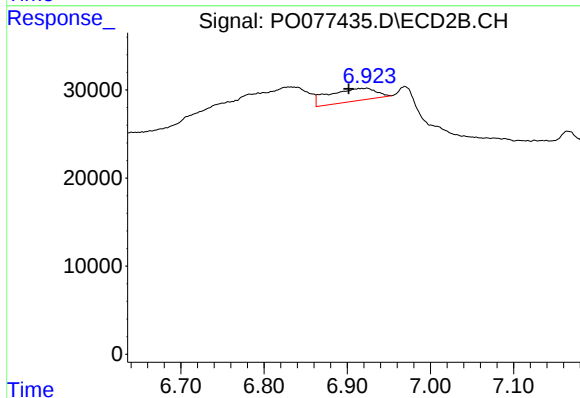


#32 AR-1260-2

R.T.: 6.924 min
Delta R.T.: 0.022 min
Response: 56590
Conc: 15.22 ng/ml

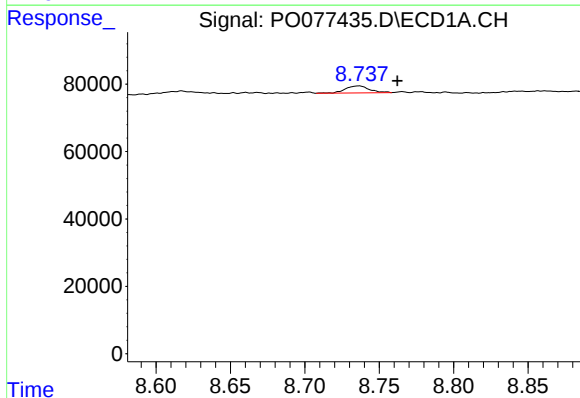

#34 AR-1260-4

R.T.: 8.737 min
Delta R.T.: -0.026 min
Response: 23732
Conc: 4.33 ng/ml

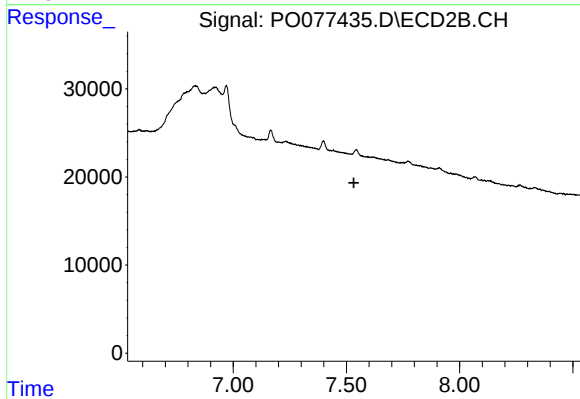

#34 AR-1260-4

R.T.: 0.000 min
Exp R.T.: 7.533 min
Response: 0
Conc: N.D.