

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042921\
 Data File : P0077405.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Apr 2021 11:17
 Operator : DD\AJ
 Sample : M2184-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 NCQ-632

Manual Integrations
 APPROVED

Ankita
 4/30/2021 2:27:49 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 29 14:55:57 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Apr 29 05:54:04 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.886	3.901	3488900	2844209	31.794	50.951m#
2) SA Decachlor...	10.864	9.124	932125	225821	8.477	6.638

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042921\
Data File : P0077405.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Apr 2021 11:17
Operator : DD\AJ
Sample : M2184-03
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
NCQ-632


Manual Integrations
APPROVED

Ankita
4/30/2021 2:27:49 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 29 14:55:57 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042821.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Apr 29 05:54:04 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

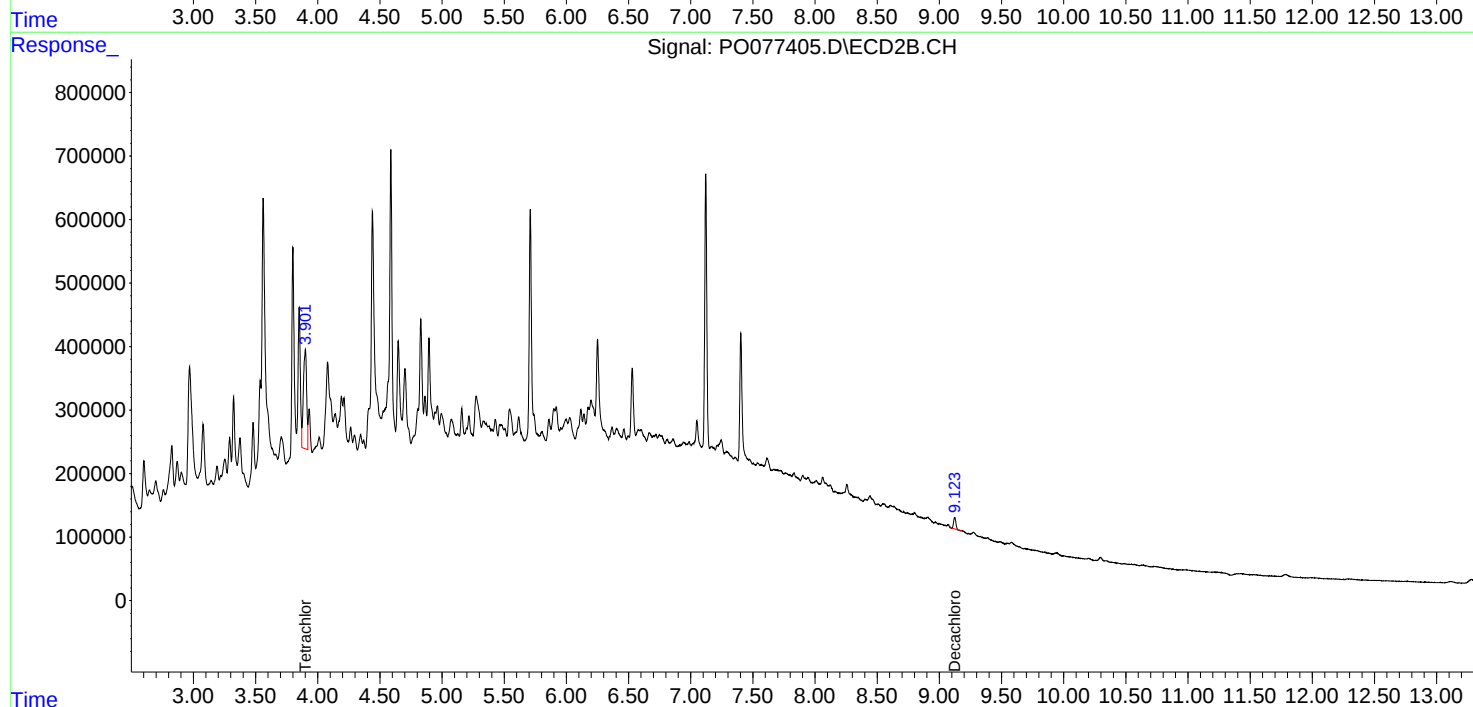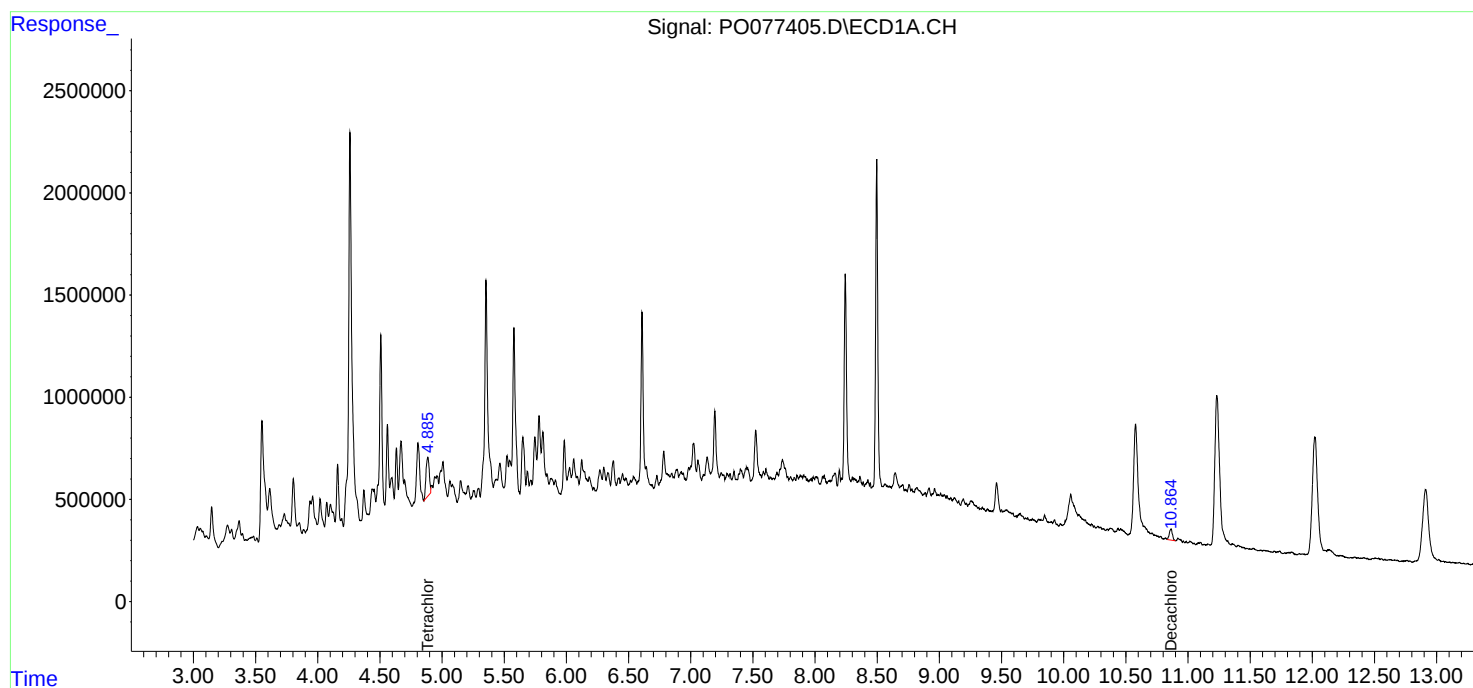

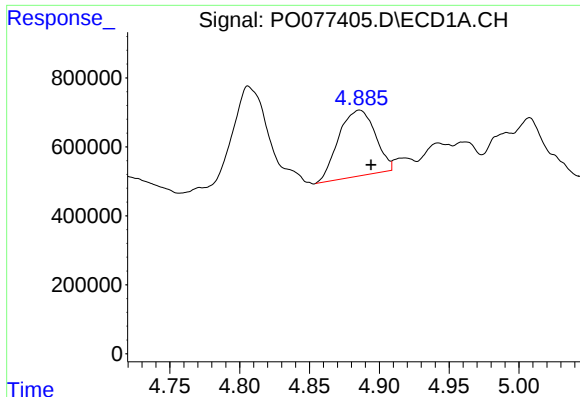


#1 Tetrachloro-m-xylene

R.T.: 4.886 min
Delta R.T.: -0.008 min
Response: 3488900
Conc: 31.79 ng/ml

Instrument :
ECD_O
ClientSampleId :
NCQ-632


Manual Integrations
APPROVED

Ankita
4/30/2021 2:27:49 PM

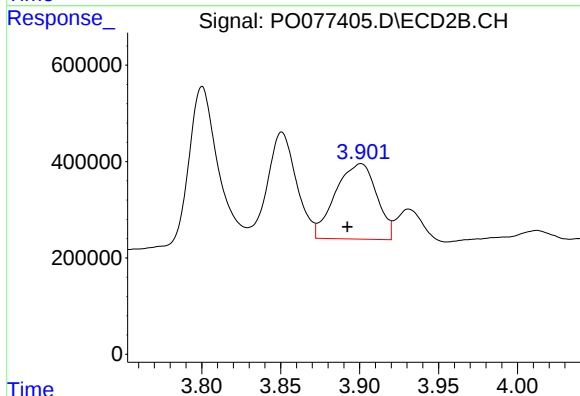


#1 Tetrachloro-m-xylene

R.T.: 3.901 min
Delta R.T.: 0.008 min
Response: 2844209
Conc: 50.95 ng/ml m

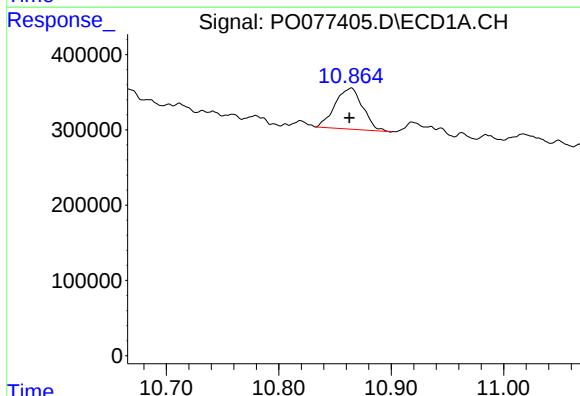

#2 Decachlorobiphenyl

R.T.: 10.864 min
Delta R.T.: 0.002 min
Response: 932125
Conc: 8.48 ng/ml

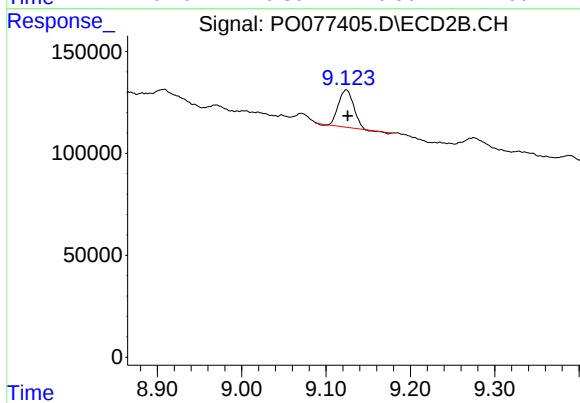

#2 Decachlorobiphenyl

R.T.: 9.124 min
Delta R.T.: -0.002 min
Response: 225821
Conc: 6.64 ng/ml