

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042921\
 Data File : P0077406.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Apr 2021 11:34
 Operator : DD\AJ
 Sample : M2184-03RE
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 NCQ-632RE

Manual Integrations
 APPROVED

Ankita
 4/30/2021 2:27:51 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 29 14:56:35 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Apr 29 05:54:04 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.885	3.899	3565498	2744155	32.492	49.158m#
2) SA Decachlor...	10.856	9.123	745663	231779	6.781	6.813

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042921\
Data File : P0077406.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Apr 2021 11:34
Operator : DD\AJ
Sample : M2184-03RE
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
NCQ-632RE


Manual Integrations
APPROVED

Ankita
4/30/2021 2:27:51 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 29 14:56:35 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042821.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Apr 29 05:54:04 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

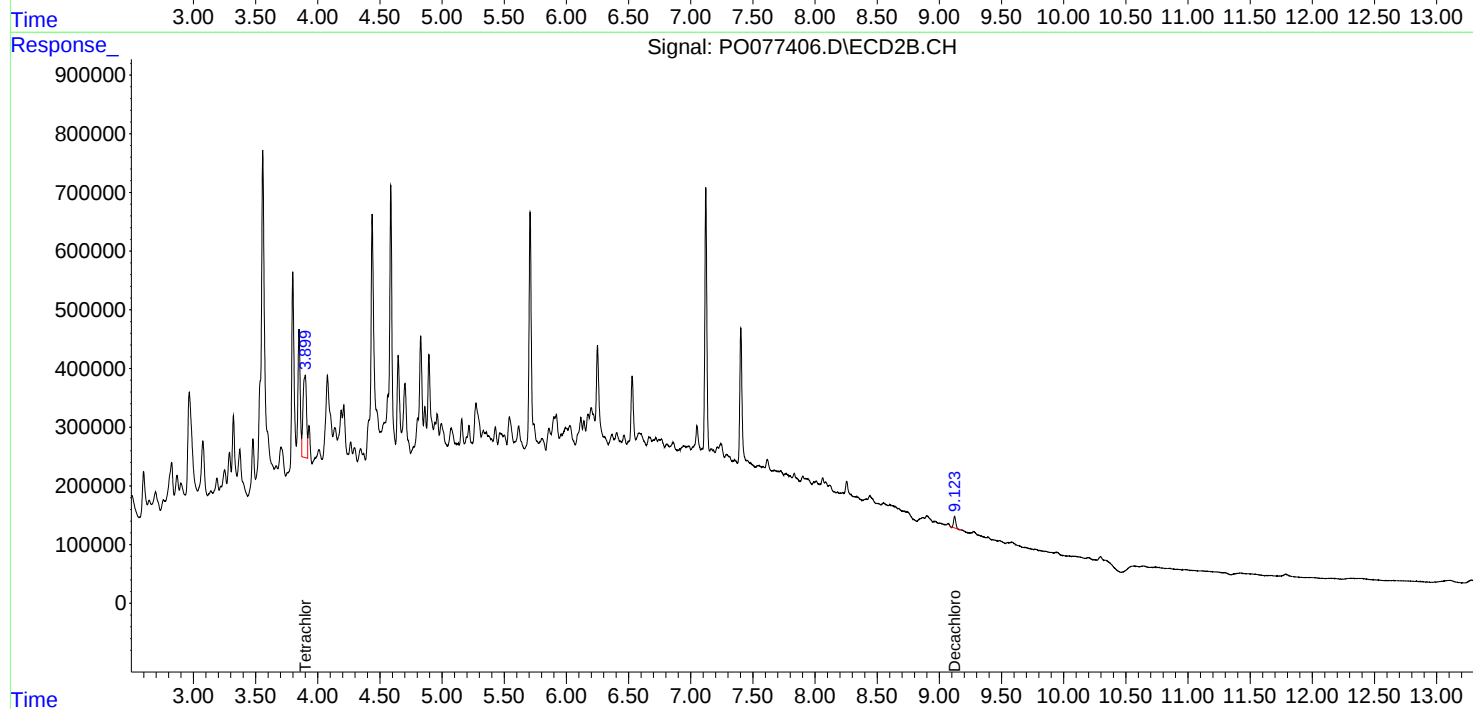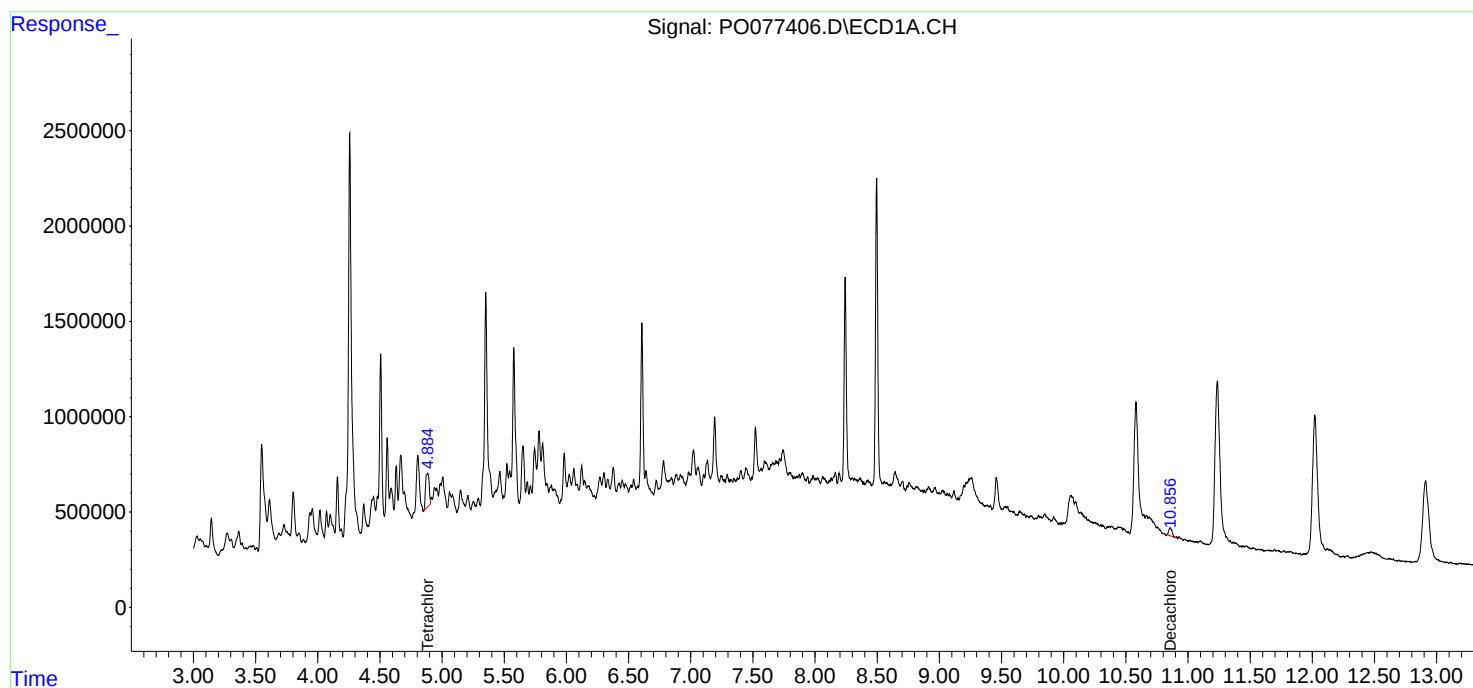

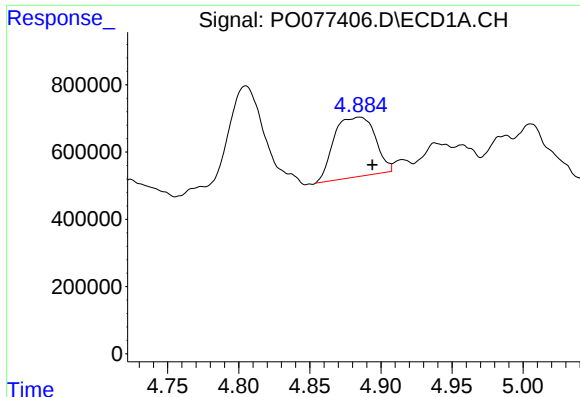


#1 Tetrachloro-m-xylene

R.T.: 4.885 min
Delta R.T.: -0.009 min
Response: 3565498
Conc: 32.49 ng/ml

Instrument :
ECD_O
ClientSampleId :
NCQ-632RE


Manual Integrations
APPROVED

Ankita
4/30/2021 2:27:51 PM

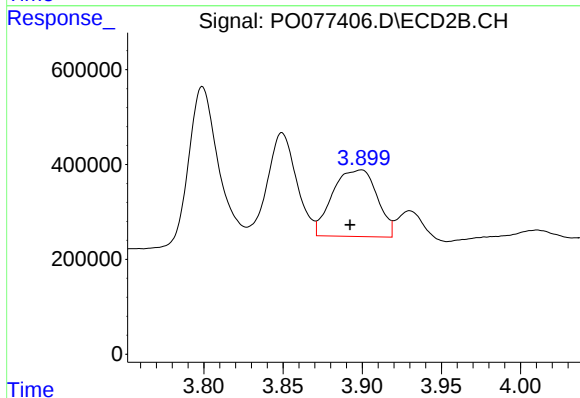


#1 Tetrachloro-m-xylene

R.T.: 3.899 min
Delta R.T.: 0.007 min
Response: 2744155
Conc: 49.16 ng/ml m

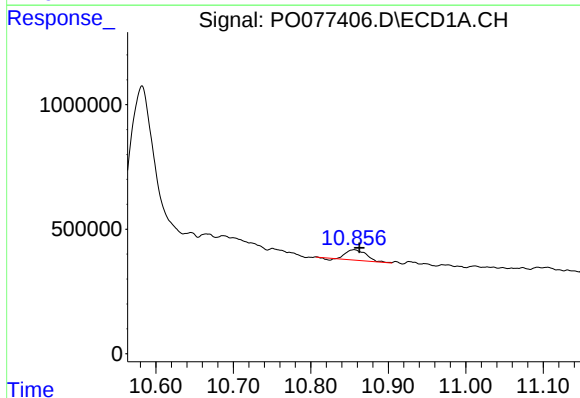

#2 Decachlorobiphenyl

R.T.: 10.856 min
Delta R.T.: -0.007 min
Response: 745663
Conc: 6.78 ng/ml

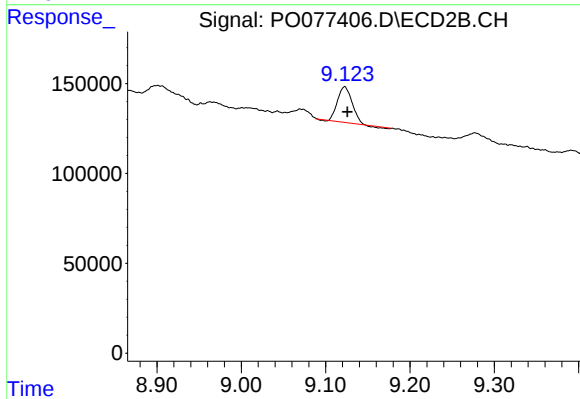

#2 Decachlorobiphenyl

R.T.: 9.123 min
Delta R.T.: -0.003 min
Response: 231779
Conc: 6.81 ng/ml