

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0042921\
 Data File : P0077407.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Apr 2021 12:08
 Operator : DD\AJ
 Sample : M2154-02
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 33096

Manual Integrations
 APPROVED

Ankita
 4/30/2021 2:27:53 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 29 16:09:38 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0042821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Apr 29 05:54:04 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.897	3.894	1892136	749907	17.243m	13.434
2) SA Decachlor...	10.866	9.125	394354	114295	3.586	3.360
Target Compounds						
26) L6 AR-1254-1	7.125	5.993	494165	371895	104.828m	120.350
27) L6 AR-1254-2	7.355	6.151	695326	334255	93.619m	120.603 #
28) L6 AR-1254-3	7.735	6.567	772745	439393	99.587m	107.806
29) L6 AR-1254-4	8.030	6.806	777717	268266	135.066m	117.430
30) L6 AR-1254-5	8.460	7.231	587735	403471	93.763m	110.023

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042921\
Data File : P0077407.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Apr 2021 12:08
Operator : DD\AJ
Sample : M2154-02
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
33096


Manual Integrations
APPROVED

Ankita
4/30/2021 2:27:53 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 29 16:09:38 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042821.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Apr 29 05:54:04 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

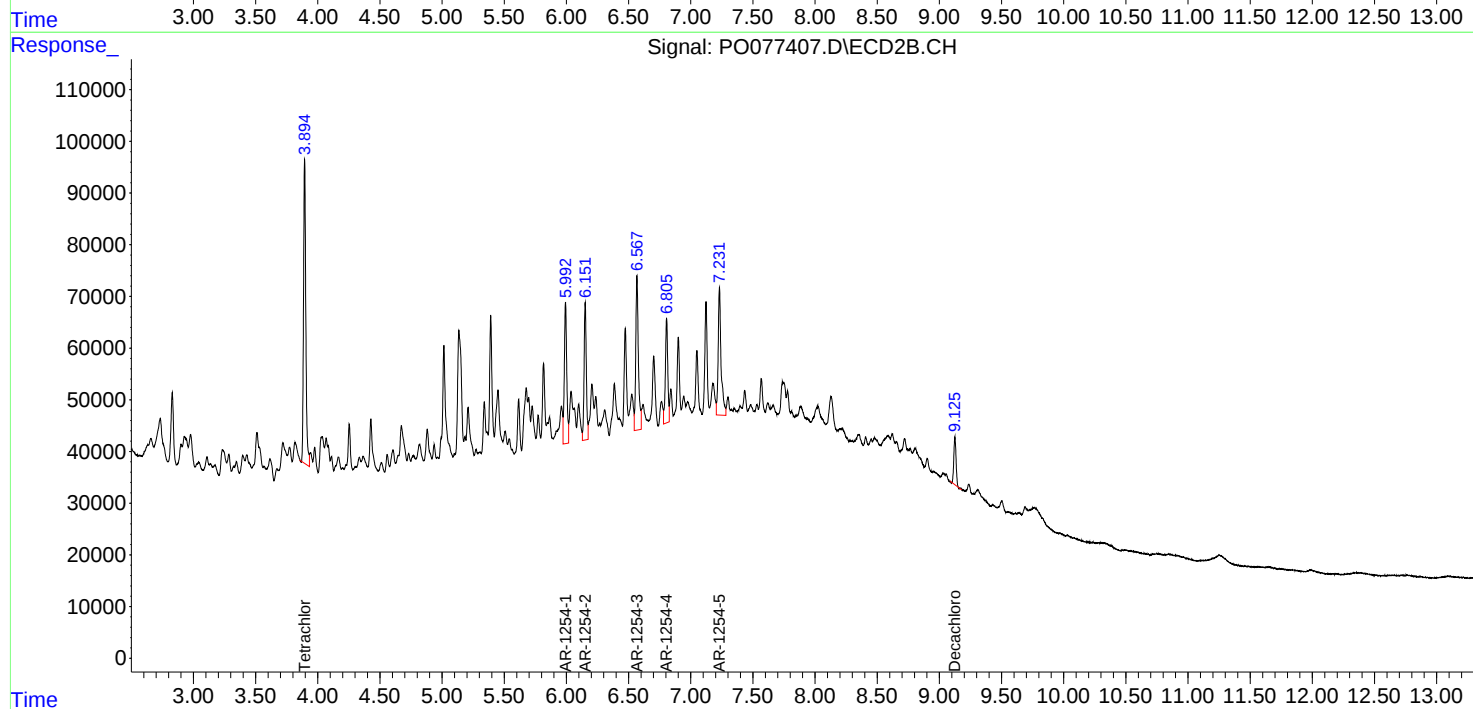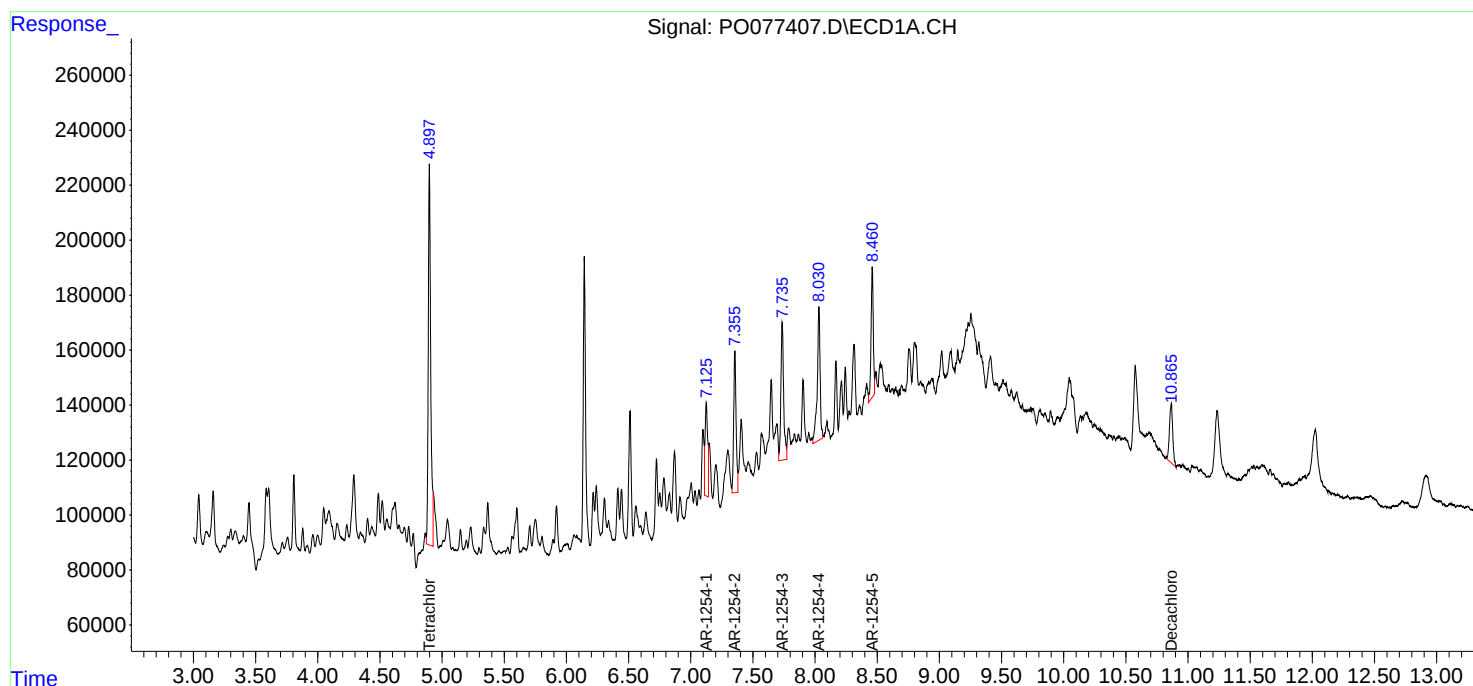

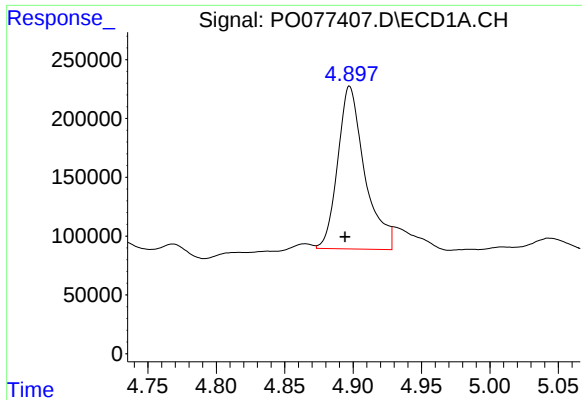


#1 Tetrachloro-m-xylene

R.T.: 4.897 min
Delta R.T.: 0.003 min
Response: 1892136
Conc: 17.24 ng/ml m

Instrument :
ECD_O
ClientSampleId :
33096


Manual Integrations
APPROVED

Ankita
4/30/2021 2:27:53 PM

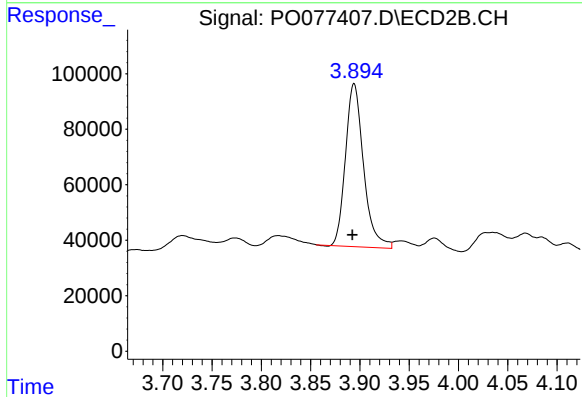


#1 Tetrachloro-m-xylene

R.T.: 3.894 min
Delta R.T.: 0.002 min
Response: 749907
Conc: 13.43 ng/ml

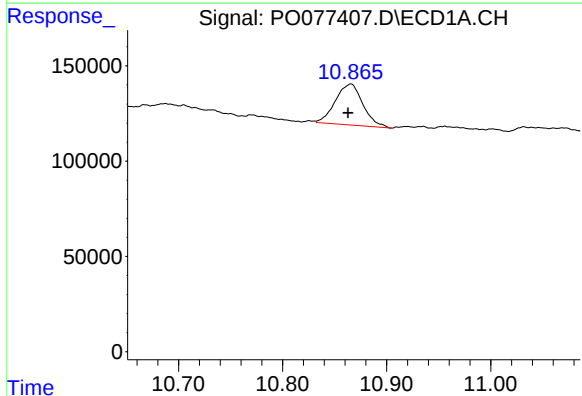


#2 Decachlorobiphenyl

R.T.: 10.866 min
Delta R.T.: 0.003 min
Response: 394354
Conc: 3.59 ng/ml

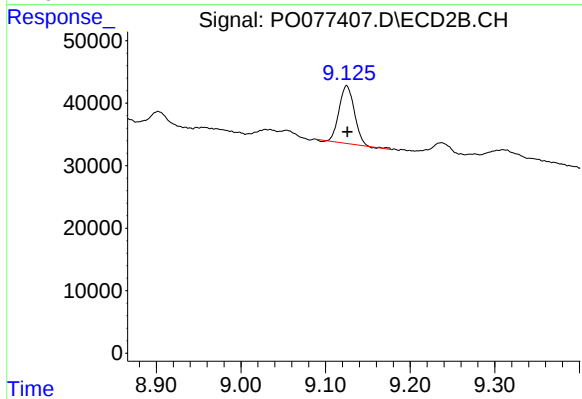

#2 Decachlorobiphenyl

R.T.: 9.125 min
Delta R.T.: 0.000 min
Response: 114295
Conc: 3.36 ng/ml

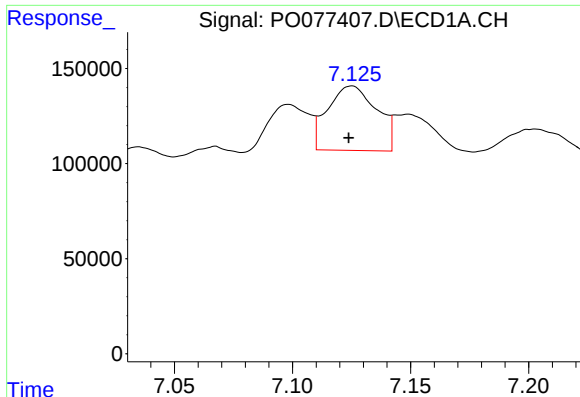


#26 AR-1254-1

R.T.: 7.125 min
Delta R.T.: 0.001 min
Response: 494165
Conc: 104.83 ng/ml m

Instrument :
ECD_O
ClientSampleId :
33096


Manual Integrations
APPROVED

Ankita
4/30/2021 2:27:53 PM

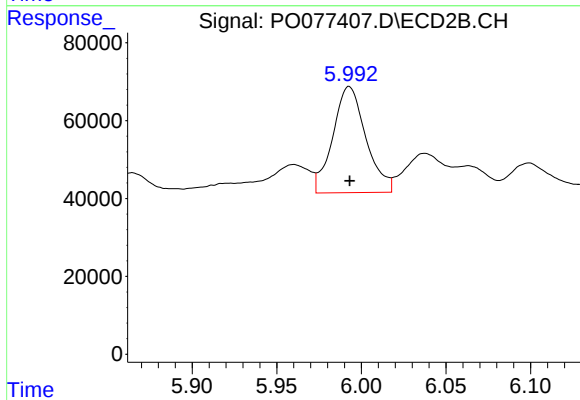


#26 AR-1254-1

R.T.: 5.993 min
Delta R.T.: 0.000 min
Response: 371895
Conc: 120.35 ng/ml

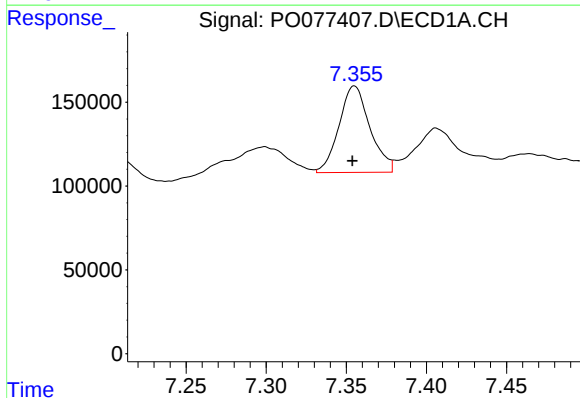


#27 AR-1254-2

R.T.: 7.355 min
Delta R.T.: 0.000 min
Response: 695326
Conc: 93.62 ng/ml m

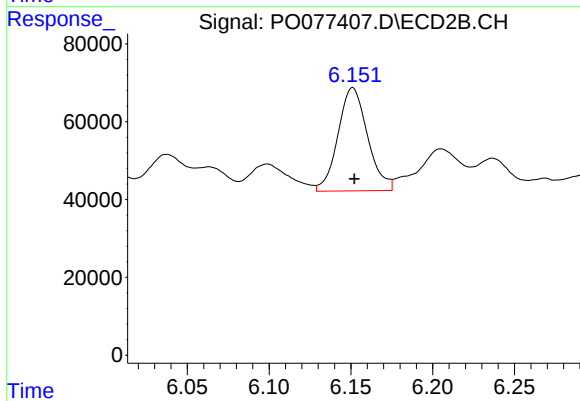

#27 AR-1254-2

R.T.: 6.151 min
Delta R.T.: 0.000 min
Response: 334255
Conc: 120.60 ng/ml

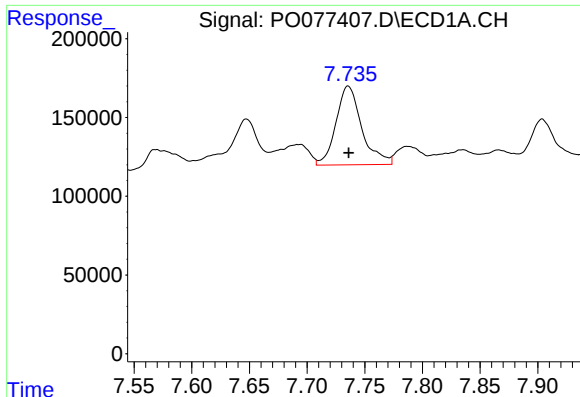


#28 AR-1254-3

R.T.: 7.735 min
Delta R.T.: 0.000 min
Response: 772745
Conc: 99.59 ng/ml m

Instrument :
ECD_O
ClientSampleId :
33096


Manual Integrations
APPROVED

Ankita
4/30/2021 2:27:53 PM

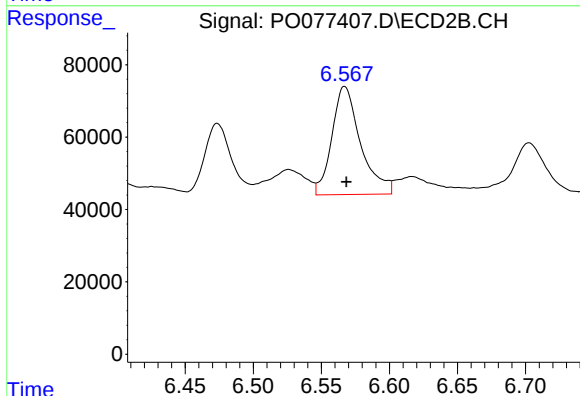


#28 AR-1254-3

R.T.: 6.567 min
Delta R.T.: -0.001 min
Response: 439393
Conc: 107.81 ng/ml

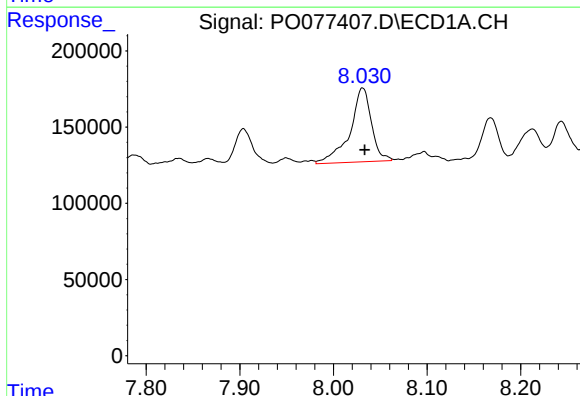


#29 AR-1254-4

R.T.: 8.030 min
Delta R.T.: -0.003 min
Response: 777717
Conc: 135.07 ng/ml m

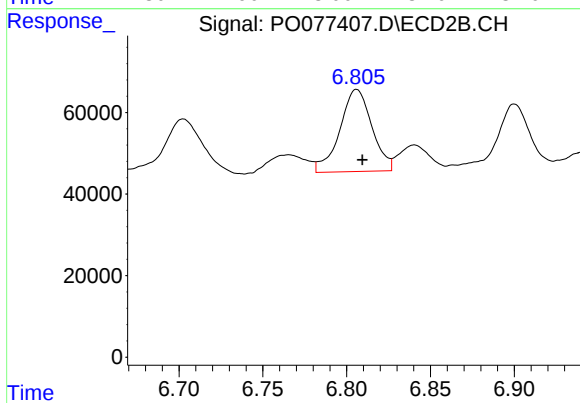

#29 AR-1254-4

R.T.: 6.806 min
Delta R.T.: -0.003 min
Response: 268266
Conc: 117.43 ng/ml

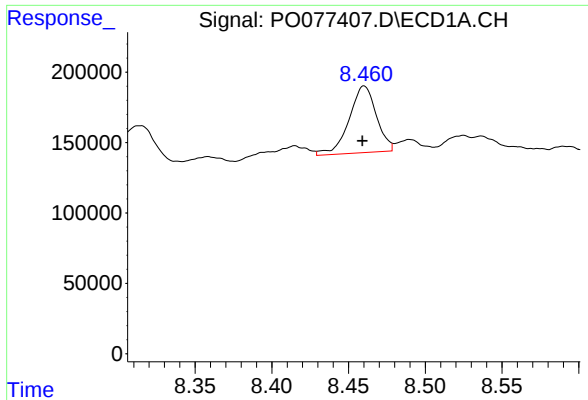


#30 AR-1254-5

R.T.: 8.460 min
Delta R.T.: 0.000 min
Response: 587735
Conc: 93.76 ng/ml m

Instrument :
ECD_O
ClientSampleId :
33096

Manual Integrations
APPROVED

Ankita
4/30/2021 2:27:53 PM

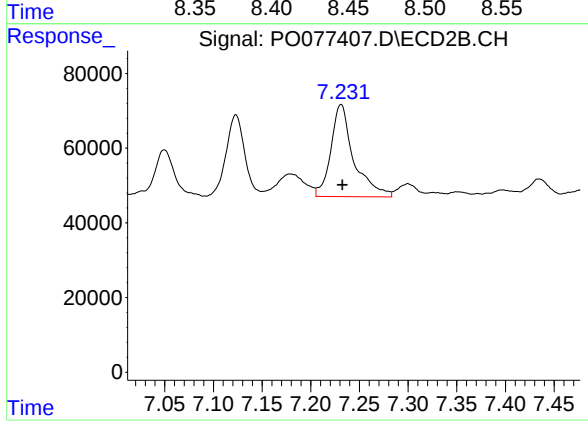

#30 AR-1254-5

R.T.: 7.231 min
Delta R.T.: -0.002 min
Response: 403471
Conc: 110.02 ng/ml