

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042921\
 Data File : P0077430.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Apr 2021 20:09
 Operator : DD\AJ
 Sample : M2217-18
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 HTRCV2-GRAB-CF02-02

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 30 01:23:55 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Apr 29 05:54:04 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.897	3.894	2404930	1167939	21.916	20.922
2) SA Decachlor...	10.866	9.125	2016827	620367	18.341	18.236

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042921\
Data File : P0077430.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Apr 2021 20:09
Operator : DD\AJ
Sample : M2217-18
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
HTCRV2-GRAB-CF02-02

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 30 01:23:55 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042821.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Apr 29 05:54:04 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

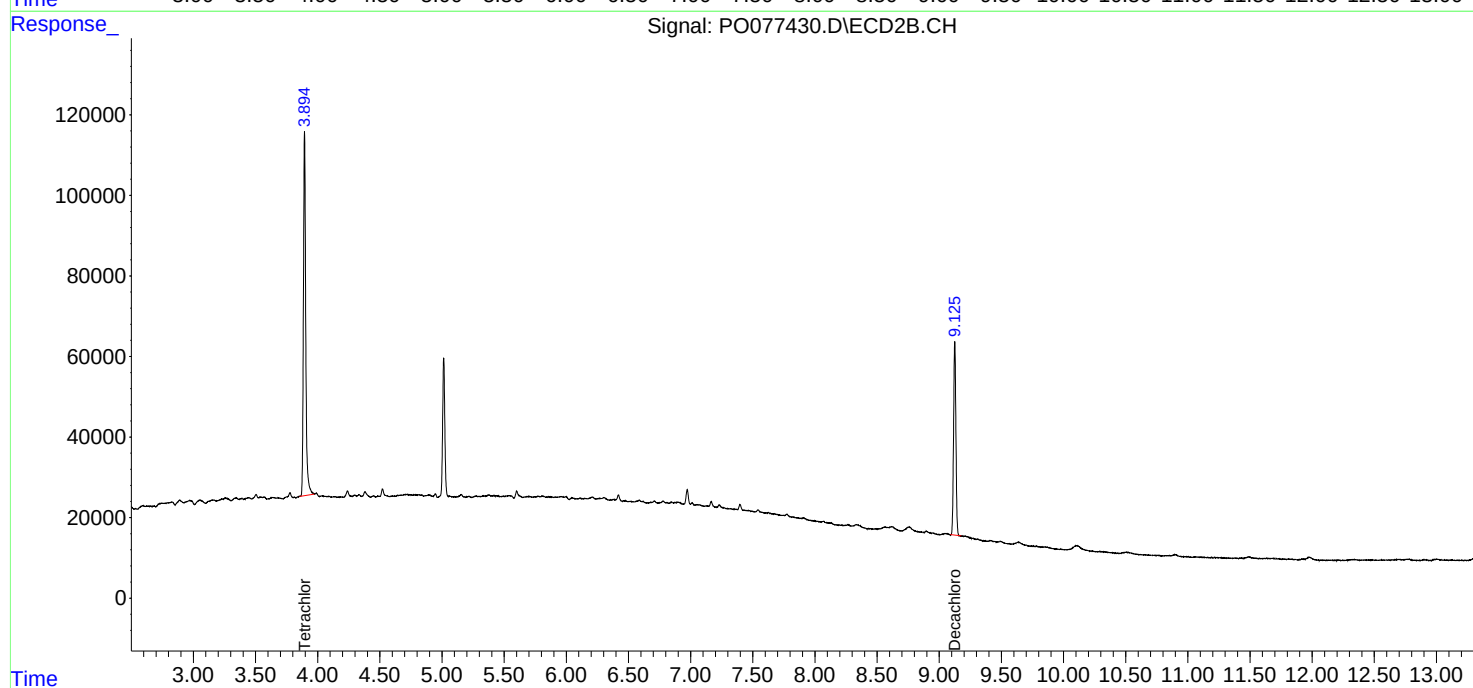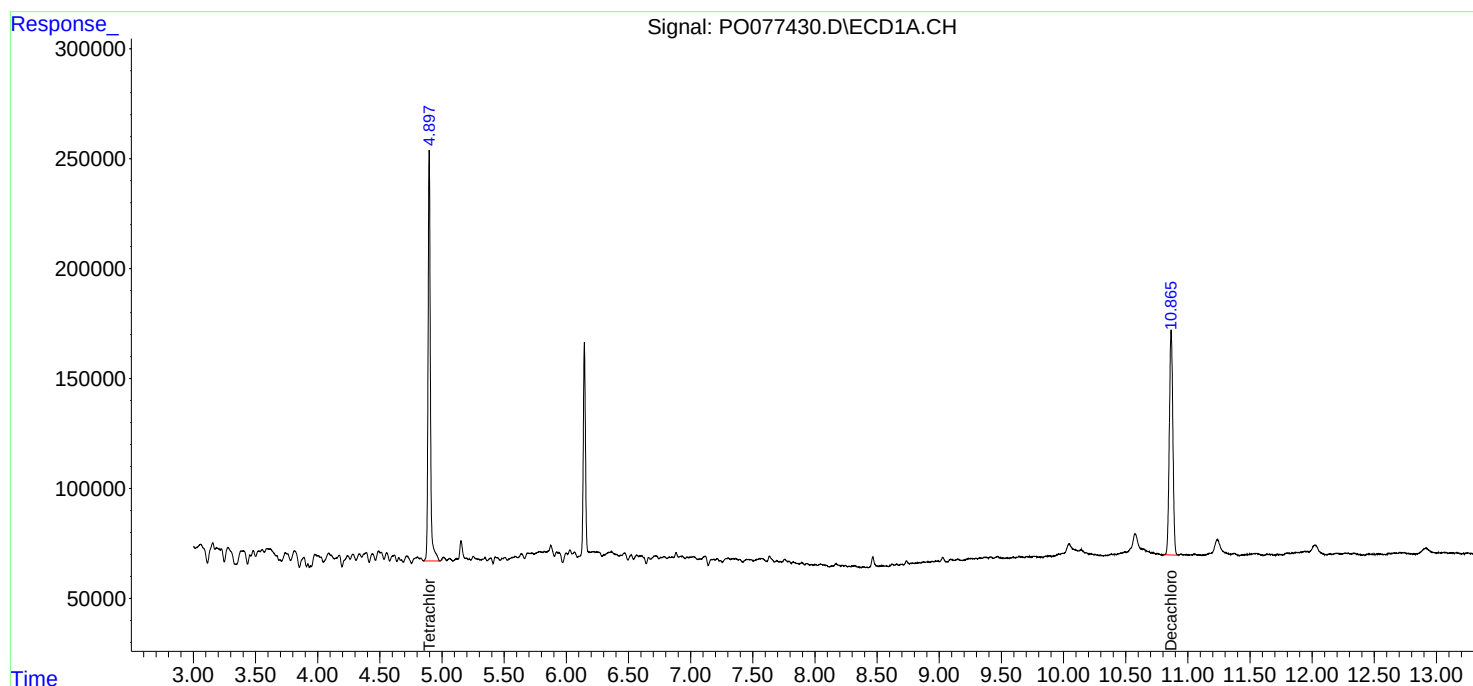


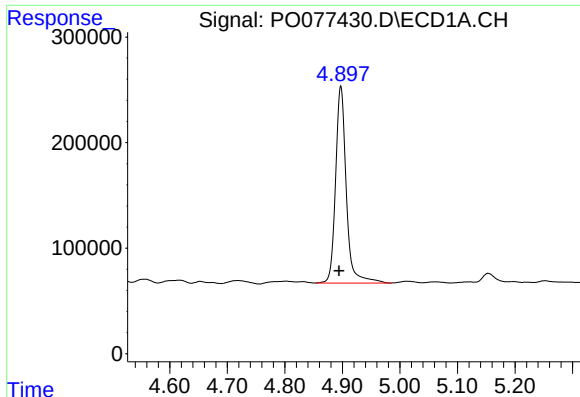

#1 Tetrachloro-m-xylene


R.T.: 4.897 min
Delta R.T.: 0.003 min
Response: 2404930
Conc: 21.92 ng/ml

Instrument :
ECD_O
ClientSampleId :
HTCRV2-GRAB-CF02-02

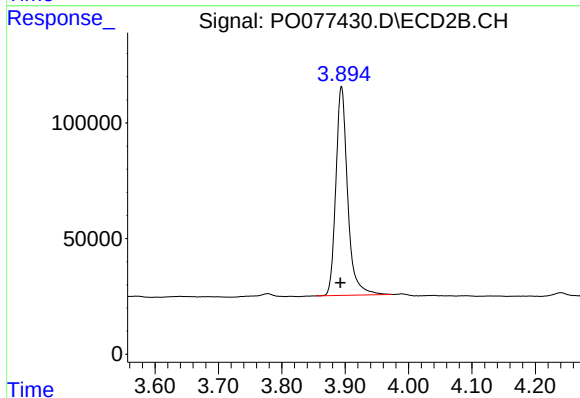


#1 Tetrachloro-m-xylene

R.T.: 3.894 min
Delta R.T.: 0.002 min
Response: 1167939
Conc: 20.92 ng/ml

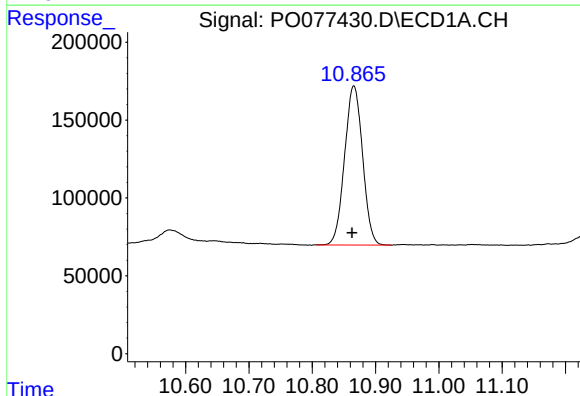

#2 Decachlorobiphenyl

R.T.: 10.866 min
Delta R.T.: 0.003 min
Response: 2016827
Conc: 18.34 ng/ml

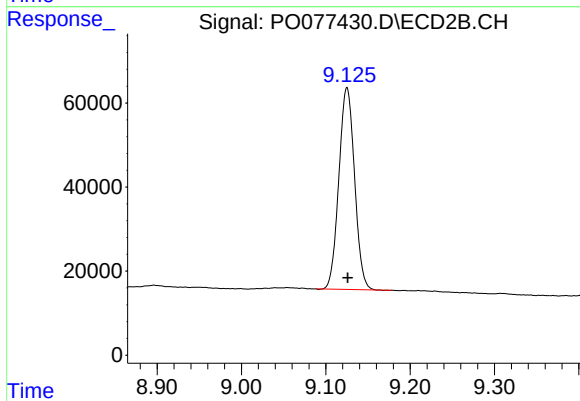

#2 Decachlorobiphenyl

R.T.: 9.125 min
Delta R.T.: 0.000 min
Response: 620367
Conc: 18.24 ng/ml