

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0043021\
 Data File : P0077470.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Apr 2021 20:11
 Operator : AJ/MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 01 01:57:18 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Apr 29 05:54:04 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.892	3.885	2171283	1080662	19.786	19.359
2)	SA Decachlor...	10.863	9.122	2334177	701996	21.227	20.636
Target Compounds							
9)	L2 AR-1221-2	5.246	0.000	24437	0	28.130	N.D. #
20)	L4 AR-1242-5	7.188	0.000	7268	0	2.633	N.D. #
24)	L5 AR-1248-4	7.150	0.000	41420	0	8.943	N.D. #
25)	L5 AR-1248-5	7.188	0.000	7268	0	1.534	N.D. #
26)	L6 AR-1254-1	7.150f	0.000	41420	0	8.786	N.D. #
28)	L6 AR-1254-3	7.759f	0.000	42503	0	5.478	N.D. #
45)	L9 AR-1268-5	10.554	0.000	33376	0	0.833	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO043021\
Data File : PO077470.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Apr 2021 20:11
Operator : AJ/MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 01 01:57:18 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO042821.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Apr 29 05:54:04 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

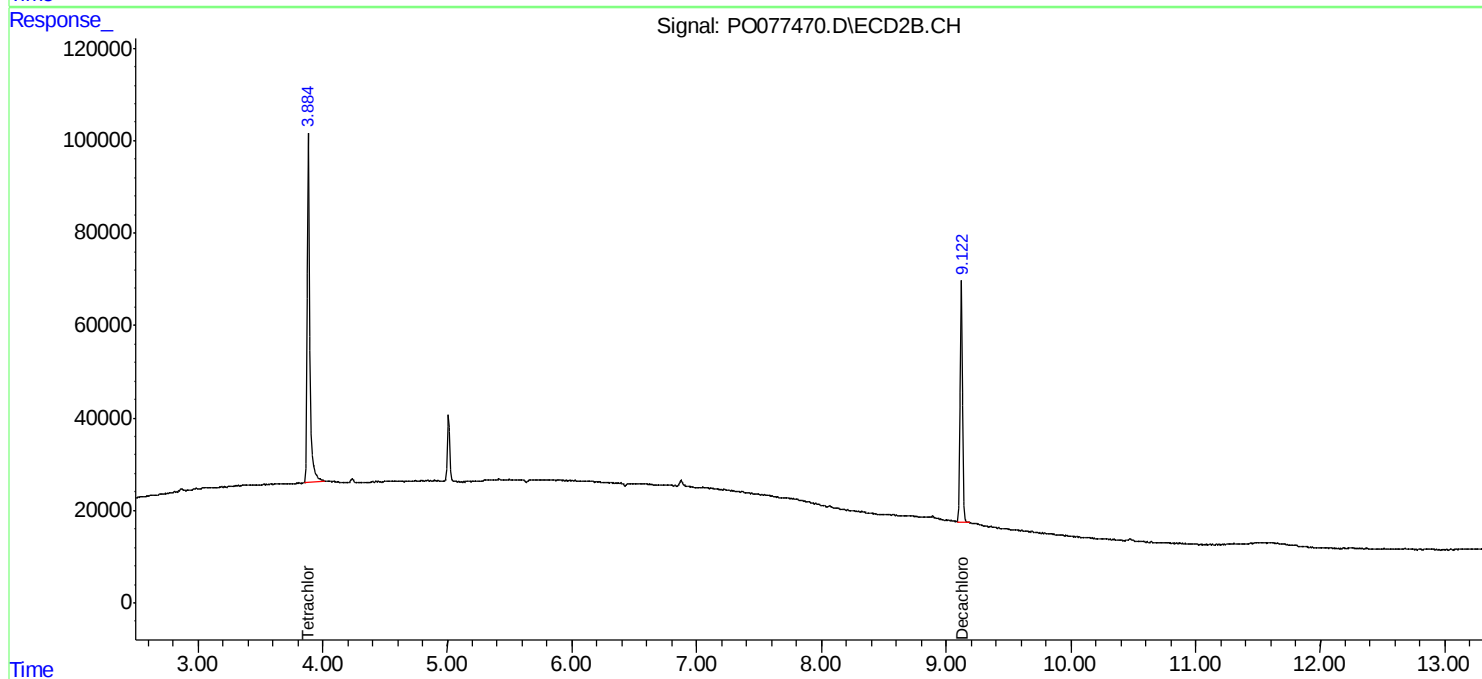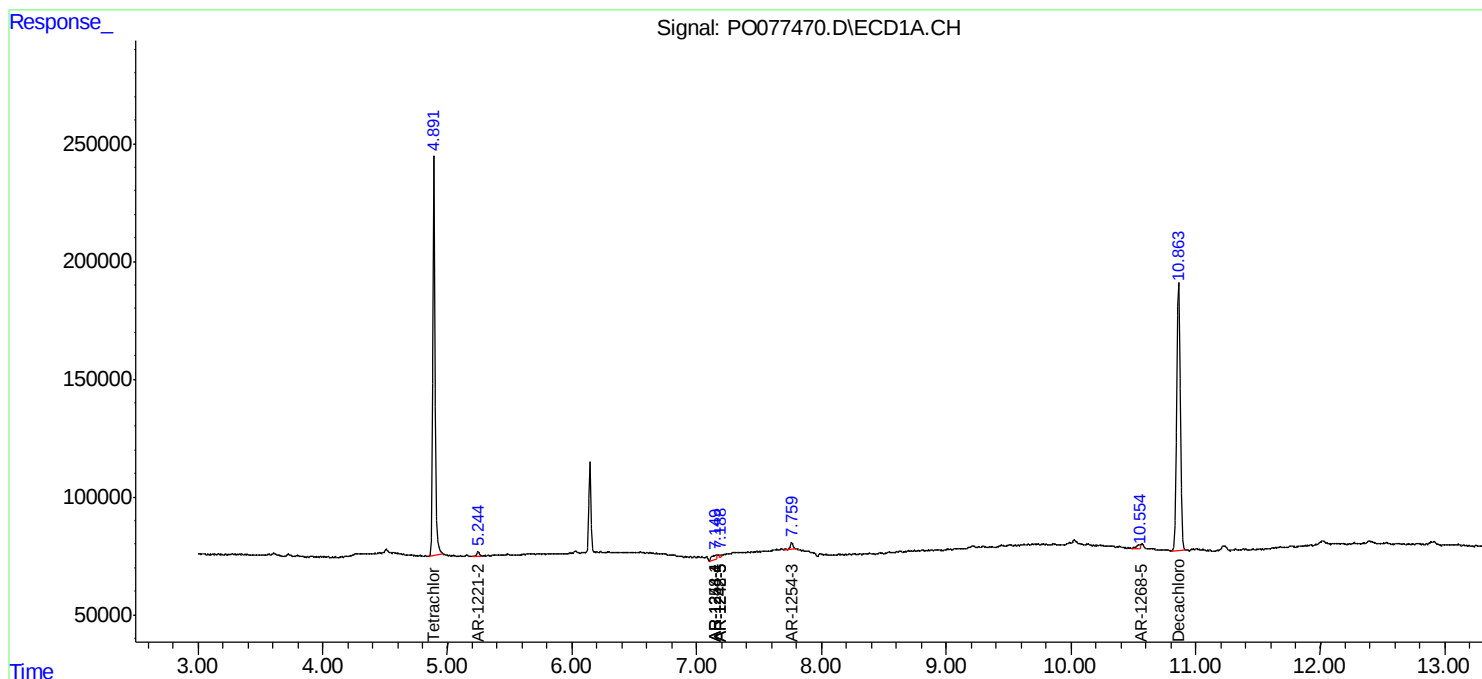


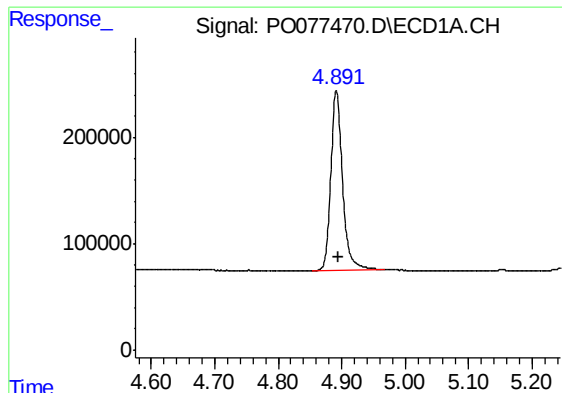

#1 Tetrachloro-m-xylene


R.T.: 4.892 min
Delta R.T.: -0.002 min
Response: 2171283
Conc: 19.79 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

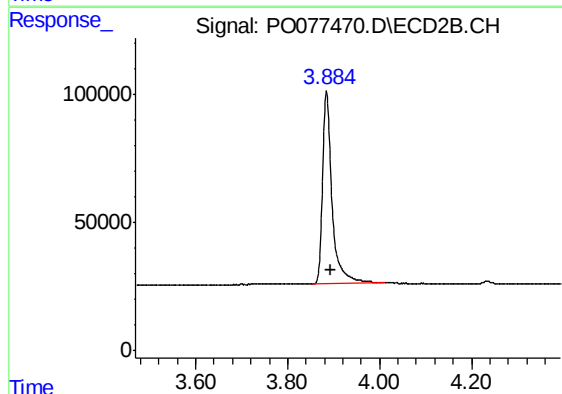


#1 Tetrachloro-m-xylene

R.T.: 3.885 min
Delta R.T.: -0.008 min
Response: 1080662
Conc: 19.36 ng/ml

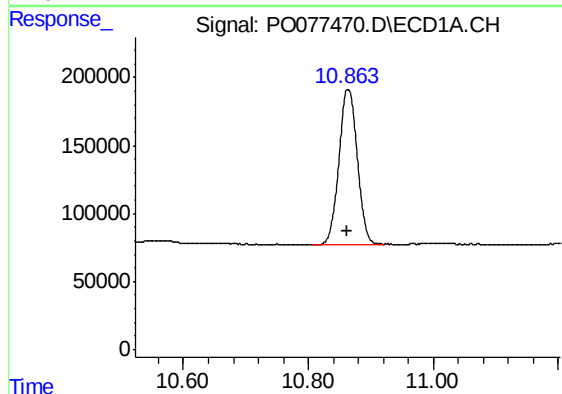


#2 Decachlorobiphenyl

R.T.: 10.863 min
Delta R.T.: 0.000 min
Response: 2334177
Conc: 21.23 ng/ml

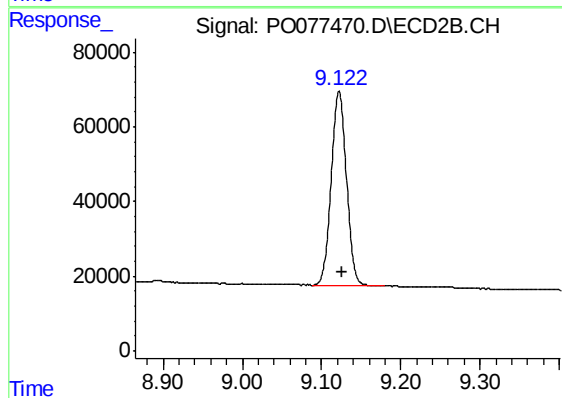

#2 Decachlorobiphenyl


R.T.: 9.122 min
Delta R.T.: -0.004 min
Response: 701996
Conc: 20.64 ng/ml

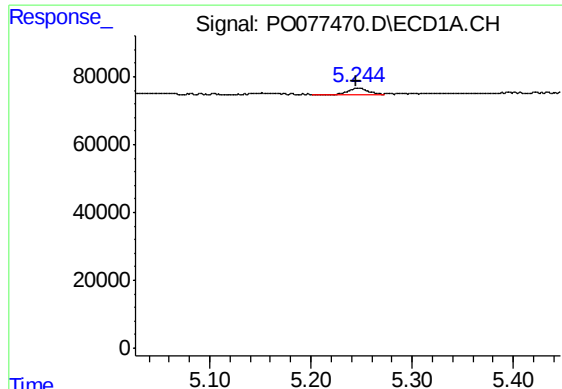

#9 AR-1221-2


R.T.: 5.246 min
Delta R.T.: 0.000 min
Response: 24437
Conc: 28.13 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

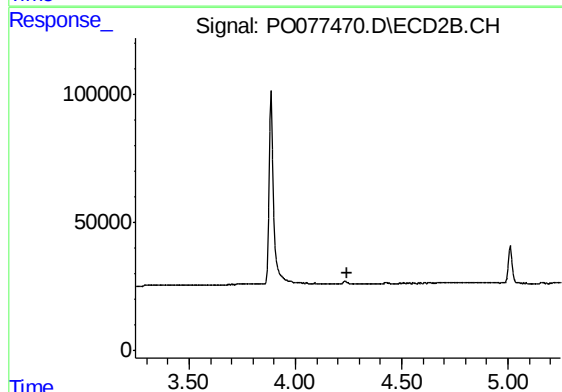


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 4.247 min
Response: 0
Conc: N.D.

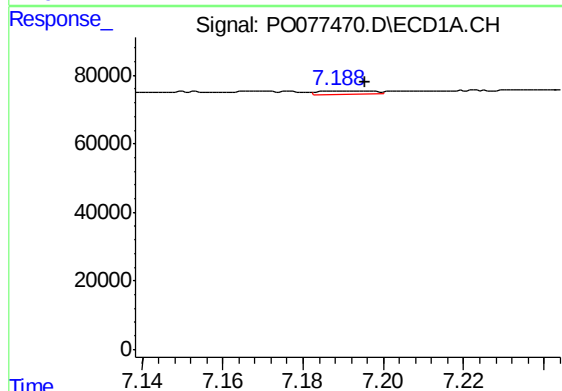


#20 AR-1242-5

R.T.: 7.188 min
Delta R.T.: -0.007 min
Response: 7268
Conc: 2.63 ng/ml

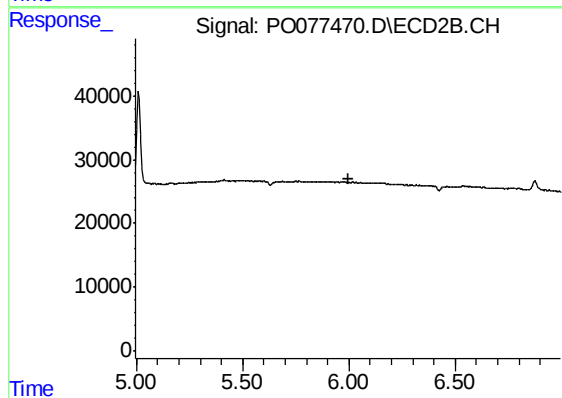

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T. : 5.996 min
Response: 0
Conc: N.D.

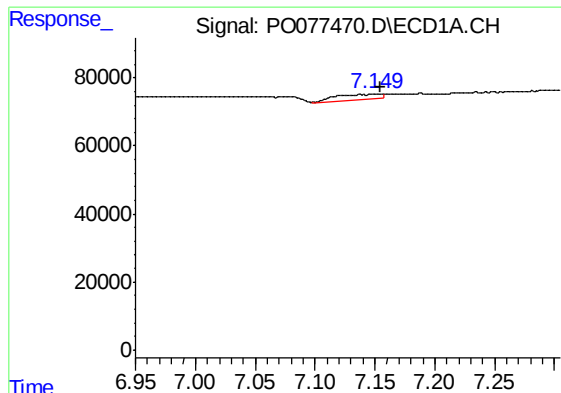

#24 AR-1248-4


R.T.: 7.150 min
Delta R.T.: -0.005 min
Response: 41420
Conc: 8.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

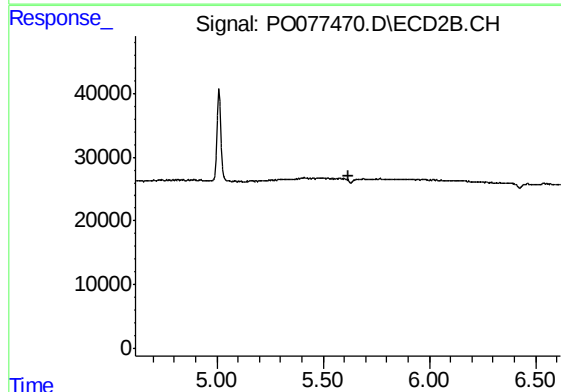


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.617 min
Response: 0
Conc: N.D.

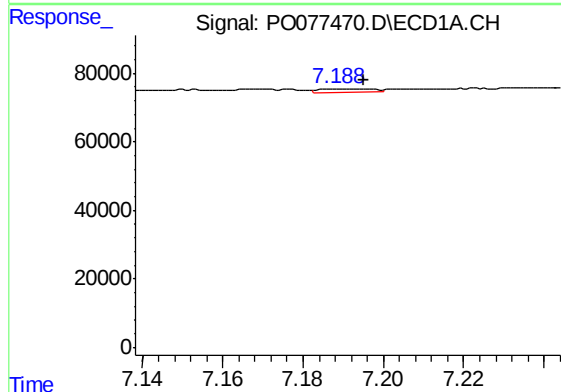


#25 AR-1248-5

R.T.: 7.188 min
Delta R.T.: -0.007 min
Response: 7268
Conc: 1.53 ng/ml

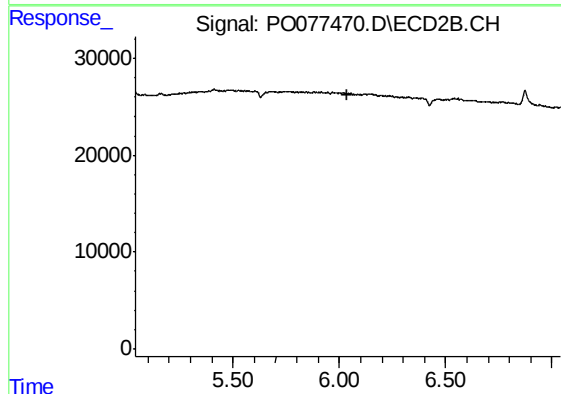

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T. : 6.040 min
Response: 0
Conc: N.D.

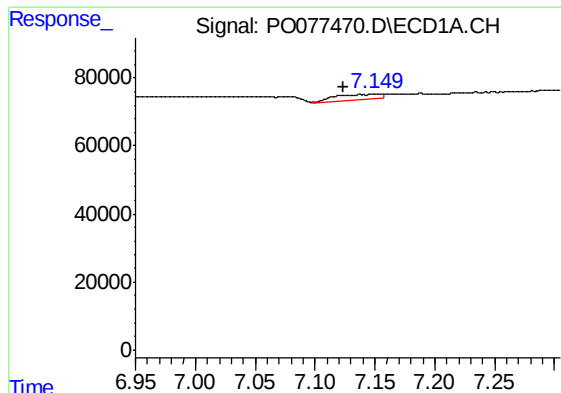

#26 AR-1254-1


R.T.: 7.150 min
Delta R.T.: 0.026 min
Response: 41420
Conc: 8.79 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

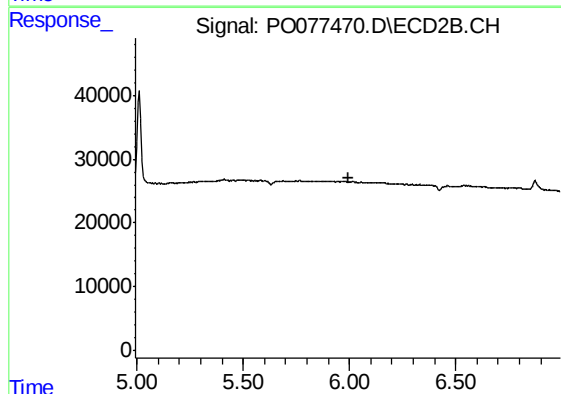


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T. : 5.993 min
Response: 0
Conc: N.D.

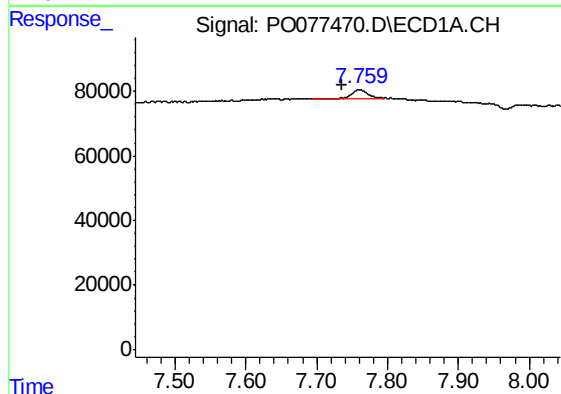


#28 AR-1254-3

R.T.: 7.759 min
Delta R.T.: 0.023 min
Response: 42503
Conc: 5.48 ng/ml

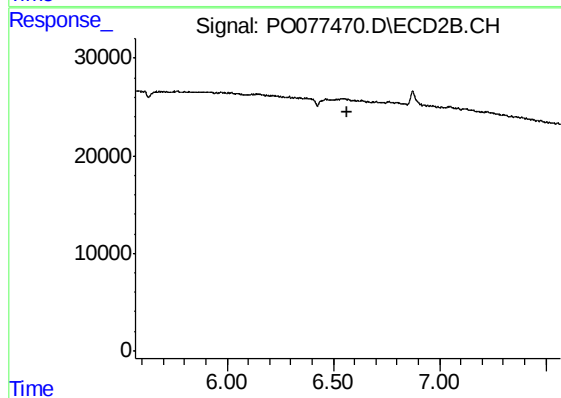

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 6.568 min
Response: 0
Conc: N.D.

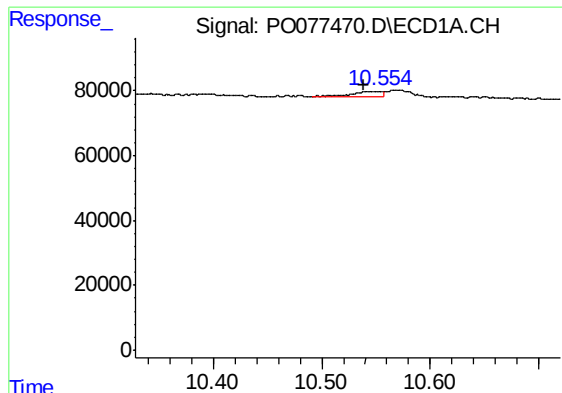

#45 AR-1268-5

R.T.: 10.554 min
Delta R.T.: 0.015 min
Response: 33376
Conc: 0.83 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

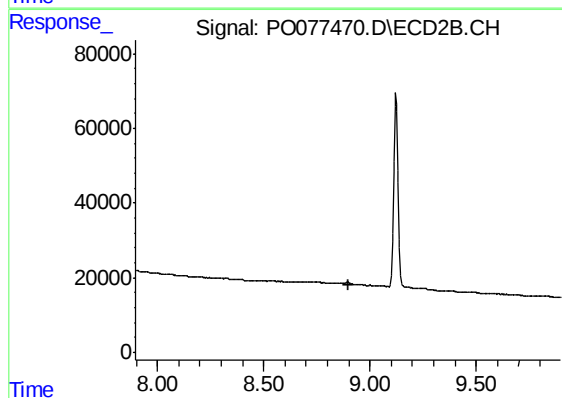

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 8.896 min
Response: 0
Conc: N.D.