

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0043021\
 Data File : P0077449.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Apr 2021 14:11
 Operator : AJ/MA
 Sample : M2224-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CL-01-042921

Manual Integrations
 APPROVED

Ankita
 5/3/2021 3:26:05 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 30 14:32:39 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Apr 29 05:54:04 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.890	3.884	2238503	1145034	20.399m	20.512
2) SA Decachlor...	10.865	9.123	2486574	693552	22.613	20.387

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0043021\
Data File : P0077449.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Apr 2021 14:11
Operator : AJ/MA
Sample : M2224-01
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
CL-01-042921


Manual Integrations
APPROVED

Ankita
5/3/2021 3:26:05 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 30 14:32:39 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042821.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Apr 29 05:54:04 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

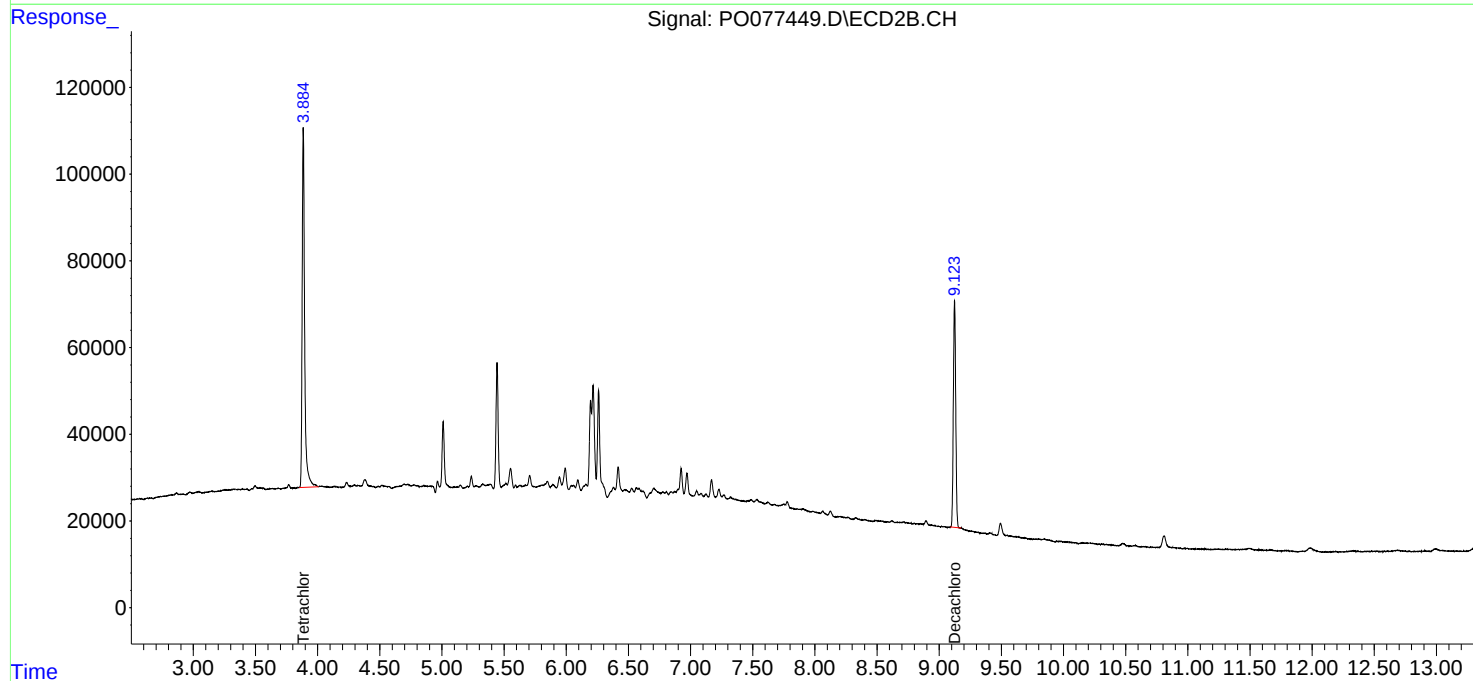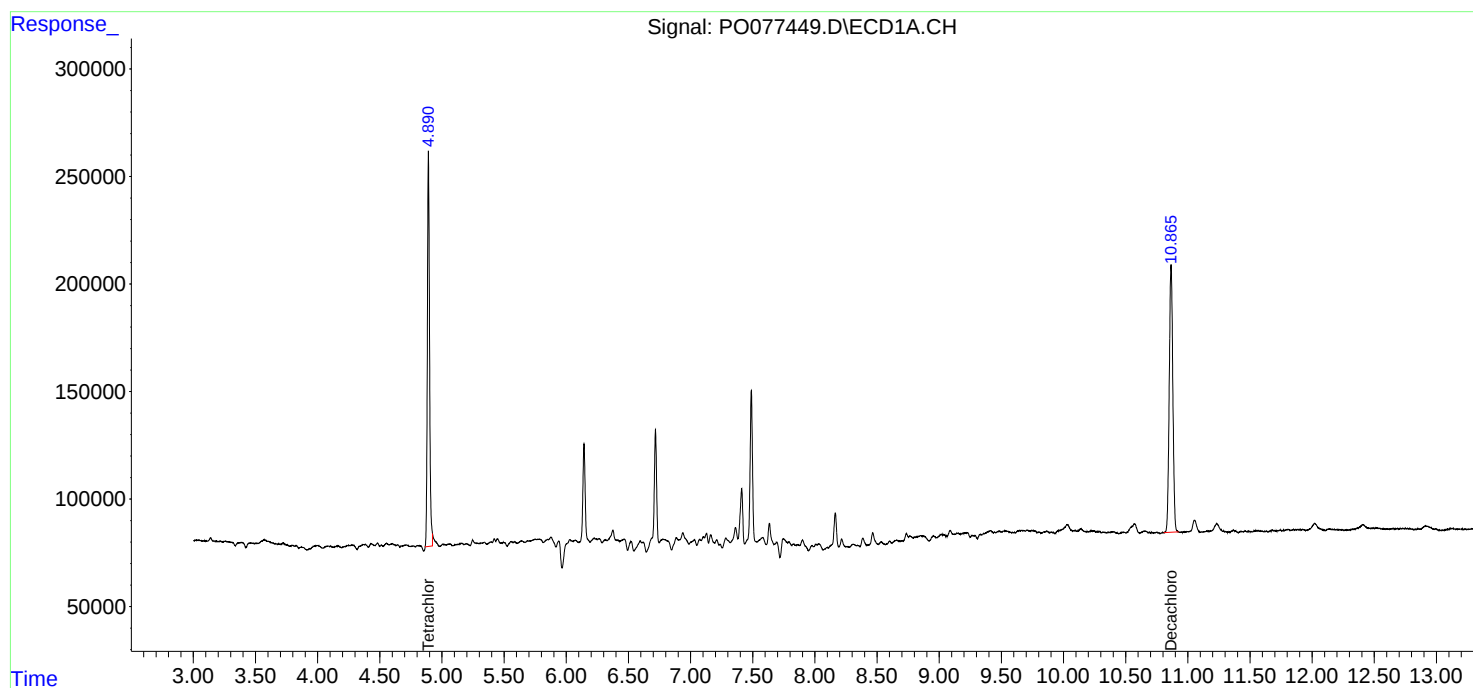

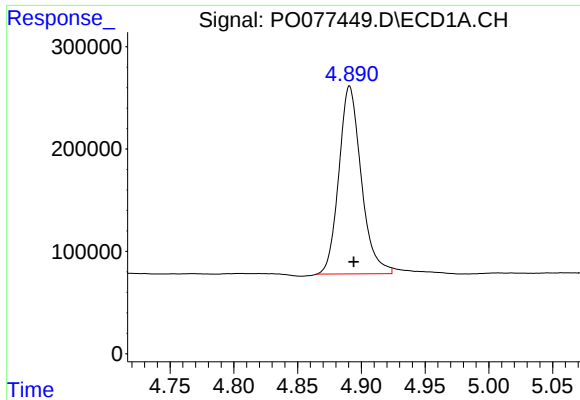


#1 Tetrachloro-m-xylene

R.T.: 4.890 min
Delta R.T.: -0.004 min
Response: 2238503
Conc: 20.40 ng/ml m

Instrument :
ECD_O
ClientSampleId :
CL-01-042921


Manual Integrations
APPROVED

Ankita
5/3/2021 3:26:05 PM

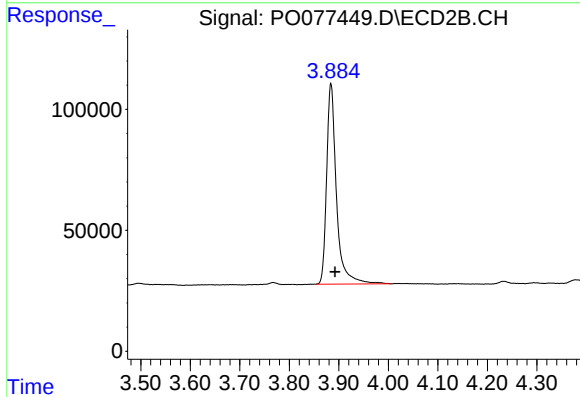


#1 Tetrachloro-m-xylene

R.T.: 3.884 min
Delta R.T.: -0.008 min
Response: 1145034
Conc: 20.51 ng/ml

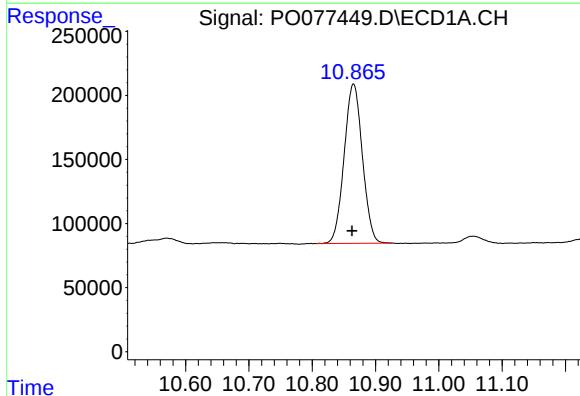

#2 Decachlorobiphenyl

R.T.: 10.865 min
Delta R.T.: 0.002 min
Response: 2486574
Conc: 22.61 ng/ml

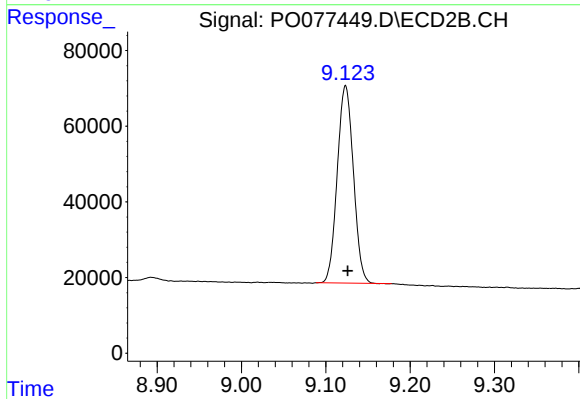

#2 Decachlorobiphenyl

R.T.: 9.123 min
Delta R.T.: -0.002 min
Response: 693552
Conc: 20.39 ng/ml