

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0043021\
 Data File : P0077451.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Apr 2021 14:45
 Operator : AJ/MA
 Sample : M2204-05
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ANTIFREEZE-1906

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 30 17:39:35 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Apr 29 05:54:04 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.893	3.886	1609055	816541	14.663	14.627
2)	SA Decachlor...	10.866	9.124	1145659	358371	10.419	10.535

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0043021\
Data File : P0077451.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Apr 2021 14:45
Operator : AJ/MA
Sample : M2204-05
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
ANTIFREEZE-1906

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 30 17:39:35 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042821.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Apr 29 05:54:04 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

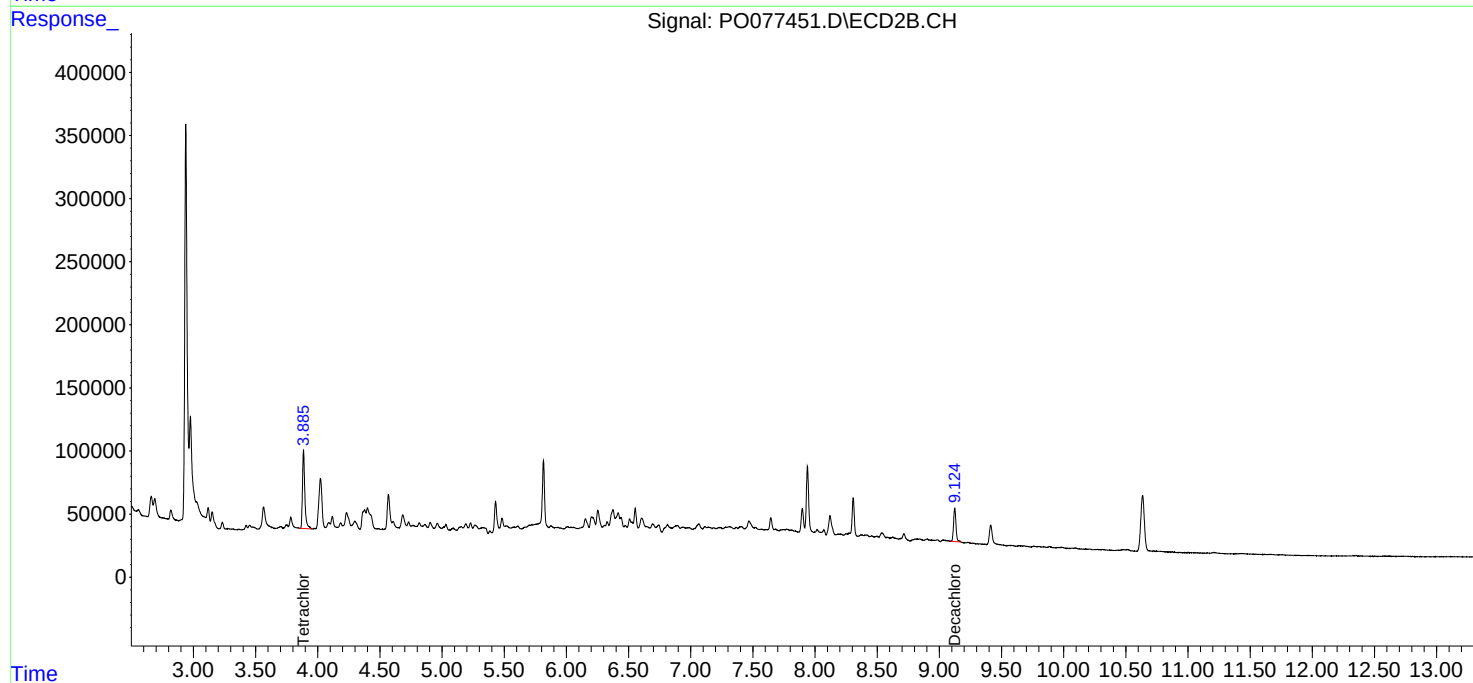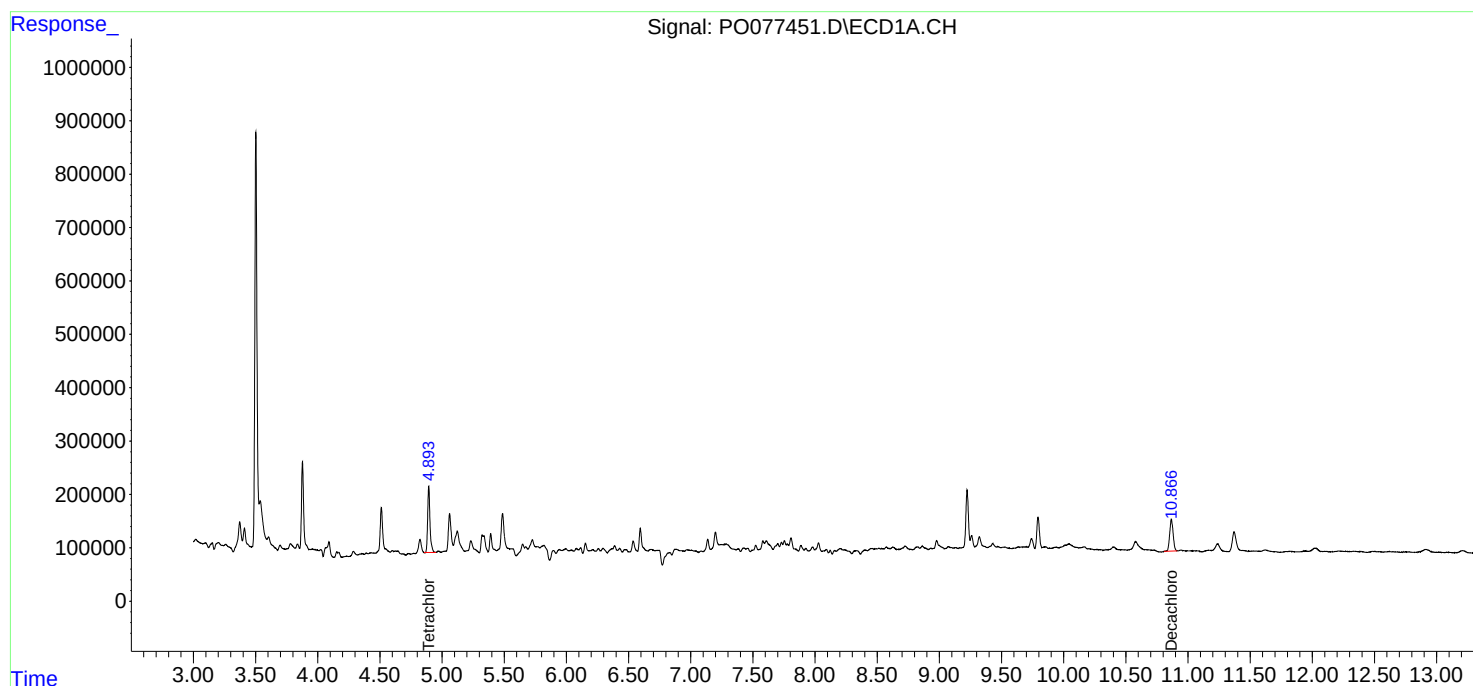


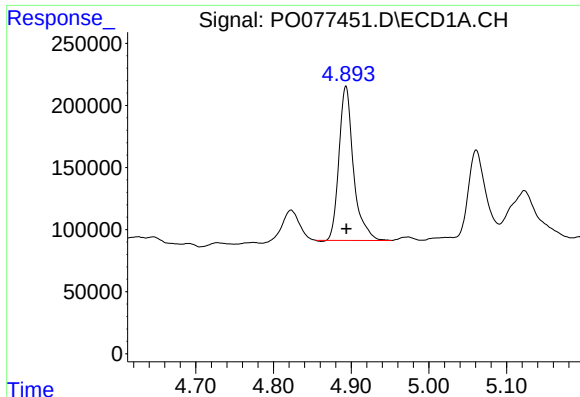

#1 Tetrachloro-m-xylene


R.T.: 4.893 min
Delta R.T.: 0.000 min
Response: 1609055
Conc: 14.66 ng/ml

Instrument :
ECD_O
ClientSampleId :
ANTIFREEZE-1906

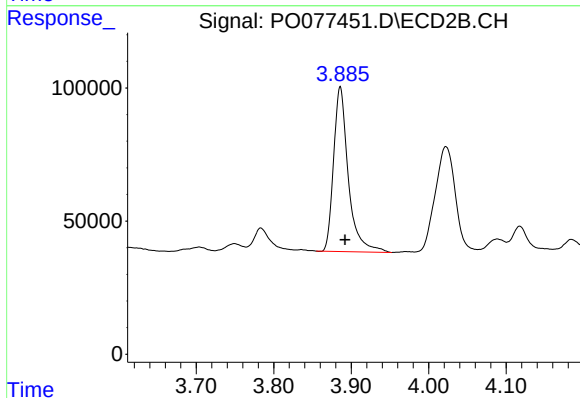


#1 Tetrachloro-m-xylene

R.T.: 3.886 min
Delta R.T.: -0.006 min
Response: 816541
Conc: 14.63 ng/ml

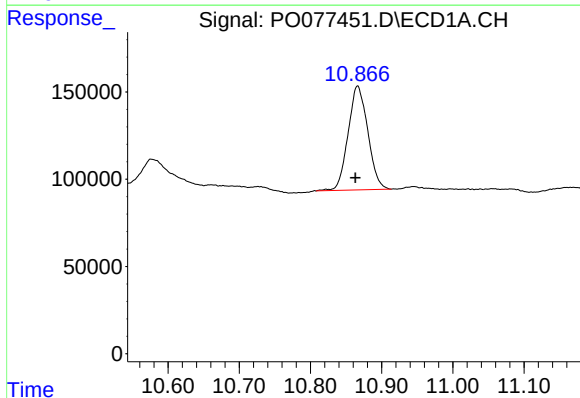

#2 Decachlorobiphenyl

R.T.: 10.866 min
Delta R.T.: 0.003 min
Response: 1145659
Conc: 10.42 ng/ml

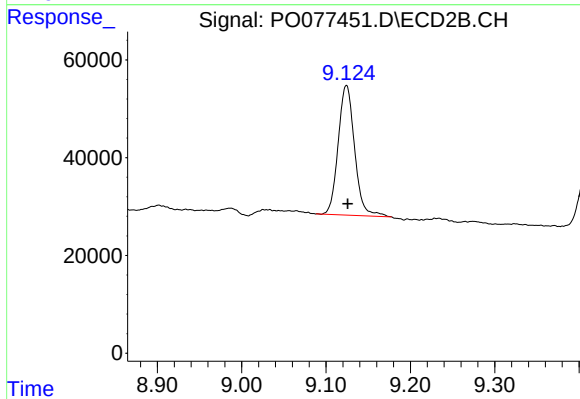

#2 Decachlorobiphenyl

R.T.: 9.124 min
Delta R.T.: -0.002 min
Response: 358371
Conc: 10.53 ng/ml