

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0050123\
 Data File : P0094619.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 May 2023 10:54
 Operator : YP/AJ
 Sample : AR1254ICC050
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1254ICC050

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/02/2023
 Supervised By :Ankita Jodhani 05/02/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 01 11:08:58 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042623.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon May 01 11:06:39 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.419	3.620	15960229	6153798	4.454	4.437
2) SA Decachlor...	10.270	8.641	11712679	5963944	4.718m	5.150
Target Compounds						
26) L6 AR-1254-1	6.463	5.505	5994204	3637833	46.471	49.668
27) L6 AR-1254-2	6.685	5.654	9540829	3377138	49.475	51.675
28) L6 AR-1254-3	7.056	6.057	9493711	5013903	50.252	50.018
29) L6 AR-1254-4	7.345	6.288	5210068	2297839	44.657	45.349
30) L6 AR-1254-5	7.769	6.707	6499519	4038212	45.203	46.769

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO050123\
Data File : PO094619.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 May 2023 10:54
Operator : YP/AJ
Sample : AR1254ICC050
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1254ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/02/2023
Supervised By :Ankita Jodhani 05/02/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 01 11:08:58 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO042623.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon May 01 11:06:39 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

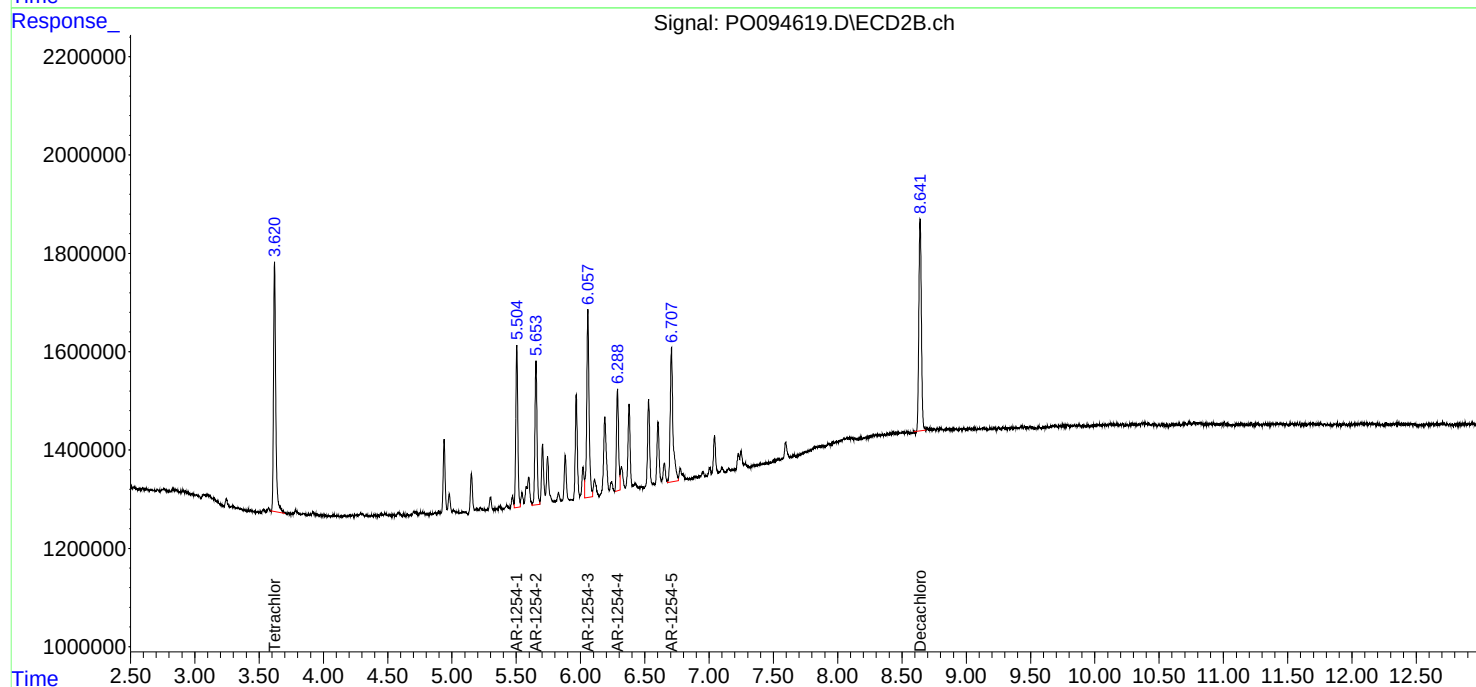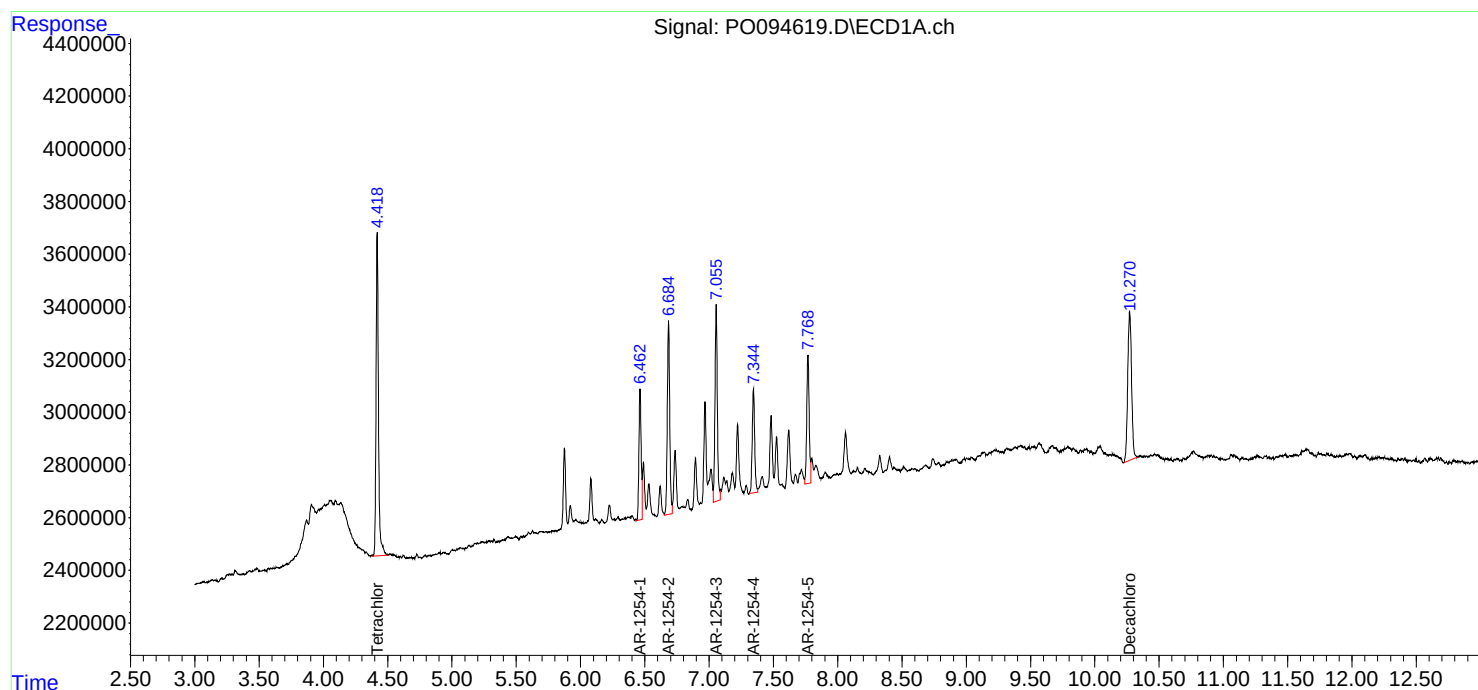

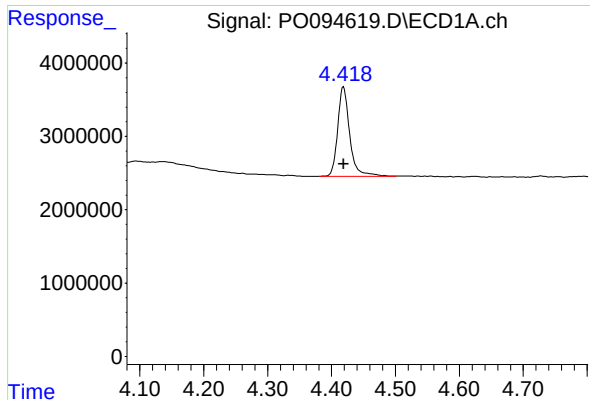


#1 Tetrachloro-m-xylene

R.T.: 4.419 min
Delta R.T.: 0.000 min
Response: 15960229
Conc: 4.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1254ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/02/2023
Supervised By :Ankita Jodhani 05/02/2023

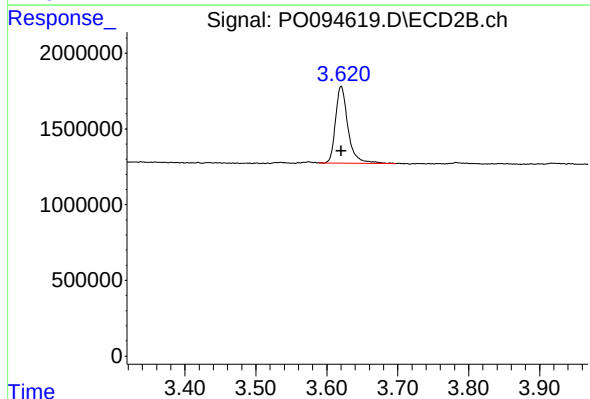


#1 Tetrachloro-m-xylene

R.T.: 3.620 min
Delta R.T.: 0.000 min
Response: 6153798
Conc: 4.44 ng/ml

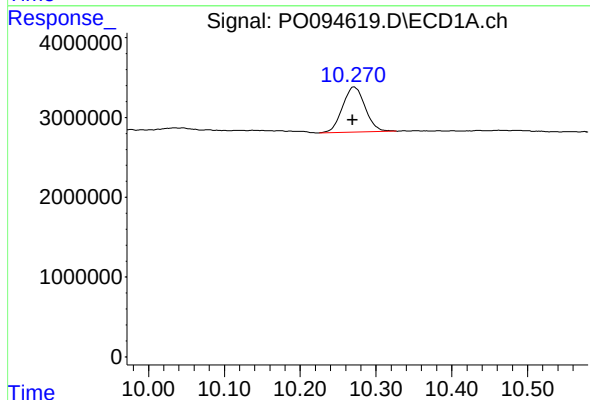


#2 Decachlorobiphenyl

R.T.: 10.270 min
Delta R.T.: 0.000 min
Response: 11712679
Conc: 4.72 ng/ml m

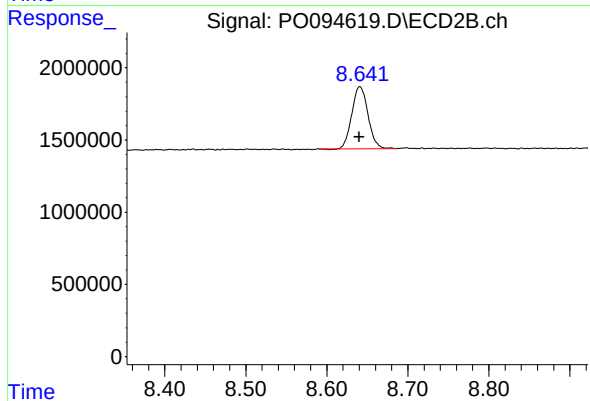

#2 Decachlorobiphenyl

R.T.: 8.641 min
Delta R.T.: 0.000 min
Response: 5963944
Conc: 5.15 ng/ml

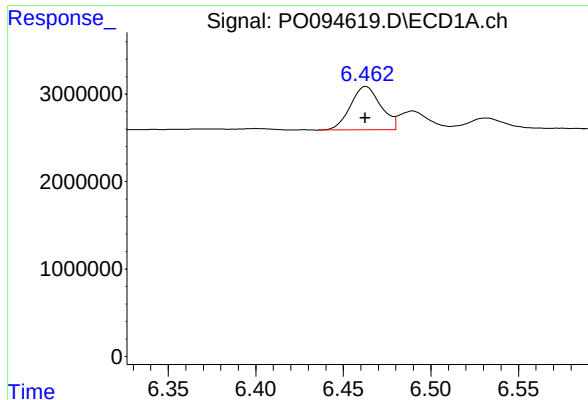


#26 AR-1254-1

R.T.: 6.463 min
Delta R.T.: 0.000 min
Response: 5994204
Conc: 46.47 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1254ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/02/2023
Supervised By :Ankita Jodhani 05/02/2023

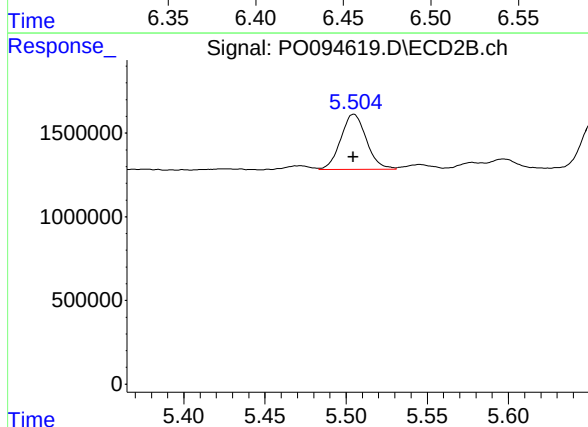


#26 AR-1254-1

R.T.: 5.505 min
Delta R.T.: 0.000 min
Response: 3637833
Conc: 49.67 ng/ml

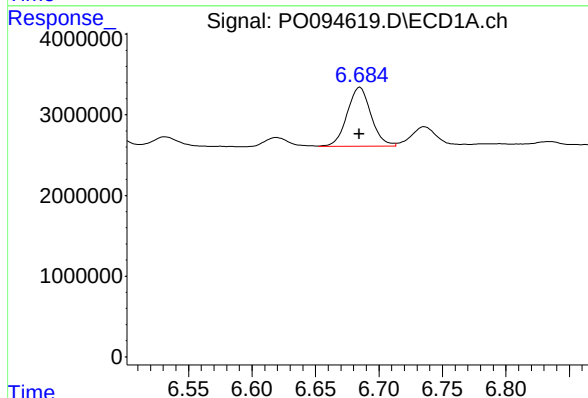


#27 AR-1254-2

R.T.: 6.685 min
Delta R.T.: 0.000 min
Response: 9540829
Conc: 49.47 ng/ml

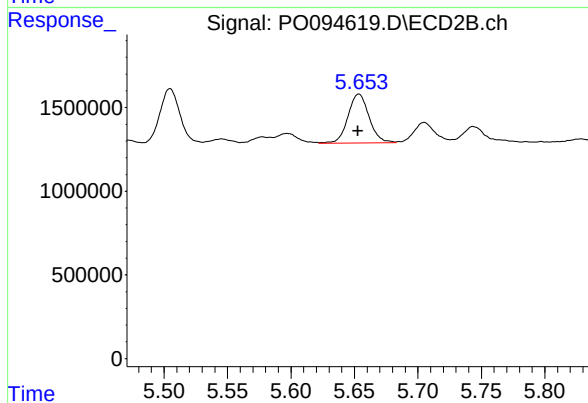

#27 AR-1254-2

R.T.: 5.654 min
Delta R.T.: 0.000 min
Response: 3377138
Conc: 51.67 ng/ml

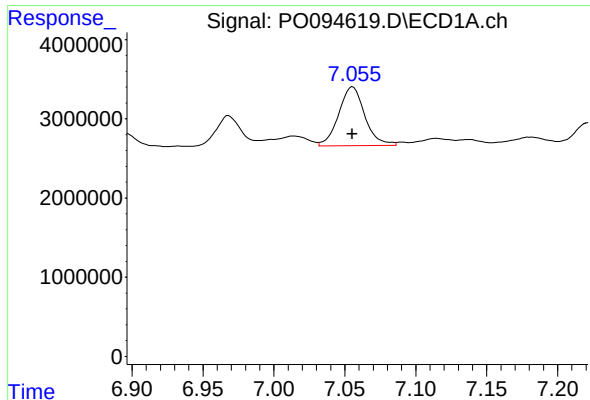


#28 AR-1254-3

R.T.: 7.056 min
Delta R.T.: 0.000 min
Response: 9493711
Conc: 50.25 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1254ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/02/2023
Supervised By :Ankita Jodhani 05/02/2023

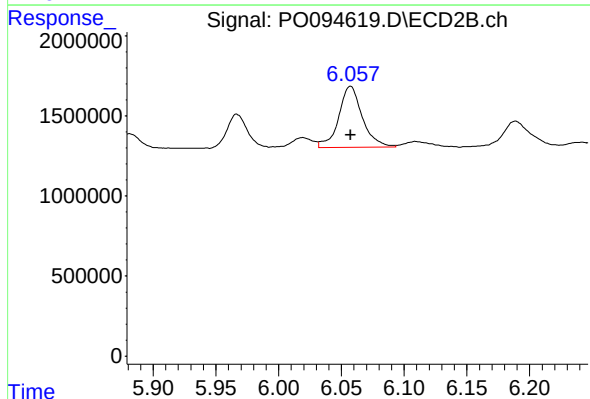


#28 AR-1254-3

R.T.: 6.057 min
Delta R.T.: 0.000 min
Response: 5013903
Conc: 50.02 ng/ml

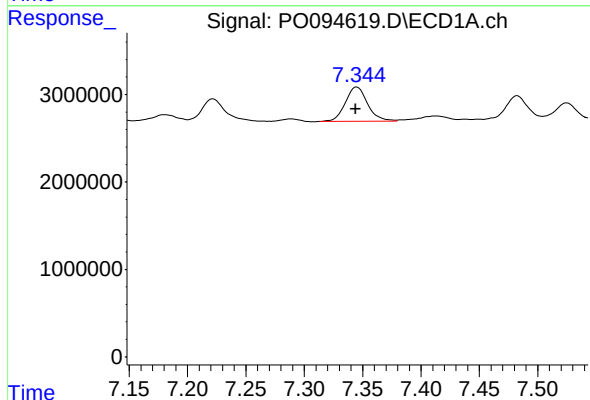


#29 AR-1254-4

R.T.: 7.345 min
Delta R.T.: 0.001 min
Response: 5210068
Conc: 44.66 ng/ml

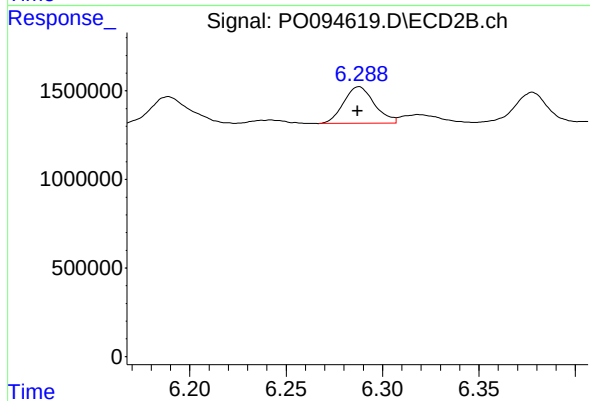

#29 AR-1254-4

R.T.: 6.288 min
Delta R.T.: 0.000 min
Response: 2297839
Conc: 45.35 ng/ml

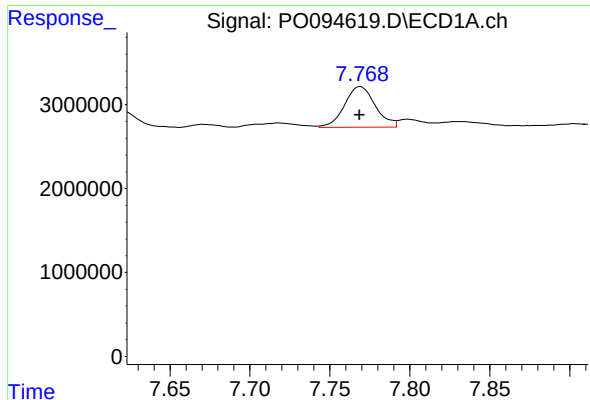


#30 AR-1254-5

R.T.: 7.769 min
Delta R.T.: 0.000 min
Response: 6499519
Conc: 45.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1254ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/02/2023
Supervised By :Ankita Jodhani 05/02/2023

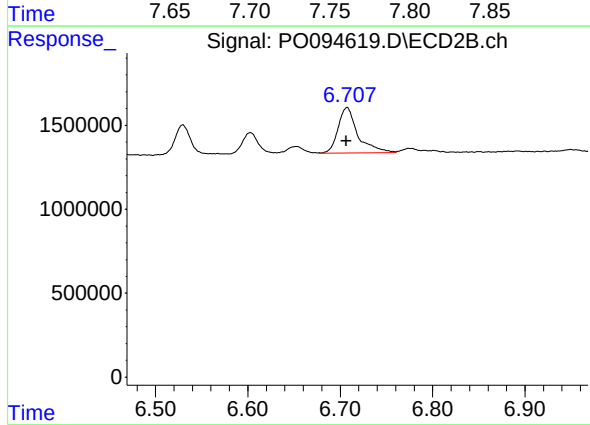

#30 AR-1254-5

R.T.: 6.707 min
Delta R.T.: 0.000 min
Response: 4038212
Conc: 46.77 ng/ml