

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0050123\
 Data File : P0094628.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 May 2023 13:27
 Operator : YP/AJ
 Sample : 02497-05
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 34558

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/02/2023
 Supervised By :Ankita Jodhani 05/02/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 01 21:31:23 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042623.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon May 01 11:12:50 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.438	3.621	25646789	21817544	7.445m	16.305 #
2) SA Decachlor...	10.257	8.640	1291324	7743658	0.532m	6.880m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO050123\
Data File : PO094628.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 May 2023 13:27
Operator : YP/AJ
Sample : 02497-05
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
34558


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/02/2023
Supervised By :Ankita Jodhani 05/02/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 01 21:31:23 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO042623.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon May 01 11:12:50 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

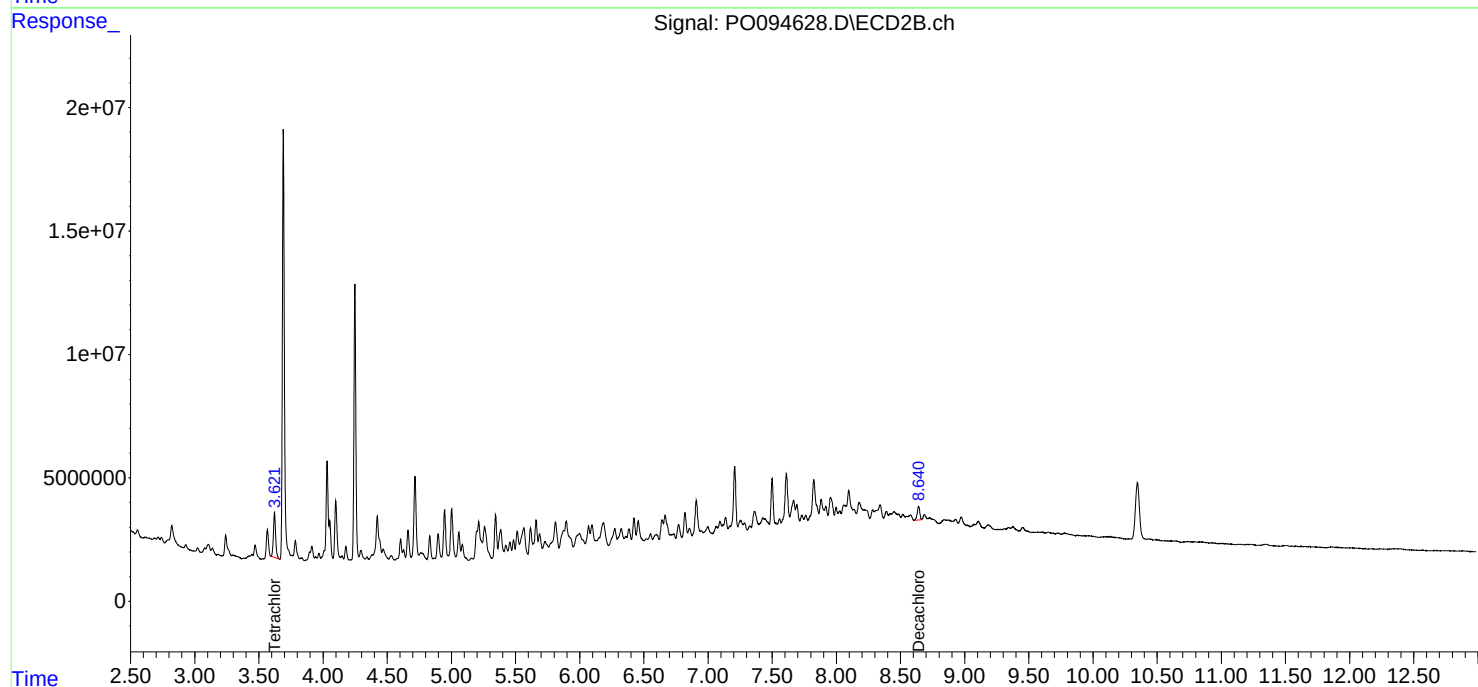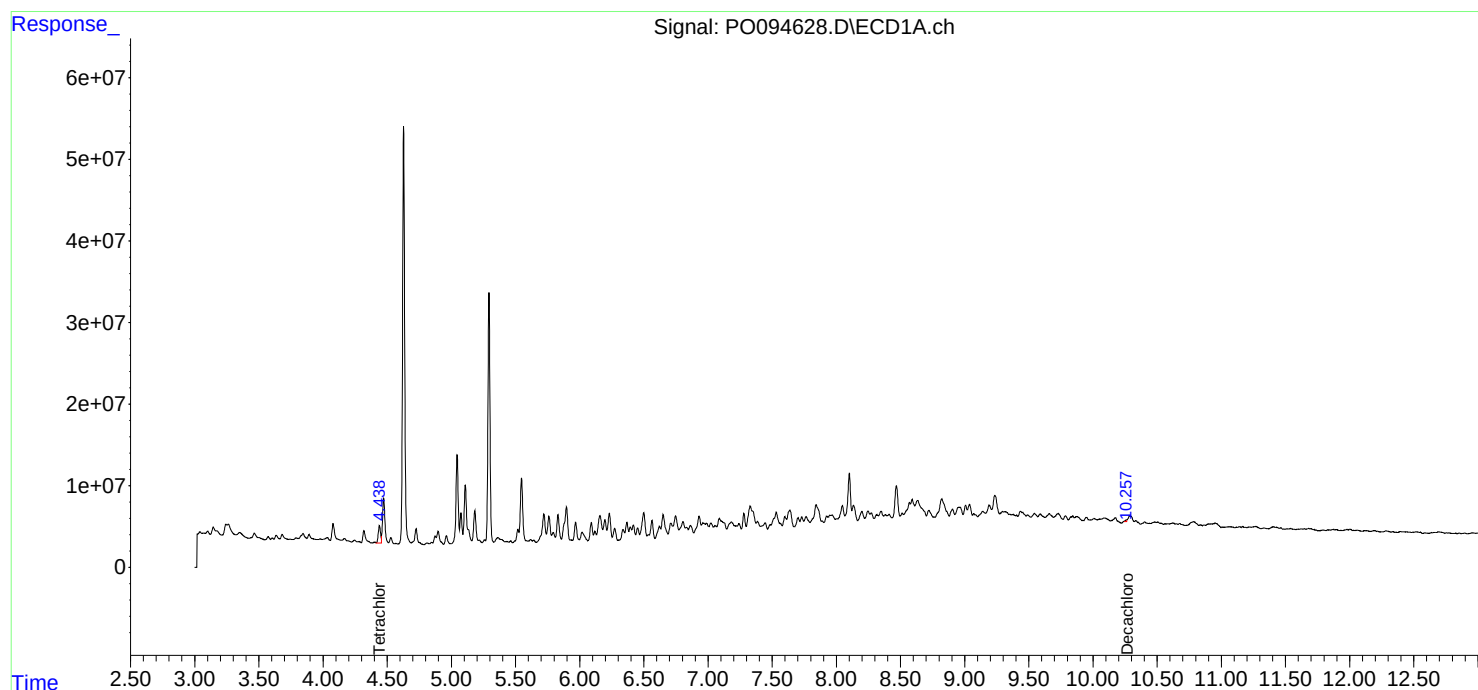

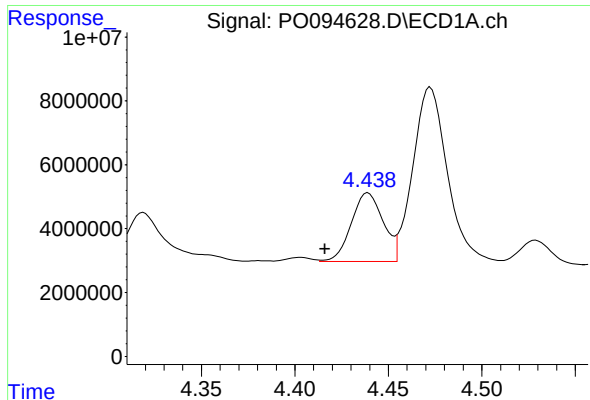


#1 Tetrachloro-m-xylene

R.T.: 4.438 min
Delta R.T.: 0.022 min
Response: 25646789
Conc: 7.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
34558


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/02/2023
Supervised By :Ankita Jodhani 05/02/2023

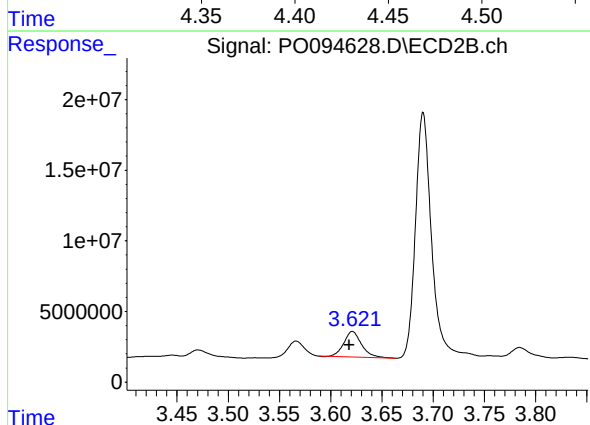


#1 Tetrachloro-m-xylene

R.T.: 3.621 min
Delta R.T.: 0.003 min
Response: 21817544
Conc: 16.31 ng/ml

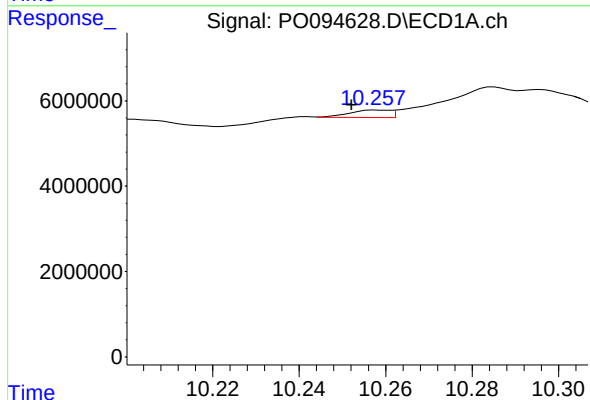

#2 Decachlorobiphenyl

R.T.: 10.257 min
Delta R.T.: 0.005 min
Response: 1291324
Conc: 0.53 ng/ml m

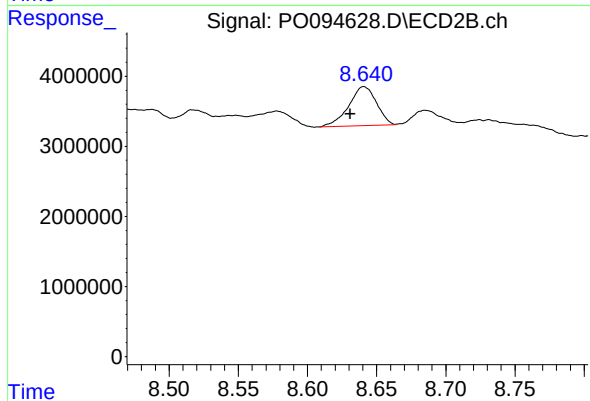

#2 Decachlorobiphenyl

R.T.: 8.640 min
Delta R.T.: 0.009 min
Response: 7743658
Conc: 6.88 ng/ml m