

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0050123\
 Data File : P0094657.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 May 2023 22:55
 Operator : YP/AJ
 Sample : 02523-10 10X
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 IRV-2023-14B

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/02/2023
 Supervised By :Ankita Jodhani 05/02/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 02 05:22:58 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042623.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon May 01 11:12:50 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.415	3.617	6047510	2336520	1.756m	1.746
2) SA Decachlor...	10.263	8.635	4542885	2177396	1.872m	1.934m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO050123\
Data File : PO094657.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 May 2023 22:55
Operator : YP/AJ
Sample : 02523-10 10X
Misc :
ALS Vial : 28 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
IRV-2023-14B


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/02/2023
Supervised By :Ankita Jodhani 05/02/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 02 05:22:58 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO042623.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon May 01 11:12:50 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

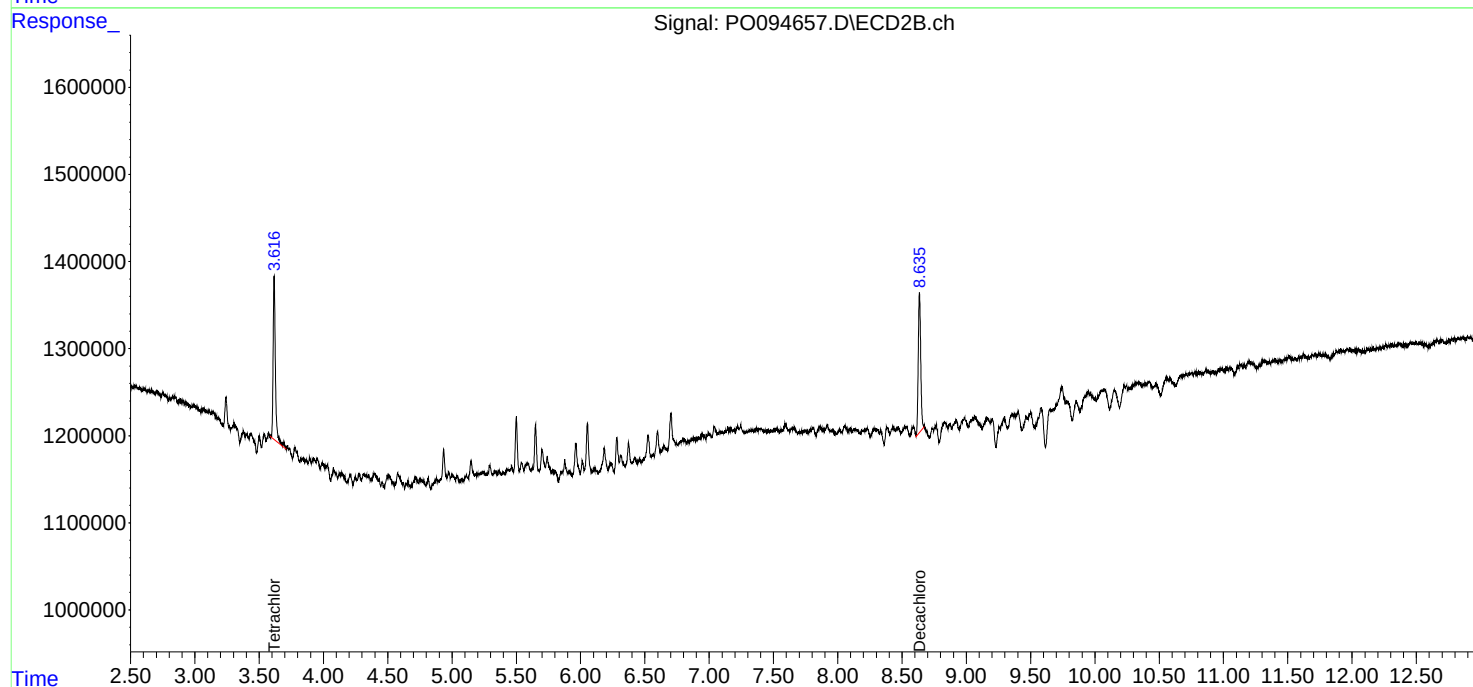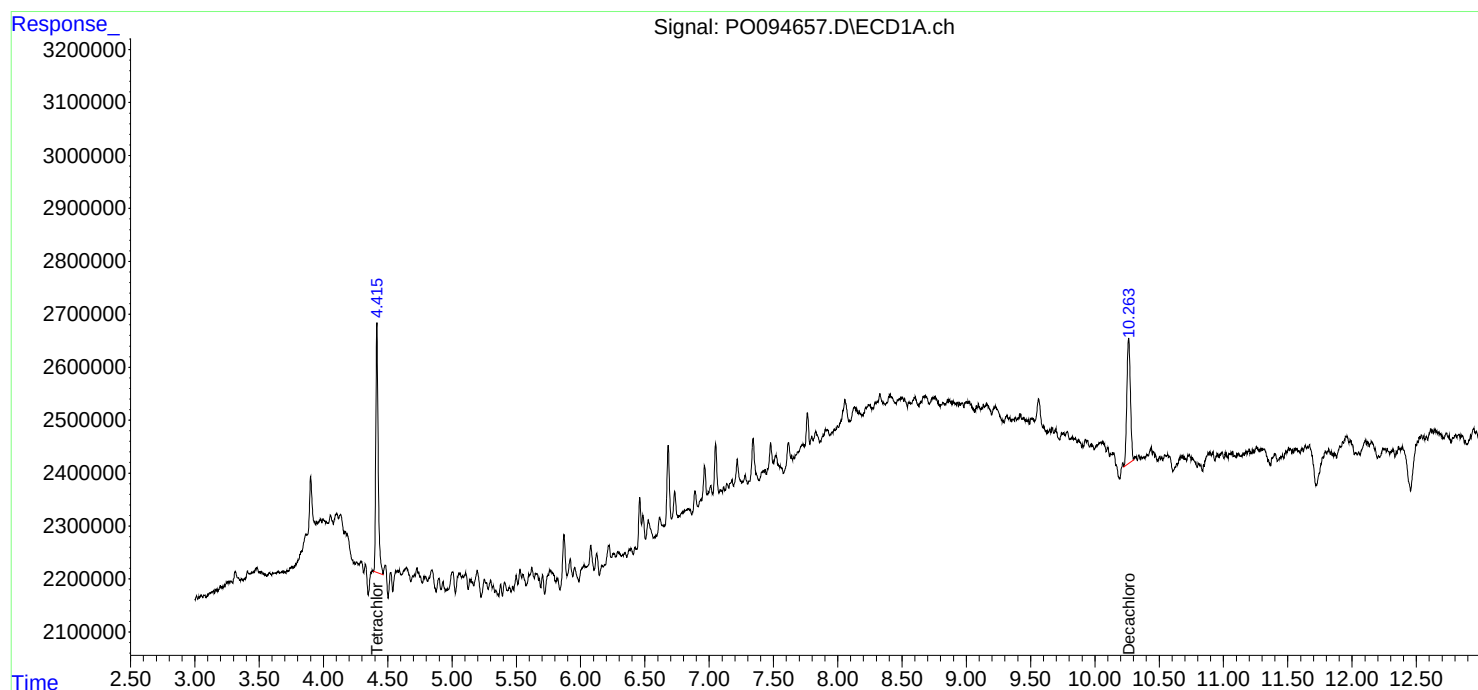

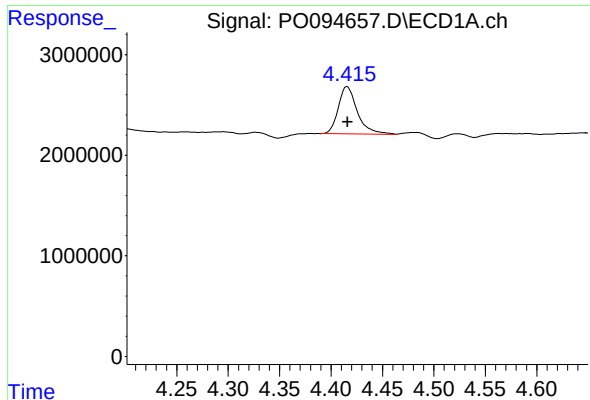


#1 Tetrachloro-m-xylene

R.T.: 4.415 min
Delta R.T.: -0.001 min
Response: 6047510
Conc: 1.76 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2023-14B


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/02/2023
Supervised By :Ankita Jodhani 05/02/2023

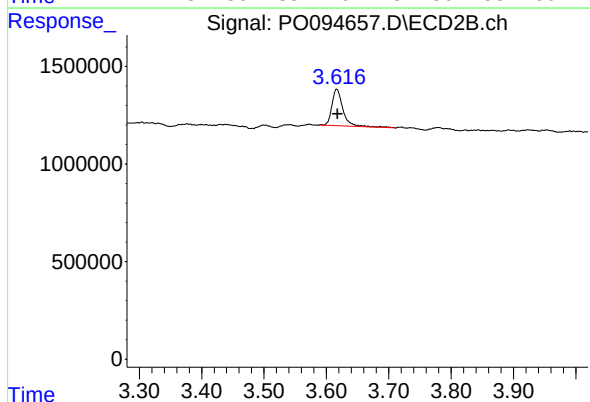


#1 Tetrachloro-m-xylene

R.T.: 3.617 min
Delta R.T.: -0.001 min
Response: 2336520
Conc: 1.75 ng/ml

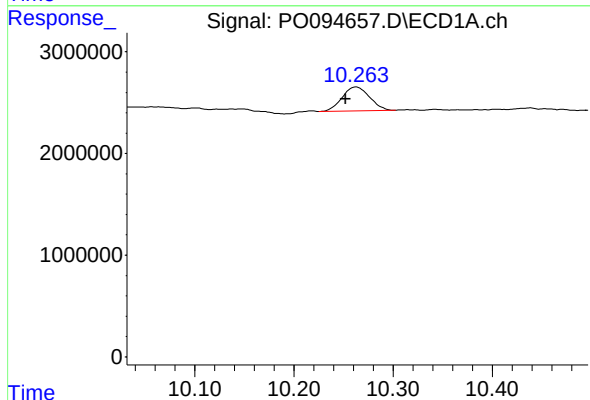

#2 Decachlorobiphenyl

R.T.: 10.263 min
Delta R.T.: 0.011 min
Response: 4542885
Conc: 1.87 ng/ml m

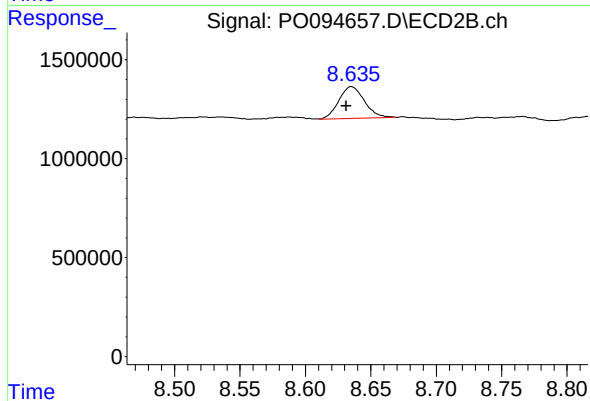

#2 Decachlorobiphenyl

R.T.: 8.635 min
Delta R.T.: 0.003 min
Response: 2177396
Conc: 1.93 ng/ml m