

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0050319\
 Data File : P0055824.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 May 2019 15:23
 Operator : SM/SJ
 Sample : AR1254ICV500
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ICVPO050319AR1254

Manual Integrations
 APPROVED

Ankita
 5/6/2019 9:56:01 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 03 16:26:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 03 15:20:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.278	3.592	1677338	1582415	56.050	56.028
2) SA Decachlor...	9.879	8.543	2021000	1550806	54.013	57.346m
Target Compounds						
26) L6 AR-1254-1	6.287	5.458	956370	1239531	455.451	463.147
27) L6 AR-1254-2	6.504	5.604	1509252	1124694	454.755	460.431
28) L6 AR-1254-3	6.869	6.005	1658721	1825556	456.254	460.115
29) L6 AR-1254-4	7.155	6.232	1254669	1245763	461.158	464.634
30) L6 AR-1254-5	7.571	6.646	1354501	1668065	472.590	460.959

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO050319\
Data File : PO055824.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 May 2019 15:23
Operator : SM/SJ
Sample : AR1254ICV500
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
ICVPO050319AR1254


Manual Integrations
APPROVED

Ankita
5/6/2019 9:56:01 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 03 16:26:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO050319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 03 15:20:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

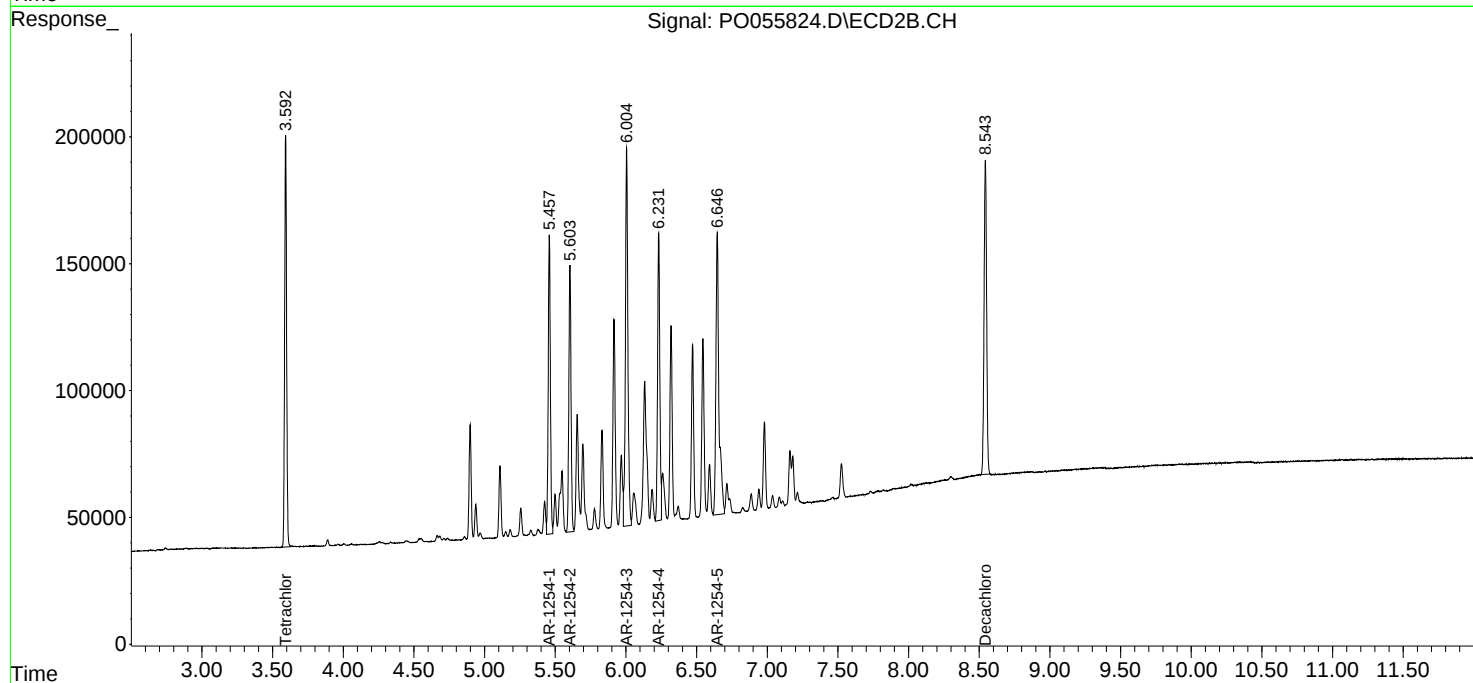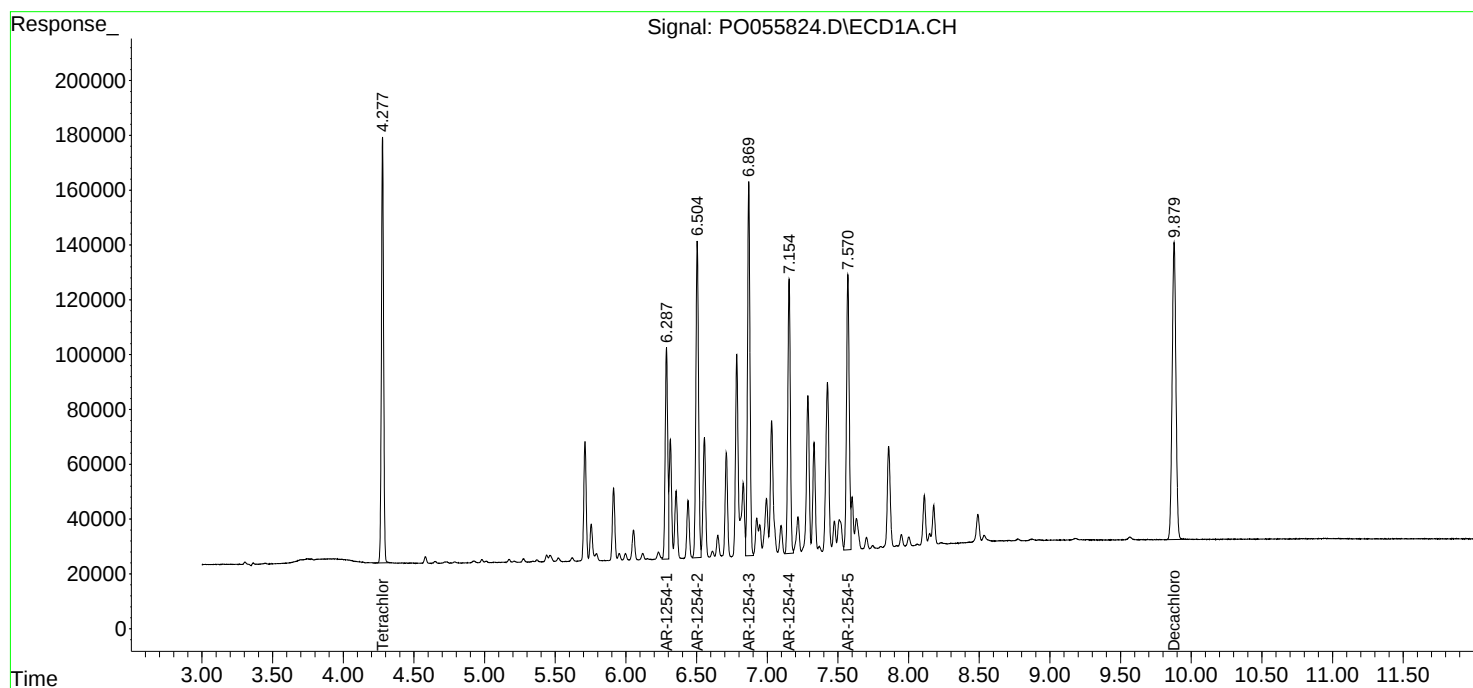

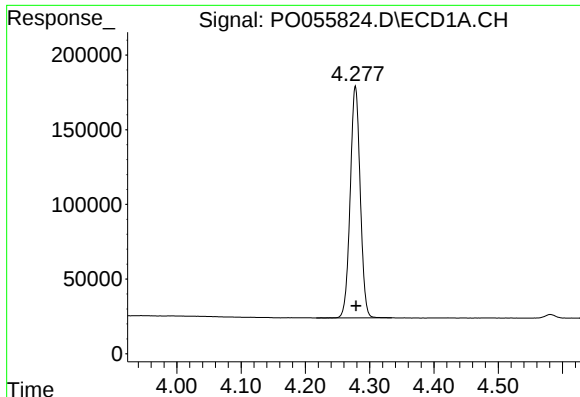


#1 Tetrachloro-m-xylene

R.T.: 4.278 min
Delta R.T.: -0.001 min
Response: 1677338
Conc: 56.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
ICVPO050319AR1254


Manual Integrations
APPROVED

Ankita
5/6/2019 9:56:01 AM

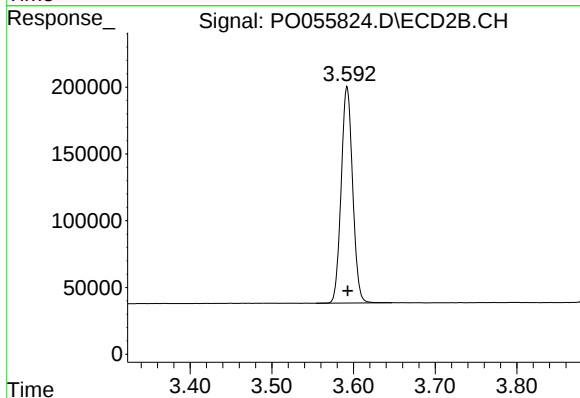


#1 Tetrachloro-m-xylene

R.T.: 3.592 min
Delta R.T.: 0.000 min
Response: 1582415
Conc: 56.03 ng/ml

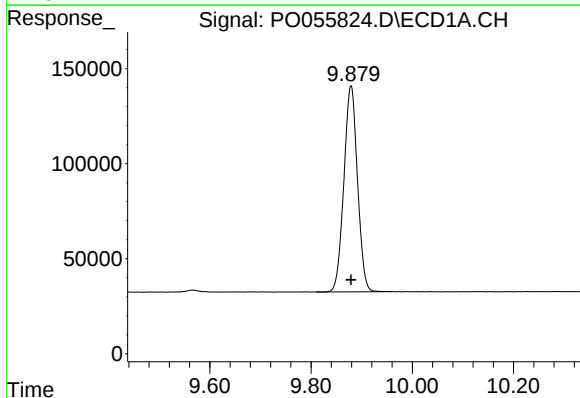


#2 Decachlorobiphenyl

R.T.: 9.879 min
Delta R.T.: 0.000 min
Response: 2021000
Conc: 54.01 ng/ml

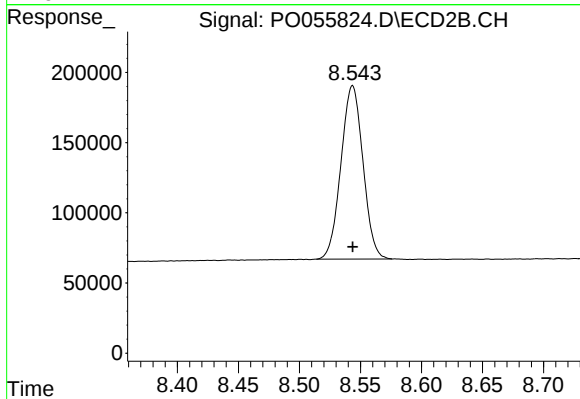

#2 Decachlorobiphenyl

R.T.: 8.543 min
Delta R.T.: 0.000 min
Response: 1550806
Conc: 57.35 ng/ml m

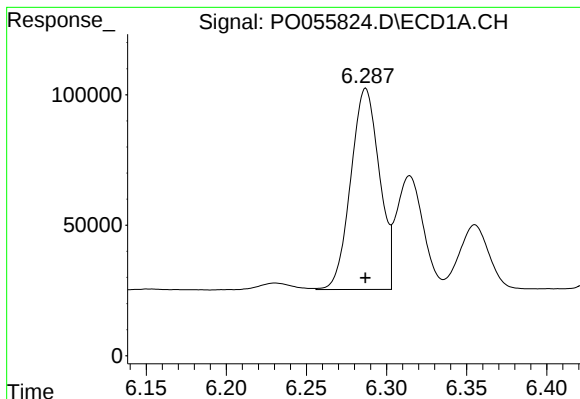


#26 AR-1254-1

R.T.: 6.287 min
Delta R.T.: 0.000 min
Response: 956370
Conc: 455.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
ICVPO050319AR1254


Manual Integrations
APPROVED

Ankita
5/6/2019 9:56:01 AM

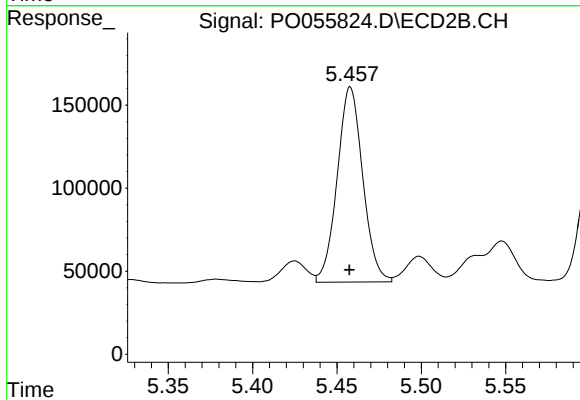


#26 AR-1254-1

R.T.: 5.458 min
Delta R.T.: 0.000 min
Response: 1239531
Conc: 463.15 ng/ml

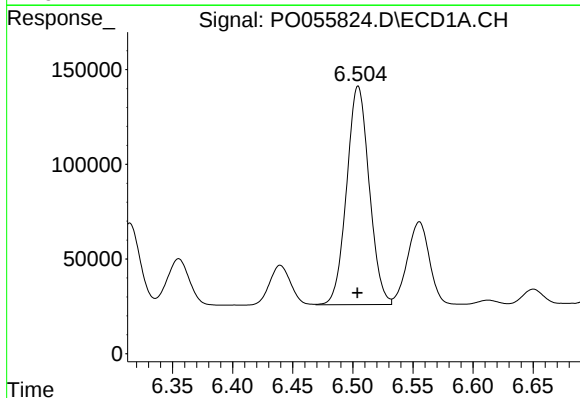


#27 AR-1254-2

R.T.: 6.504 min
Delta R.T.: 0.000 min
Response: 1509252
Conc: 454.75 ng/ml

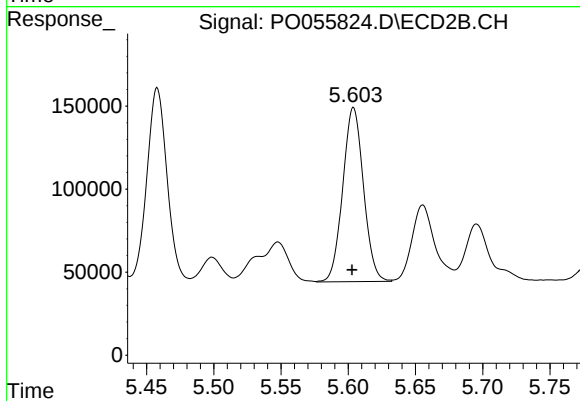

#27 AR-1254-2

R.T.: 5.604 min
Delta R.T.: 0.001 min
Response: 1124694
Conc: 460.43 ng/ml

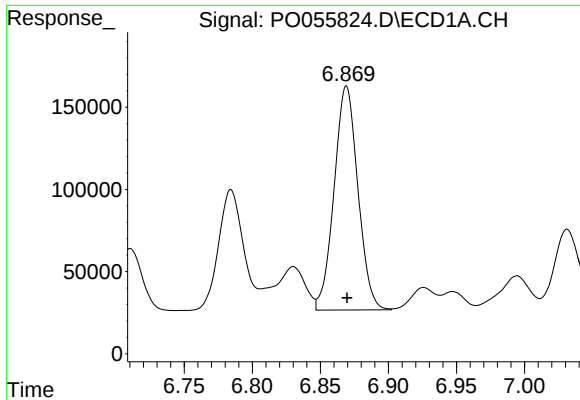


#28 AR-1254-3

R.T.: 6.869 min
Delta R.T.: 0.000 min
Response: 1658721
Conc: 456.25 ng/ml

Instrument :
ECD_O
ClientSampleId :
ICVPO050319AR1254


Manual Integrations
APPROVED

Ankita
5/6/2019 9:56:01 AM

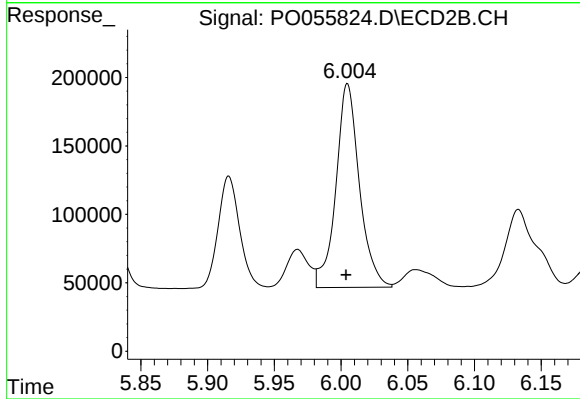


#28 AR-1254-3

R.T.: 6.005 min
Delta R.T.: 0.001 min
Response: 1825556
Conc: 460.11 ng/ml

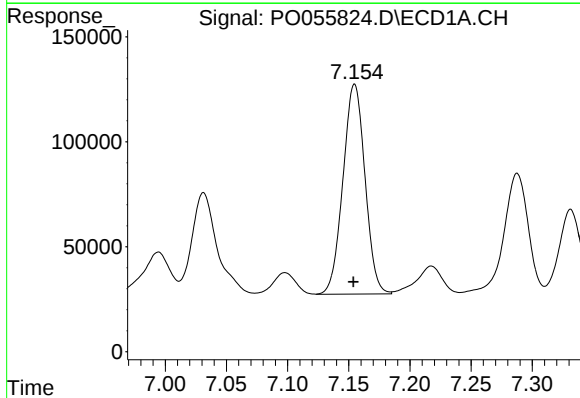


#29 AR-1254-4

R.T.: 7.155 min
Delta R.T.: 0.000 min
Response: 1254669
Conc: 461.16 ng/ml

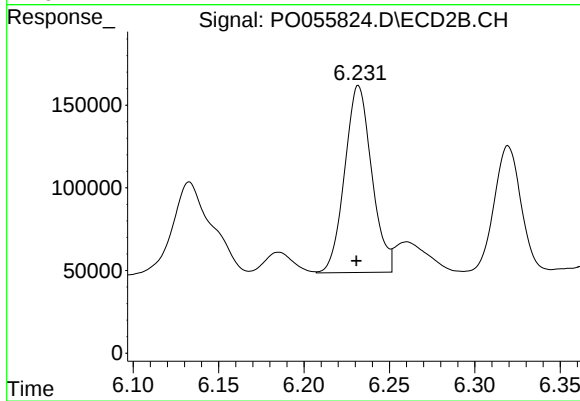

#29 AR-1254-4

R.T.: 6.232 min
Delta R.T.: 0.001 min
Response: 1245763
Conc: 464.63 ng/ml

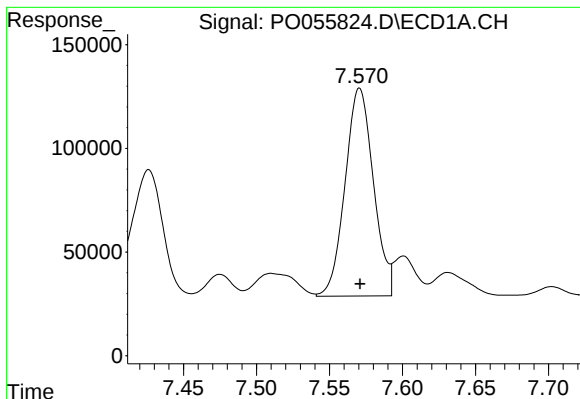


#30 AR-1254-5

R.T.: 7.571 min
Delta R.T.: 0.000 min
Response: 1354501
Conc: 472.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
ICVPO050319AR1254

Manual Integrations
APPROVED

Ankita
5/6/2019 9:56:01 AM

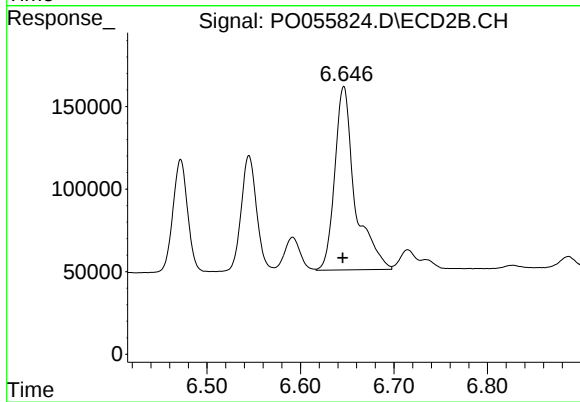

#30 AR-1254-5

R.T.: 6.646 min
Delta R.T.: 0.001 min
Response: 1668065
Conc: 460.96 ng/ml