

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0050319\
 Data File : P0055837.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 May 2019 19:24
 Operator : SM/SJ
 Sample : K2538-06 10X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 NB-20523

Manual Integrations
 APPROVED

Ankita
 5/6/2019 9:56:15 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 03 22:57:02 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 03 15:20:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.280	3.590	67347	109573	2.250m	3.880m#
2) SA Decachlor...	9.833	8.543	91919	76629	2.457	2.834m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO050319\
Data File : PO055837.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 May 2019 19:24
Operator : SM/SJ
Sample : K2538-06 10X
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
NB-20523


Manual Integrations
APPROVED

Ankita
5/6/2019 9:56:15 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 03 22:57:02 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO050319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 03 15:20:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

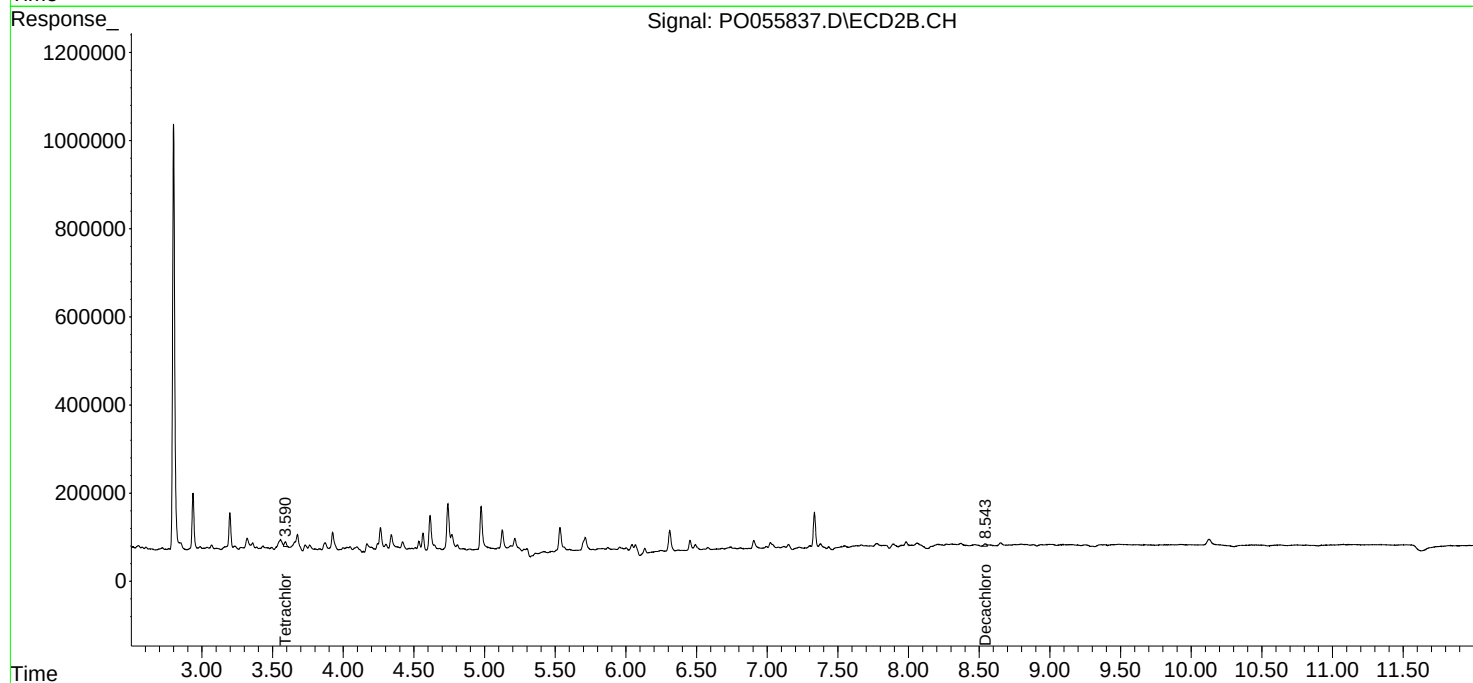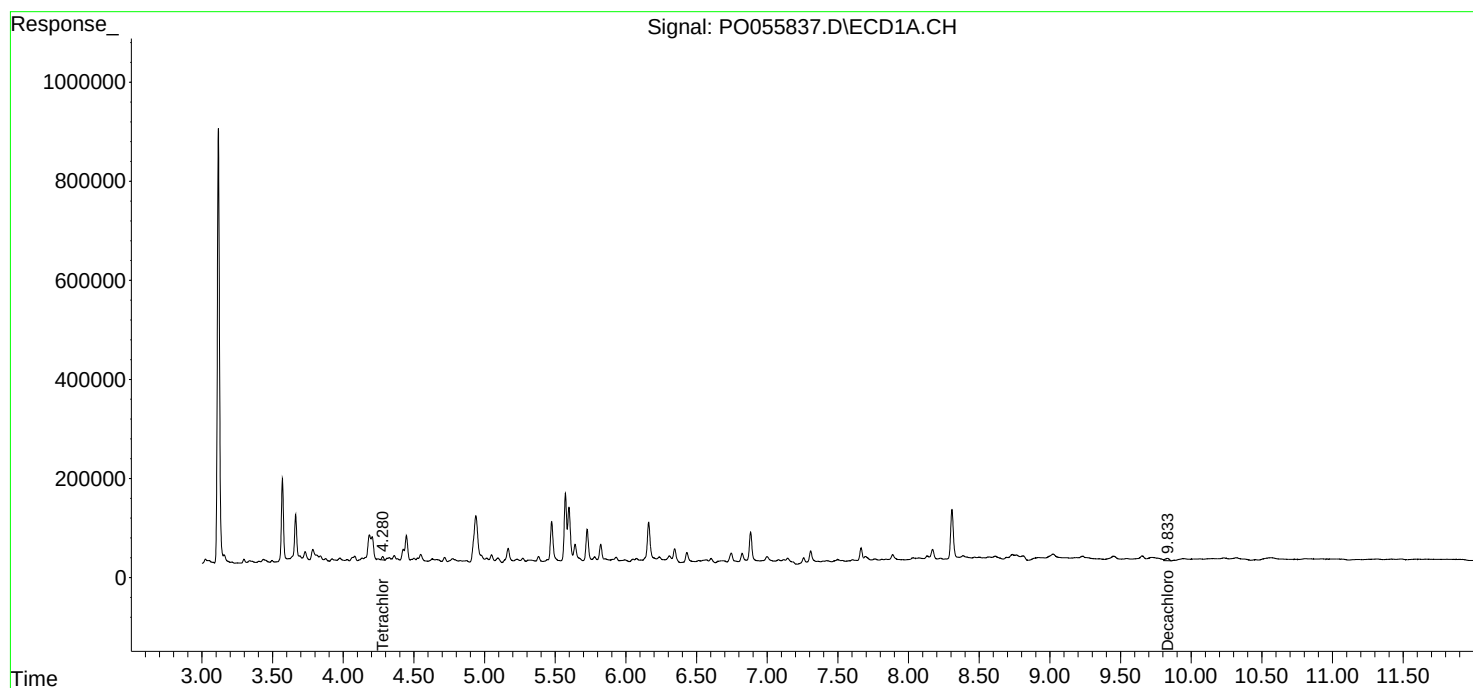

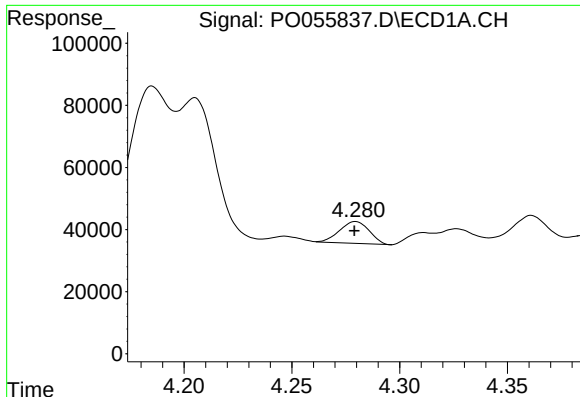


#1 Tetrachloro-m-xylene

R.T.: 4.280 min
Delta R.T.: 0.000 min
Response: 67347
Conc: 2.25 ng/ml m

Instrument :
ECD_O
ClientSampleId :
NB-20523


Manual Integrations
APPROVED

Ankita
5/6/2019 9:56:15 AM

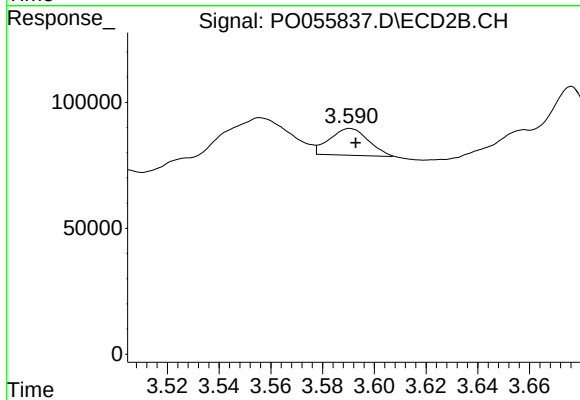


#1 Tetrachloro-m-xylene

R.T.: 3.590 min
Delta R.T.: -0.003 min
Response: 109573
Conc: 3.88 ng/ml m

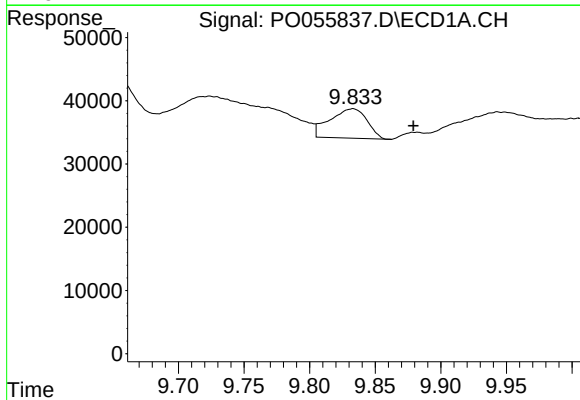

#2 Decachlorobiphenyl

R.T.: 9.833 min
Delta R.T.: -0.046 min
Response: 91919
Conc: 2.46 ng/ml

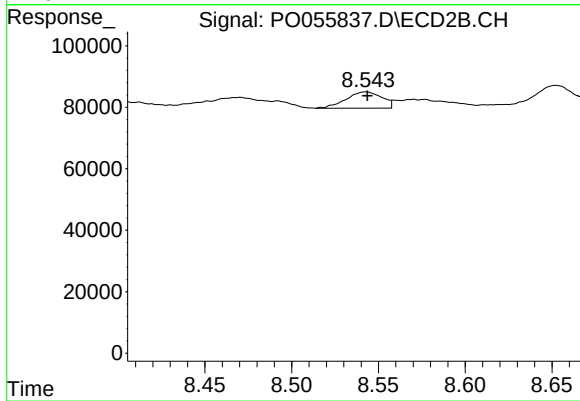

#2 Decachlorobiphenyl

R.T.: 8.543 min
Delta R.T.: -0.001 min
Response: 76629
Conc: 2.83 ng/ml m