

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0050319\
 Data File : P0055839.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 May 2019 19:58
 Operator : SM/SJ
 Sample : PB119287BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB119287BL

Manual Integrations
 APPROVED

Ankita
 5/6/2019 9:56:18 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 03 22:58:06 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 03 15:20:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.278	3.591	662799	666767	22.148	23.608
2) SA Decachlor...	9.878	8.543	705816	548526	18.864m	20.283

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0050319\
Data File : P0055839.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 May 2019 19:58
Operator : SM/SJ
Sample : PB119287BL
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PB119287BL


Manual Integrations
APPROVED

Ankita
5/6/2019 9:56:18 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 03 22:58:06 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 03 15:20:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

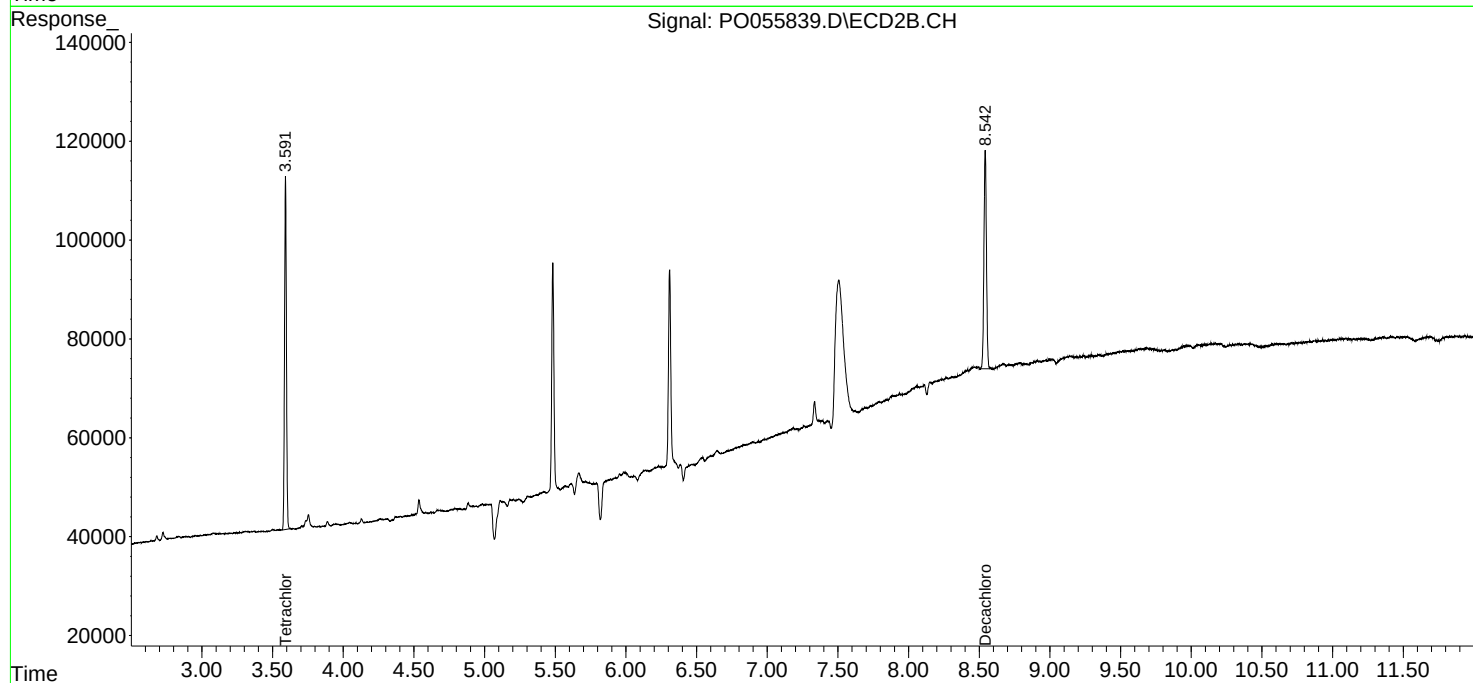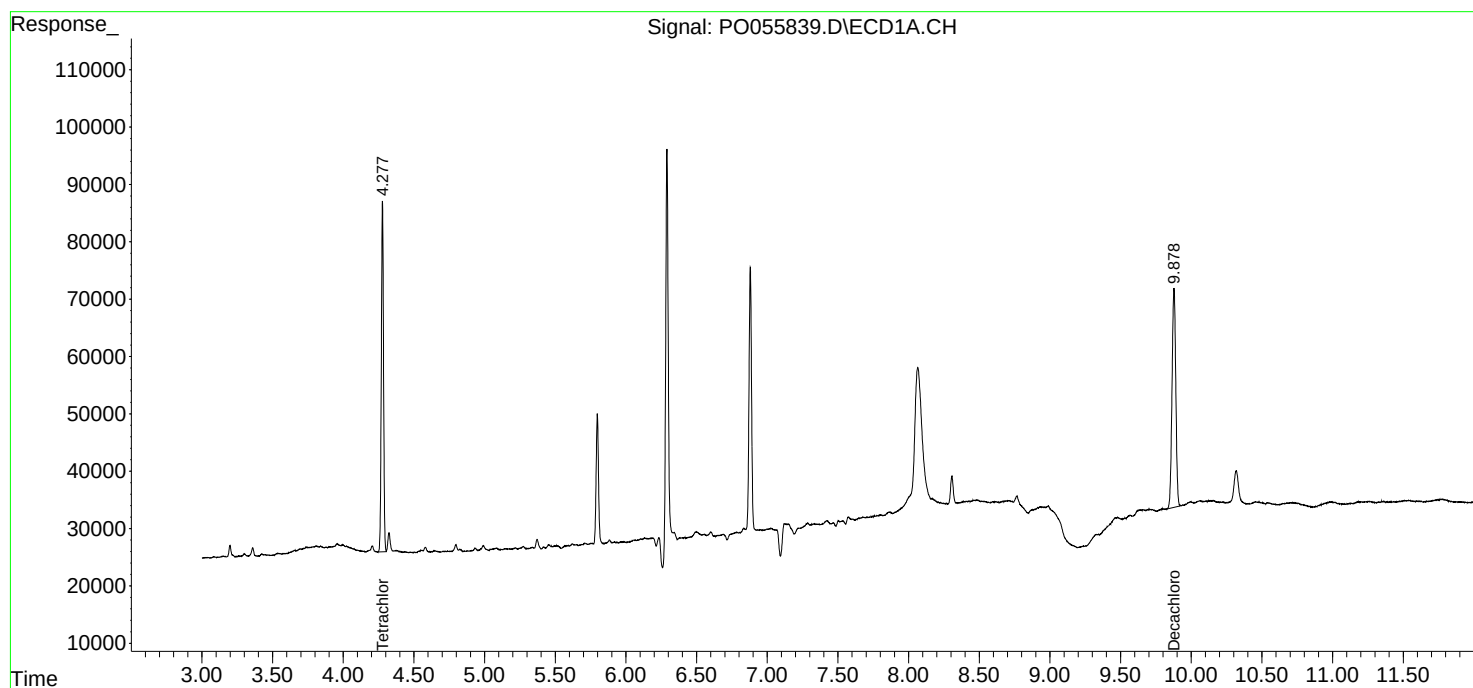

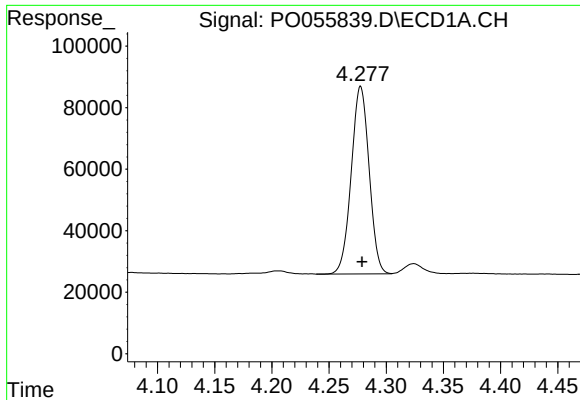


#1 Tetrachloro-m-xylene

R.T.: 4.278 min
Delta R.T.: -0.001 min
Response: 662799
Conc: 22.15 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB119287BL


Manual Integrations
APPROVED

Ankita
5/6/2019 9:56:18 AM

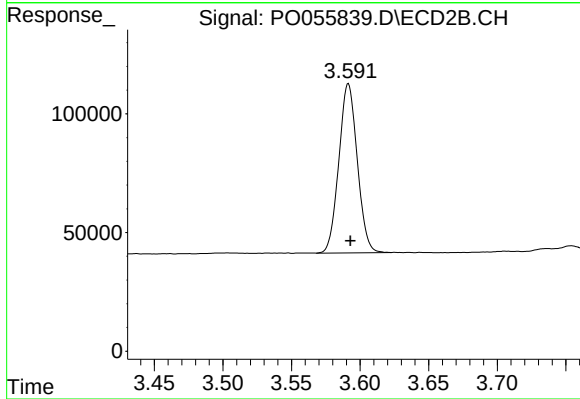


#1 Tetrachloro-m-xylene

R.T.: 3.591 min
Delta R.T.: -0.001 min
Response: 666767
Conc: 23.61 ng/ml

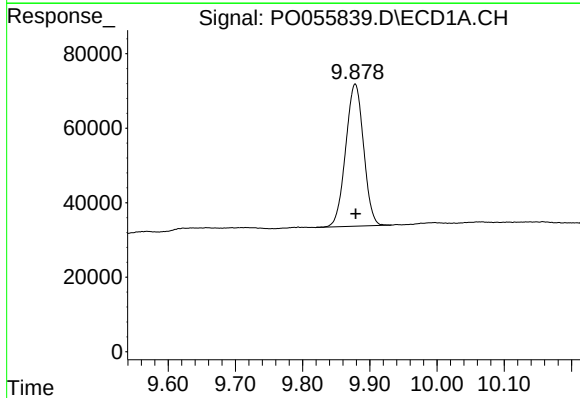

#2 Decachlorobiphenyl

R.T.: 9.878 min
Delta R.T.: -0.001 min
Response: 705816
Conc: 18.86 ng/ml m

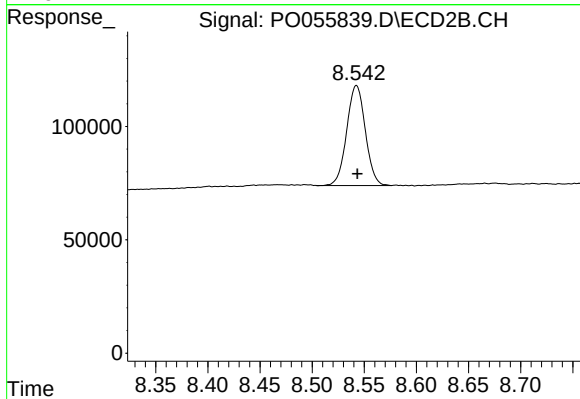

#2 Decachlorobiphenyl

R.T.: 8.543 min
Delta R.T.: -0.001 min
Response: 548526
Conc: 20.28 ng/ml