

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0050319\
 Data File : P0055849.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 May 2019 22:47
 Operator : SM/SJ
 Sample : K2650-01RE
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 GROUND-WATERRE

Manual Integrations
 APPROVED

Ankita
 5/6/2019 9:56:28 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 04 00:37:04 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 03 15:20:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.279	3.592	353411	359815	11.810m	12.740m
2) SA Decachlor...	9.876	8.542	43475	34921	1.162m	1.291

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0050319\
Data File : P0055849.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 May 2019 22:47
Operator : SM/SJ
Sample : K2650-01RE
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
GROUND-WATERRE


Manual Integrations
APPROVED

Ankita
5/6/2019 9:56:28 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 04 00:37:04 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 03 15:20:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

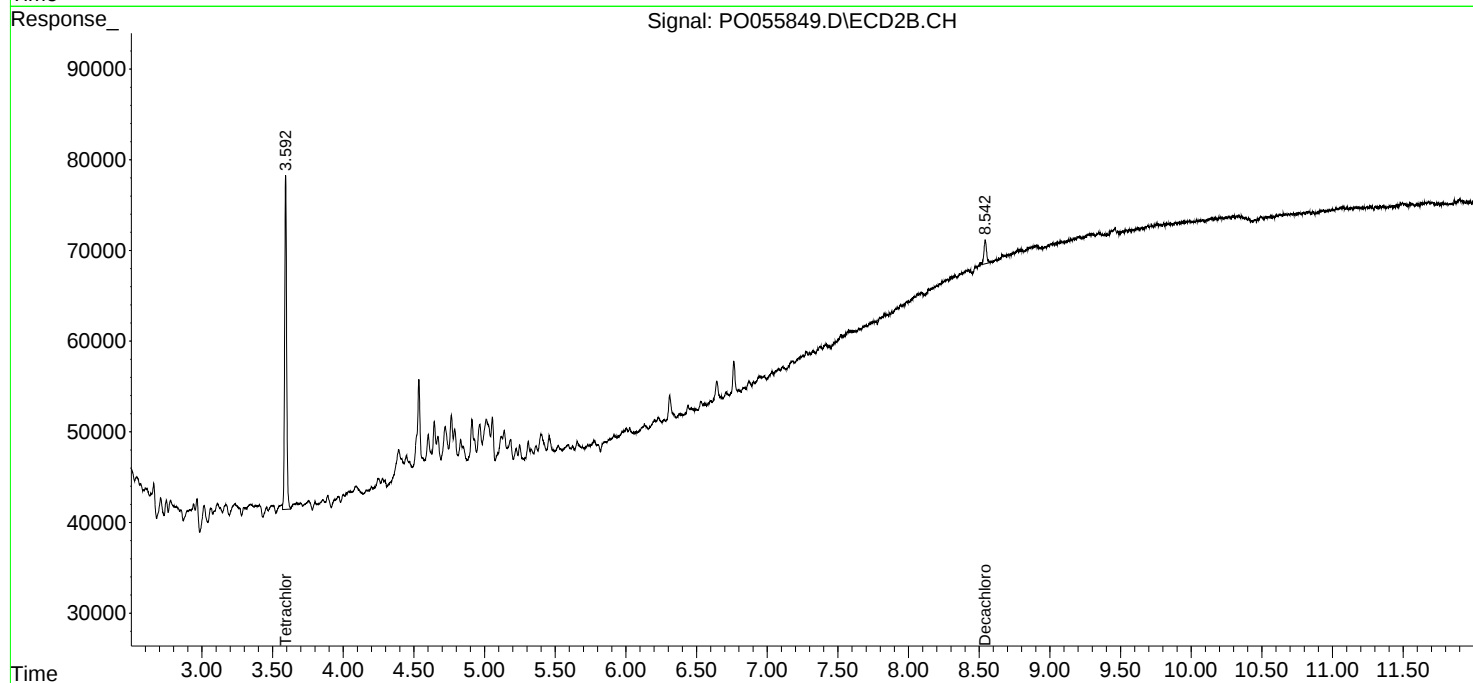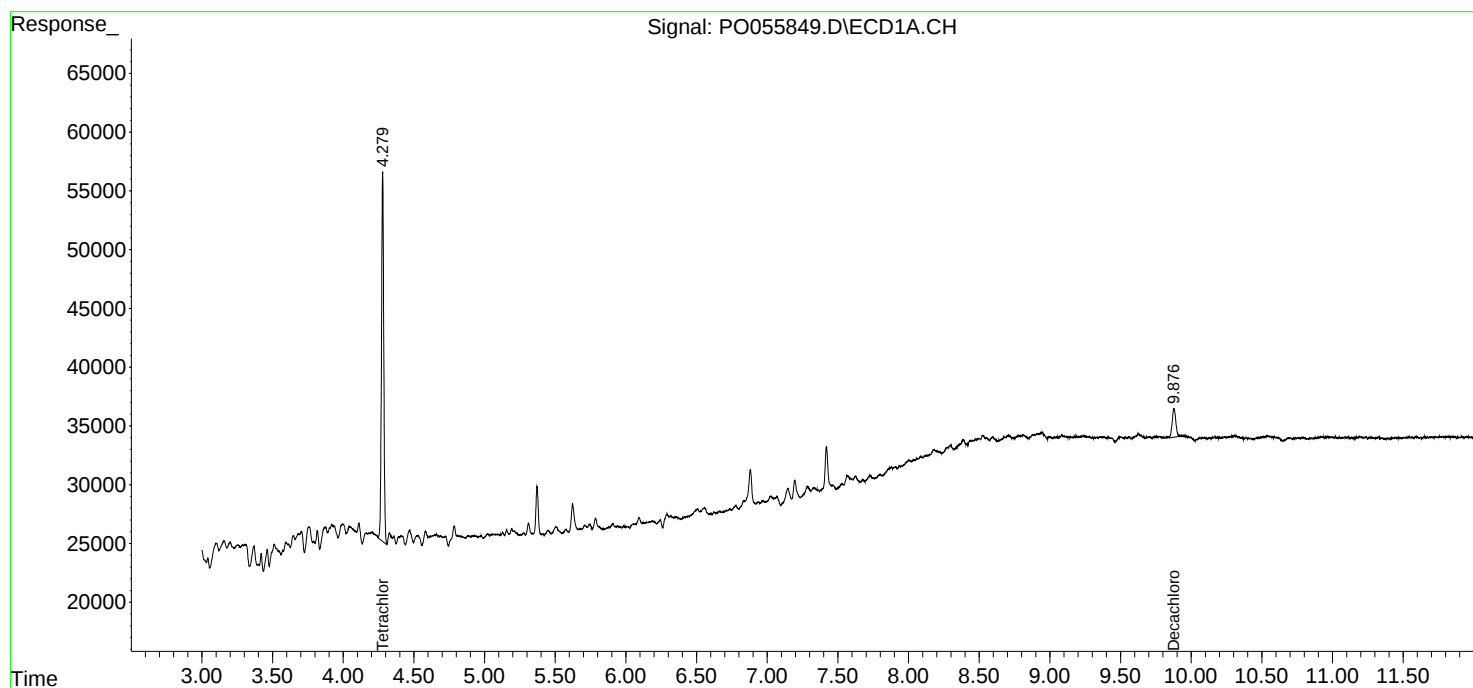

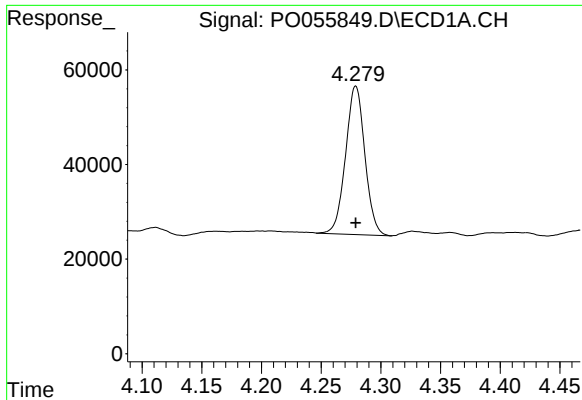


#1 Tetrachloro-m-xylene

R.T.: 4.279 min
Delta R.T.: 0.000 min
Response: 353411
Conc: 11.81 ng/ml m

Instrument :
ECD_O
ClientSampleId :
GROUND-WATERRE


Manual Integrations
APPROVED

Ankita
5/6/2019 9:56:28 AM

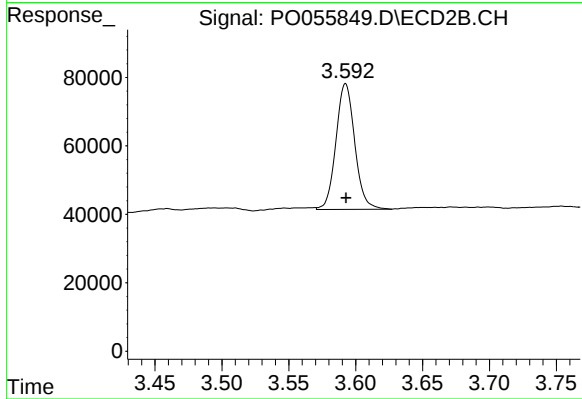


#1 Tetrachloro-m-xylene

R.T.: 3.592 min
Delta R.T.: 0.000 min
Response: 359815
Conc: 12.74 ng/ml m

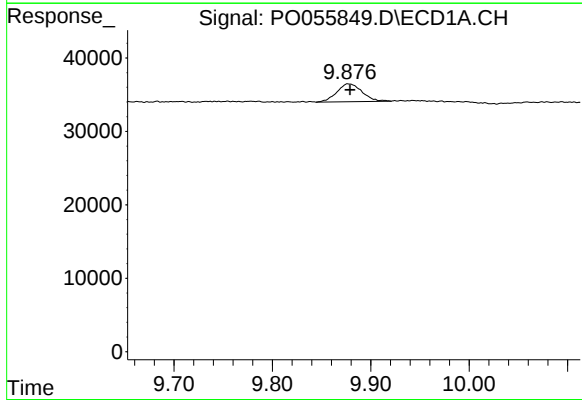

#2 Decachlorobiphenyl

R.T.: 9.876 min
Delta R.T.: -0.003 min
Response: 43475
Conc: 1.16 ng/ml m

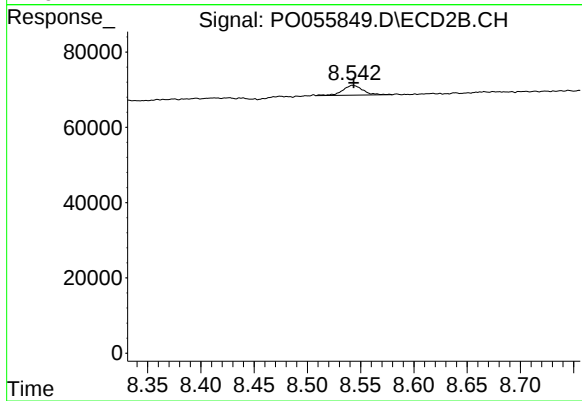

#2 Decachlorobiphenyl

R.T.: 8.542 min
Delta R.T.: -0.001 min
Response: 34921
Conc: 1.29 ng/ml