

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0050319\
 Data File : P0055863.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 May 2019 2:44
 Operator : SM/SJ
 Sample : K2668-03
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 04 06:54:25 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 03 15:20:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.279	3.593	945358	1005780	31.590	35.611
2) SA Decachlor...	9.880	8.545	619900	429901	16.567	15.897

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO050319\
Data File : PO055863.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 May 2019 2:44
Operator : SM/SJ
Sample : K2668-03
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 04 06:54:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO050319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 03 15:20:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

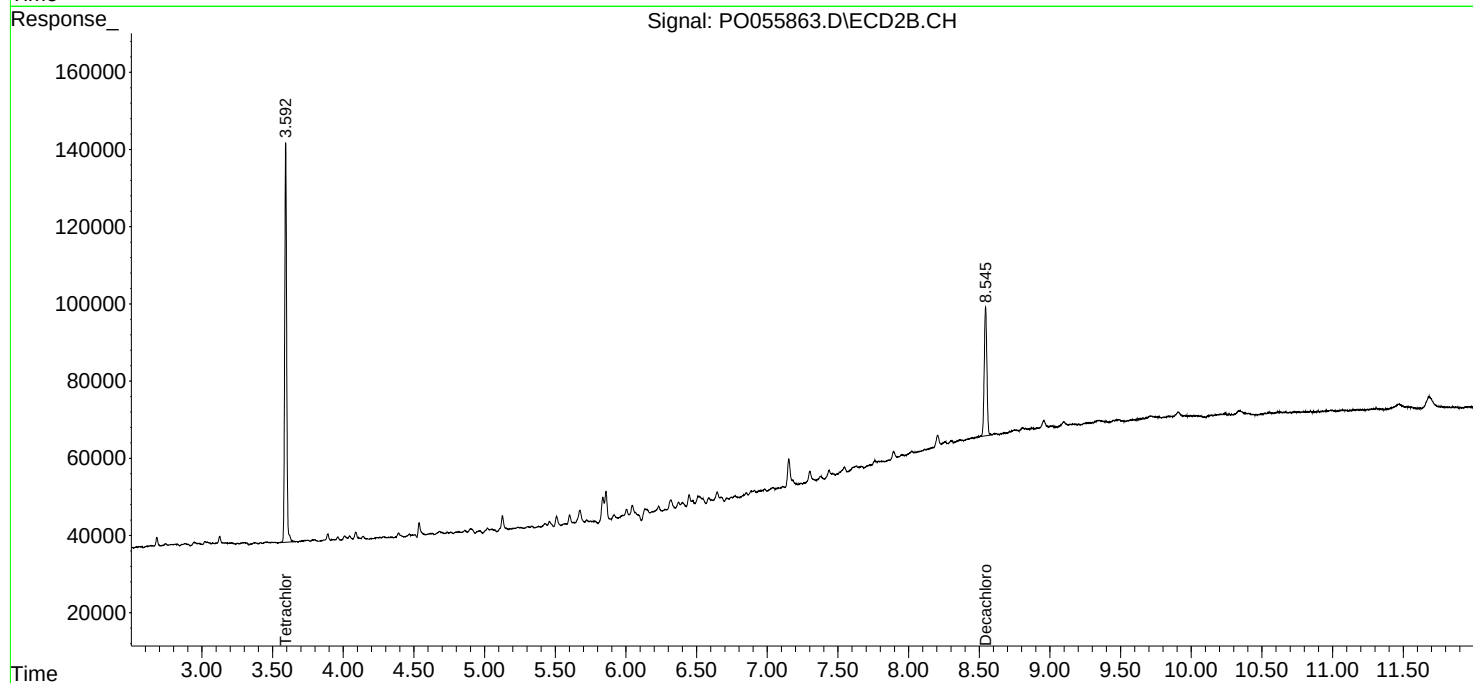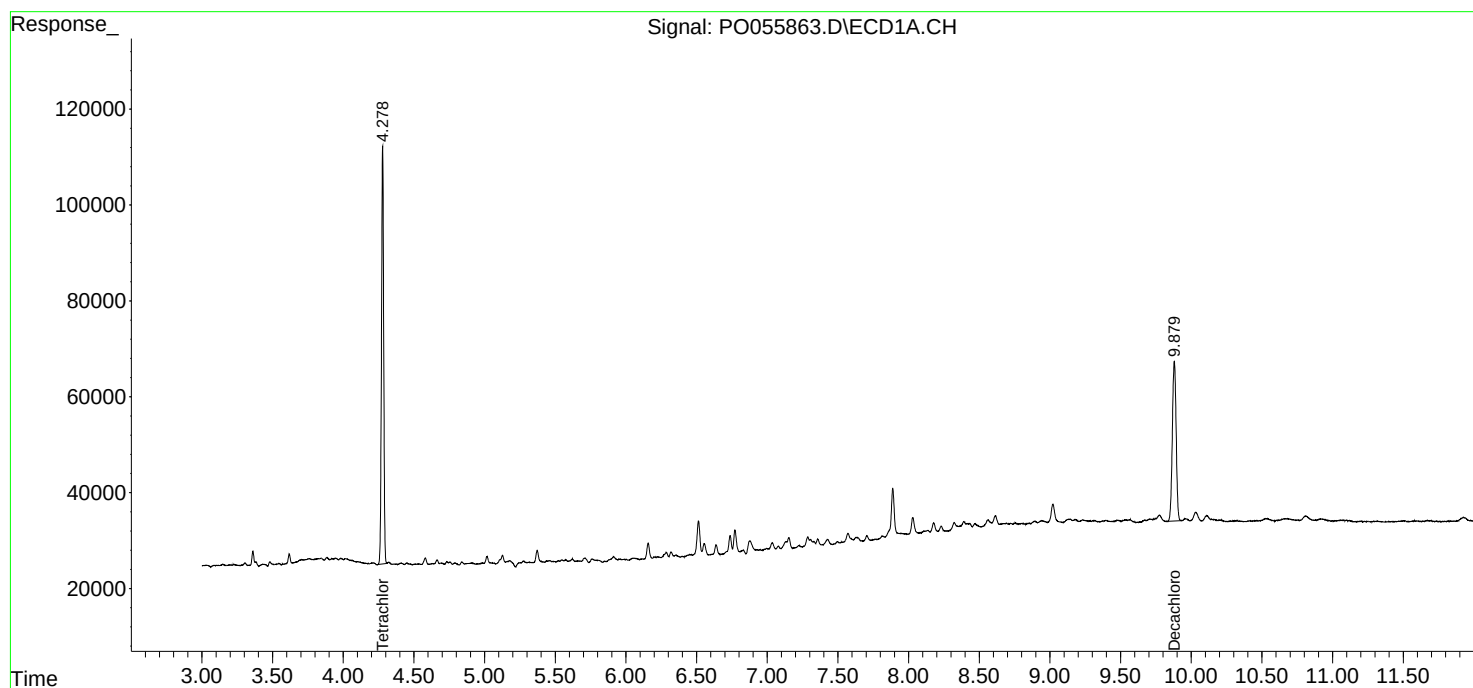


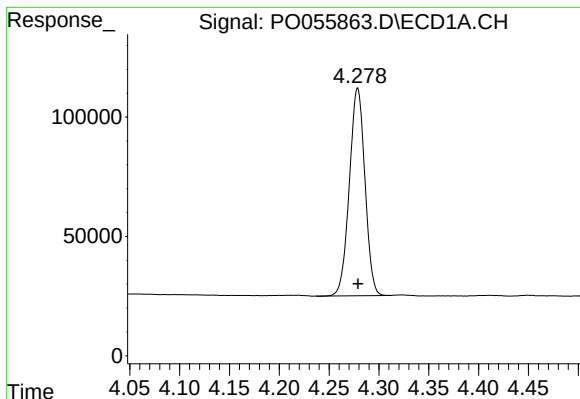

#1 Tetrachloro-m-xylene


R.T.: 4.279 min
Delta R.T.: 0.000 min
Response: 945358
Conc: 31.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-2

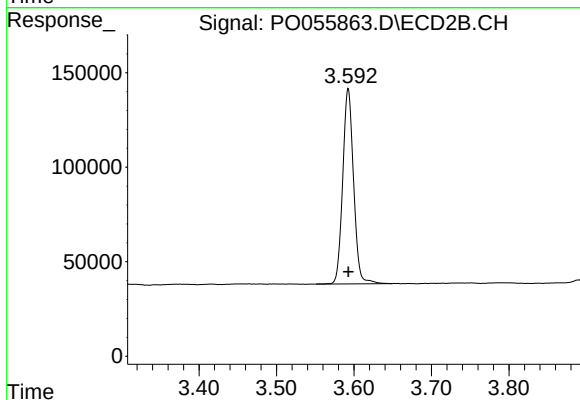


#1 Tetrachloro-m-xylene

R.T.: 3.593 min
Delta R.T.: 0.000 min
Response: 1005780
Conc: 35.61 ng/ml

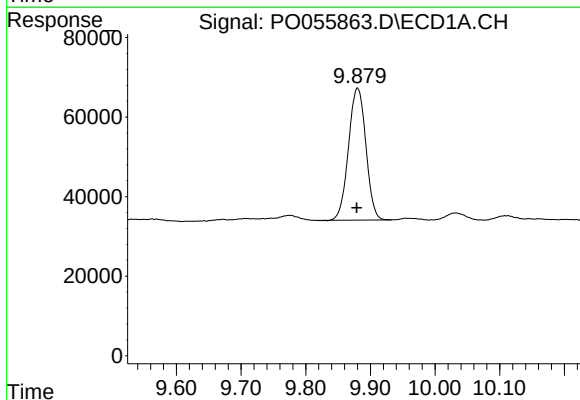

#2 Decachlorobiphenyl

R.T.: 9.880 min
Delta R.T.: 0.001 min
Response: 619900
Conc: 16.57 ng/ml

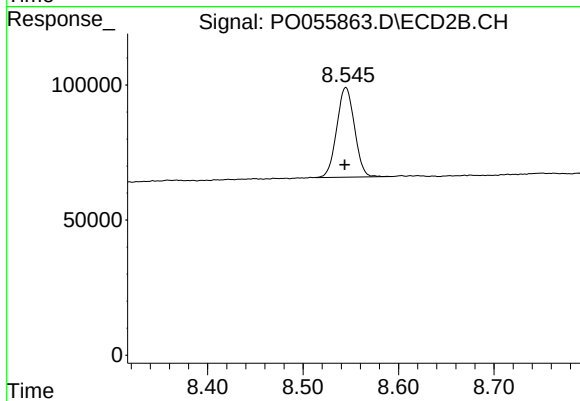

#2 Decachlorobiphenyl

R.T.: 8.545 min
Delta R.T.: 0.001 min
Response: 429901
Conc: 15.90 ng/ml