

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0050321\
 Data File : P0077491.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 May 2021 15:09
 Operator : DD\AJ
 Sample : M2238-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 HR-02-043021

Manual Integrations
 APPROVED

Ankita
 5/4/2021 4:39:08 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 03 16:46:05 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Apr 29 05:54:04 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.890	3.883	2386635	1184172	21.749	21.213
2) SA Decachlor...	10.856	9.118	2207746	648343	20.077	19.058
Target Compounds						
31) L7 AR-1260-1	7.897	6.697	50976	43649	8.245m	13.871 #
32) L7 AR-1260-2	8.164	6.896	157583	34052	21.037	9.157m#
33) L7 AR-1260-3	8.532	7.046	62314	29161	12.447	8.478 #
34) L7 AR-1260-4	8.760	7.529	79186	40183	14.460	16.818m
35) L7 AR-1260-5	9.083	7.774	156032	89601	14.383	17.097

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0050321\
Data File : P0077491.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 May 2021 15:09
Operator : DD\AJ
Sample : M2238-01
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
HR-02-043021


Manual Integrations
APPROVED

Ankita
5/4/2021 4:39:08 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 03 16:46:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042821.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Apr 29 05:54:04 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

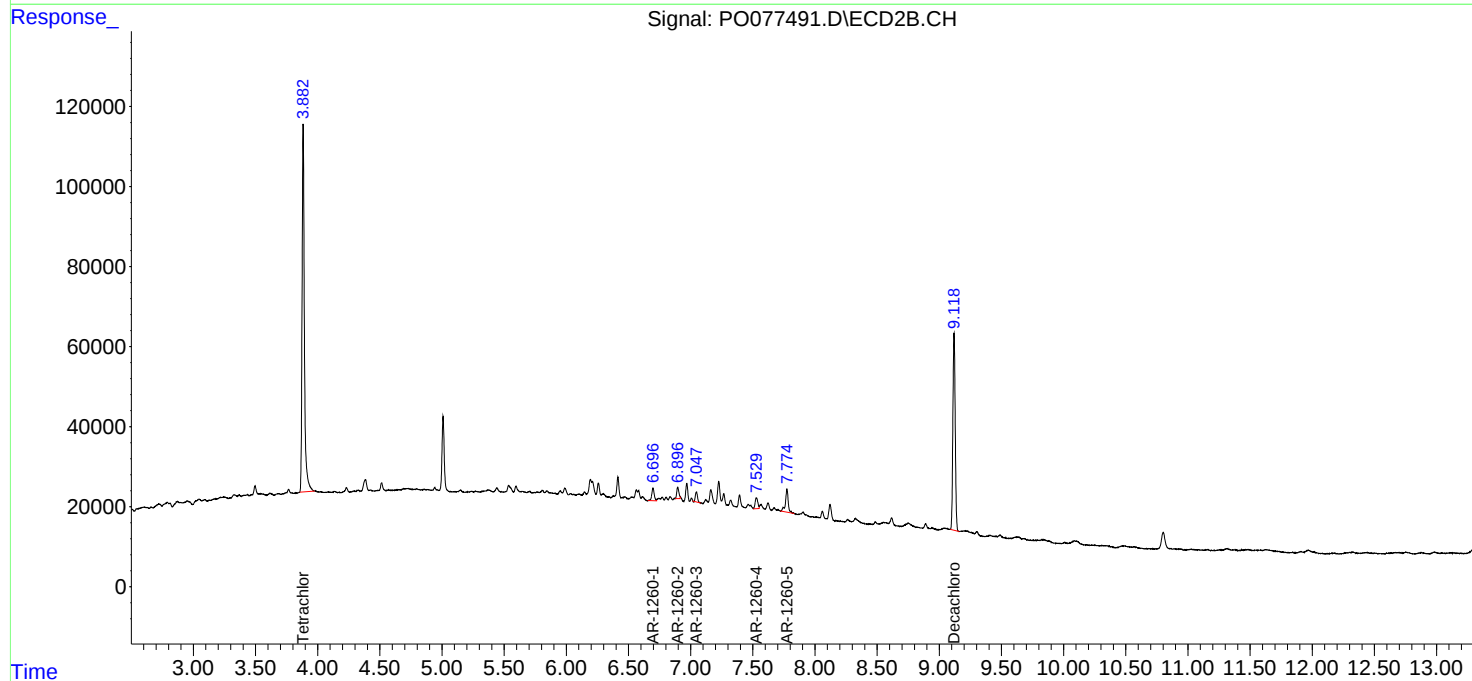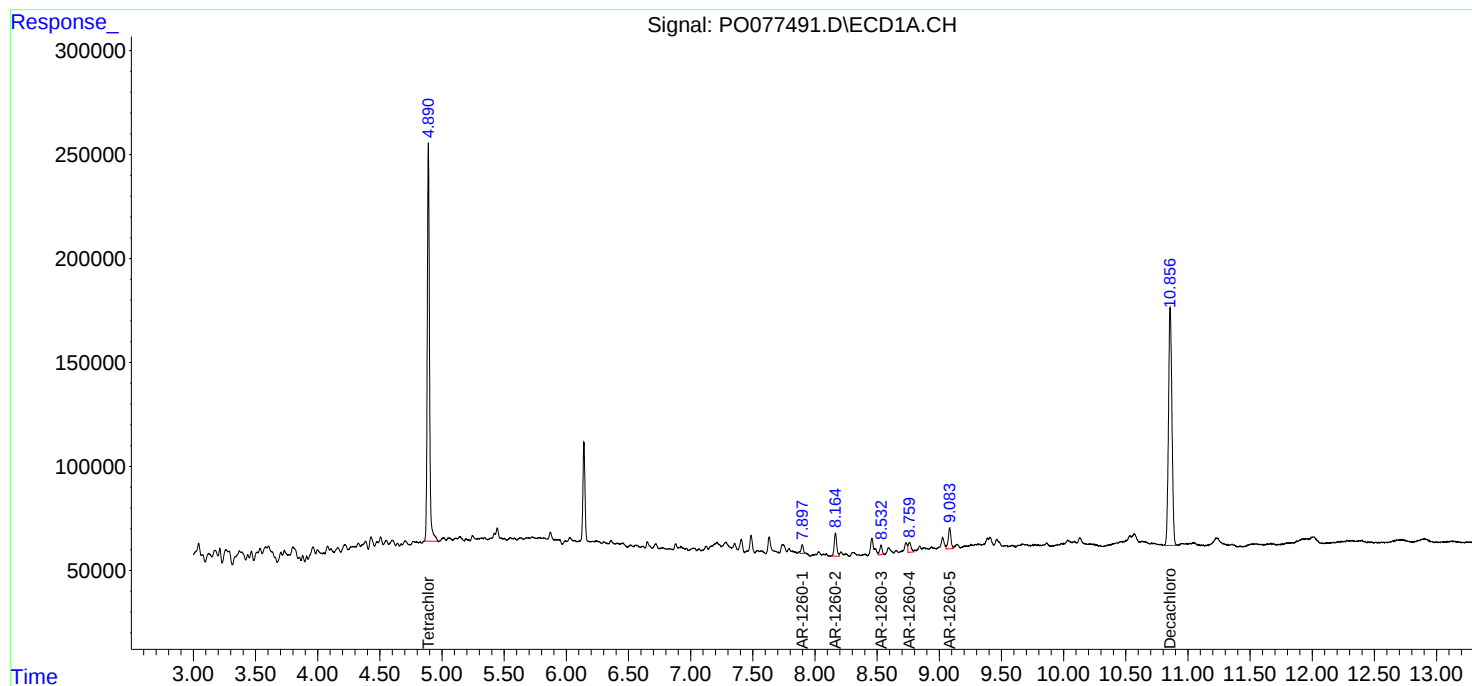

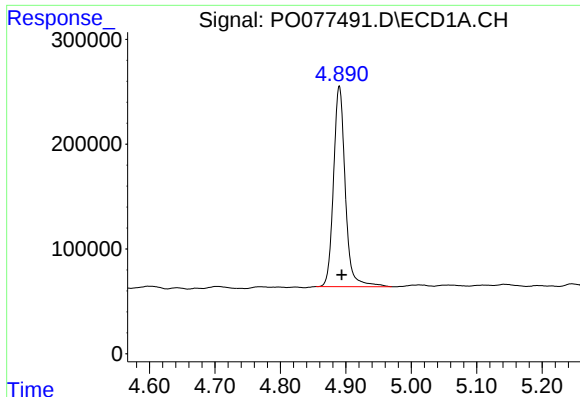


#1 Tetrachloro-m-xylene

R.T.: 4.890 min
Delta R.T.: -0.004 min
Response: 2386635
Conc: 21.75 ng/ml

Instrument :
ECD_O
ClientSampleId :
HR-02-043021


Manual Integrations
APPROVED

Ankita
5/4/2021 4:39:08 PM

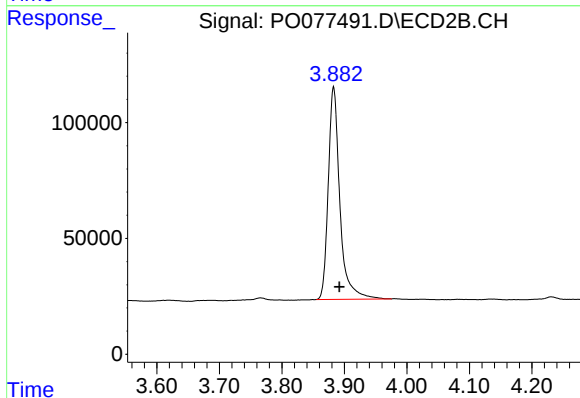


#1 Tetrachloro-m-xylene

R.T.: 3.883 min
Delta R.T.: -0.010 min
Response: 1184172
Conc: 21.21 ng/ml

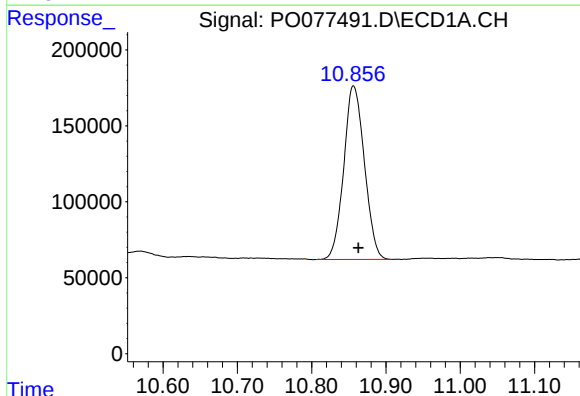


#2 Decachlorobiphenyl

R.T.: 10.856 min
Delta R.T.: -0.007 min
Response: 2207746
Conc: 20.08 ng/ml

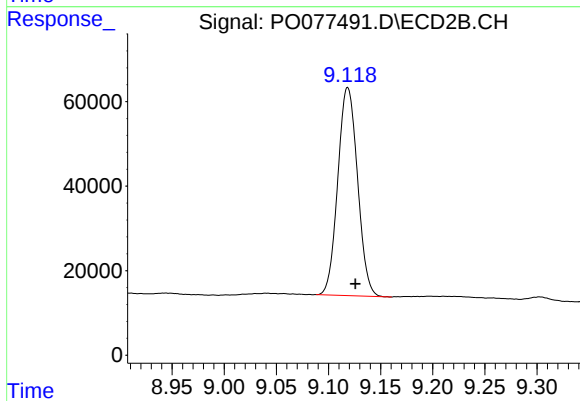

#2 Decachlorobiphenyl

R.T.: 9.118 min
Delta R.T.: -0.007 min
Response: 648343
Conc: 19.06 ng/ml

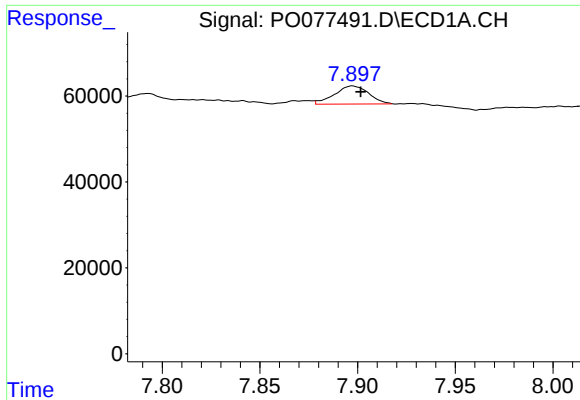


#31 AR-1260-1

R.T.: 7.897 min
Delta R.T.: -0.005 min
Response: 50976
Conc: 8.25 ng/ml m

Instrument :
ECD_O
ClientSampleId :
HR-02-043021


Manual Integrations
APPROVED

Ankita
5/4/2021 4:39:08 PM

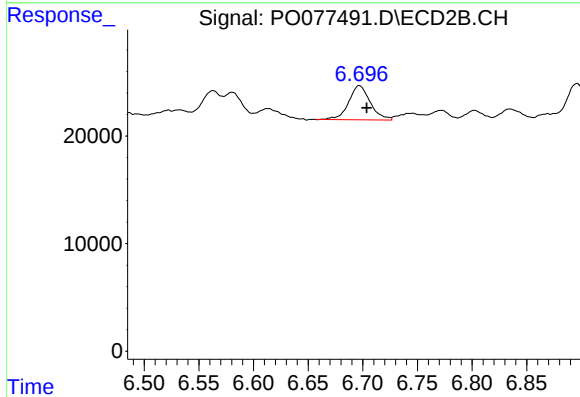


#31 AR-1260-1

R.T.: 6.697 min
Delta R.T.: -0.007 min
Response: 43649
Conc: 13.87 ng/ml

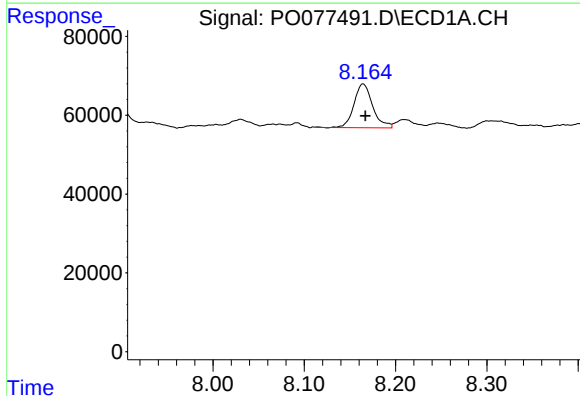


#32 AR-1260-2

R.T.: 8.164 min
Delta R.T.: -0.003 min
Response: 157583
Conc: 21.04 ng/ml

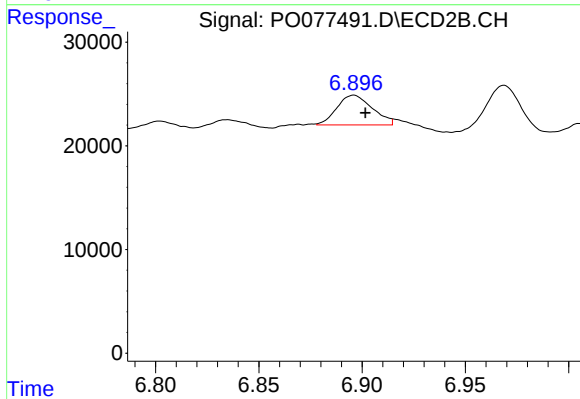

#32 AR-1260-2

R.T.: 6.896 min
Delta R.T.: -0.006 min
Response: 34052
Conc: 9.16 ng/ml m

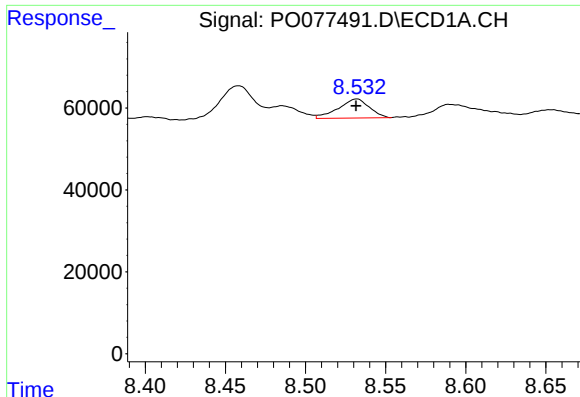


#33 AR-1260-3

R.T.: 8.532 min
Delta R.T.: 0.000 min
Response: 62314
Conc: 12.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
HR-02-043021


Manual Integrations
APPROVED

Ankita
5/4/2021 4:39:08 PM

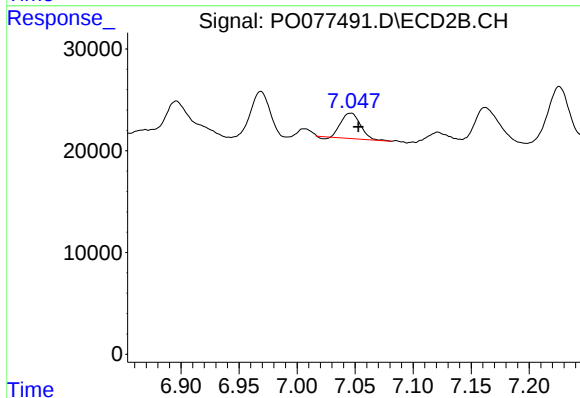


#33 AR-1260-3

R.T.: 7.046 min
Delta R.T.: -0.006 min
Response: 29161
Conc: 8.48 ng/ml

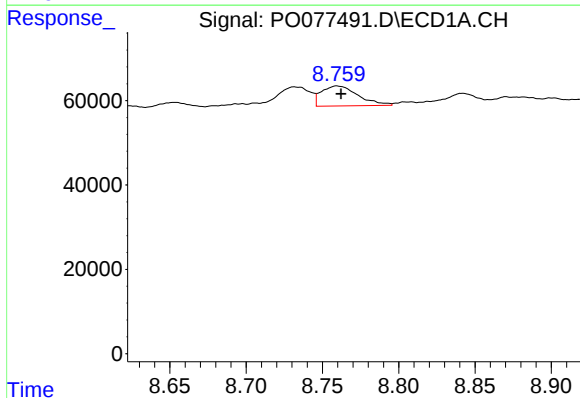


#34 AR-1260-4

R.T.: 8.760 min
Delta R.T.: -0.003 min
Response: 79186
Conc: 14.46 ng/ml

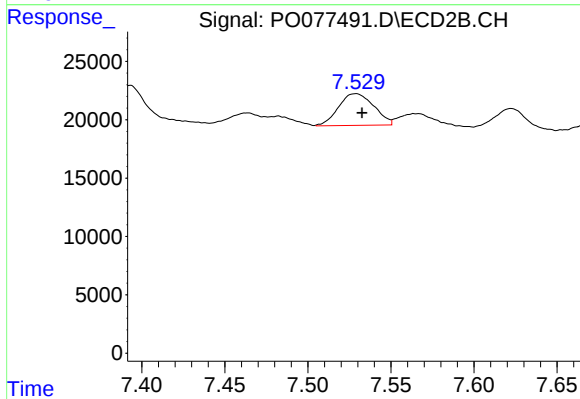

#34 AR-1260-4

R.T.: 7.529 min
Delta R.T.: -0.004 min
Response: 40183
Conc: 16.82 ng/ml m

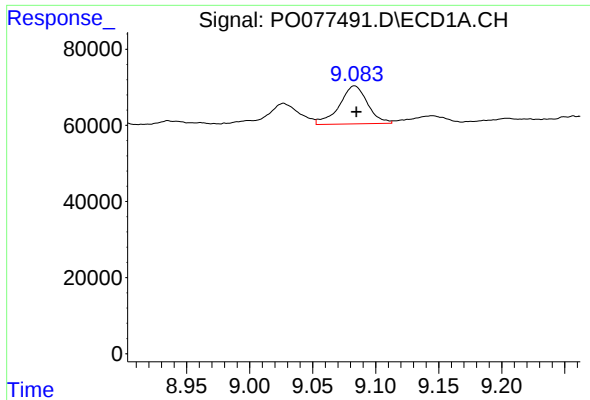


#35 AR-1260-5

R.T.: 9.083 min
Delta R.T.: -0.001 min
Response: 156032
Conc: 14.38 ng/ml

Instrument :
ECD_O
ClientSampleId :
HR-02-043021

Manual Integrations
APPROVED

Ankita
5/4/2021 4:39:08 PM

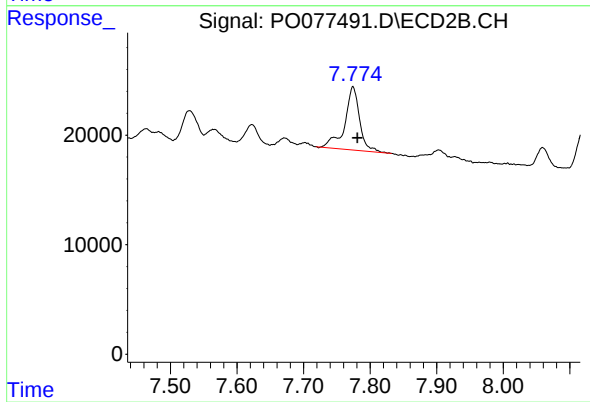

#35 AR-1260-5

R.T.: 7.774 min
Delta R.T.: -0.007 min
Response: 89601
Conc: 17.10 ng/ml