

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0050321\
 Data File : P0077493.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 May 2021 15:43
 Operator : DD\AJ
 Sample : M2242-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 STOCK-PILE

Manual Integrations
 APPROVED

Ankita
 5/4/2021 4:39:15 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 03 16:47:00 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0042821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Apr 29 05:54:04 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.889	3.882	2481331	1291164	22.612	23.130
2) SA Decachlor...	10.856	9.118	2301392	691982	20.929	20.341
Target Compounds						
31) L7 AR-1260-1	7.897	6.696	272675	168556	44.104m	53.564
32) L7 AR-1260-2	8.165	6.897	898163	199256	119.905	53.583 #
33) L7 AR-1260-3	8.529	7.044	145345	102508	29.032	29.801
34) L7 AR-1260-4	8.758	7.526	289767	89773	52.914	37.573 #
35) L7 AR-1260-5	9.082	7.773	362466	226616	33.412	43.240 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO050321\
Data File : PO077493.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 May 2021 15:43
Operator : DD\AJ
Sample : M2242-01
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
STOCK-PILE


Manual Integrations
APPROVED

Ankita
5/4/2021 4:39:15 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 03 16:47:00 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO042821.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Apr 29 05:54:04 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

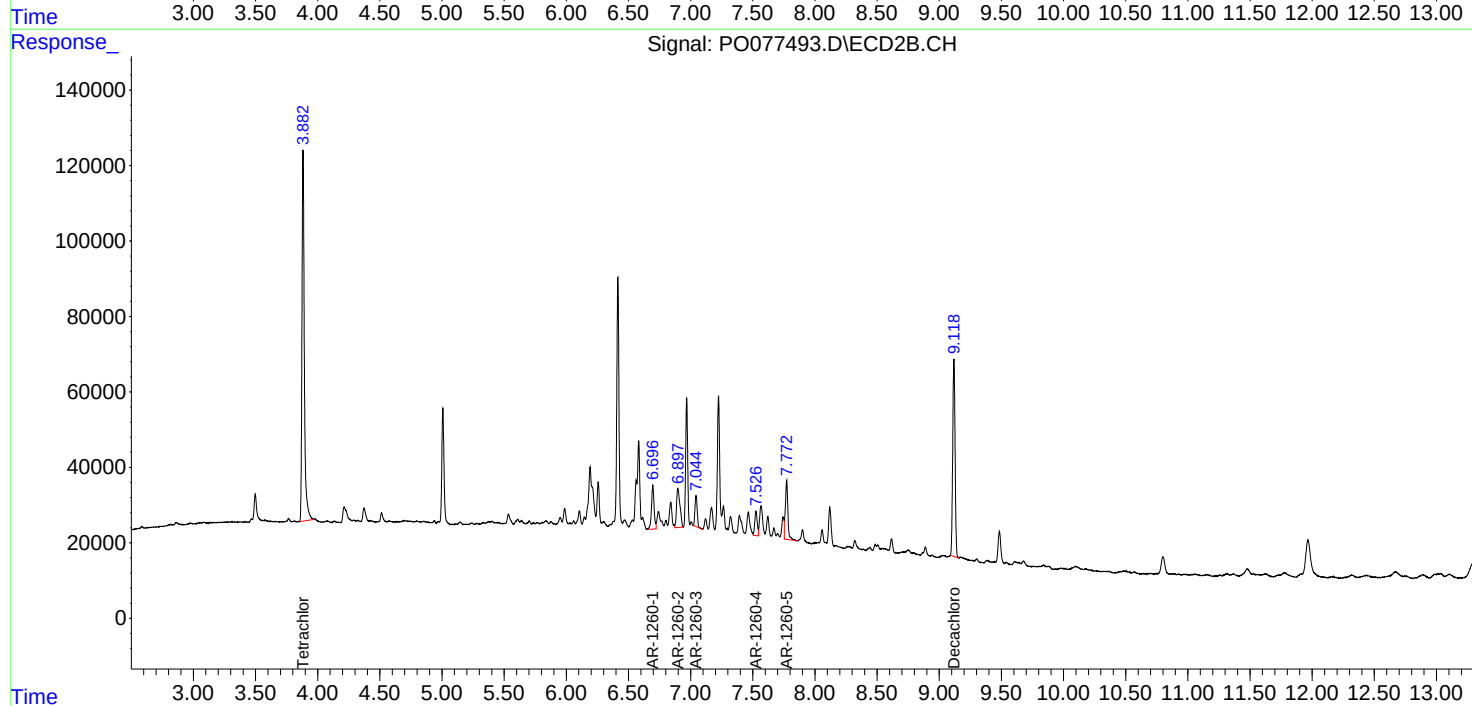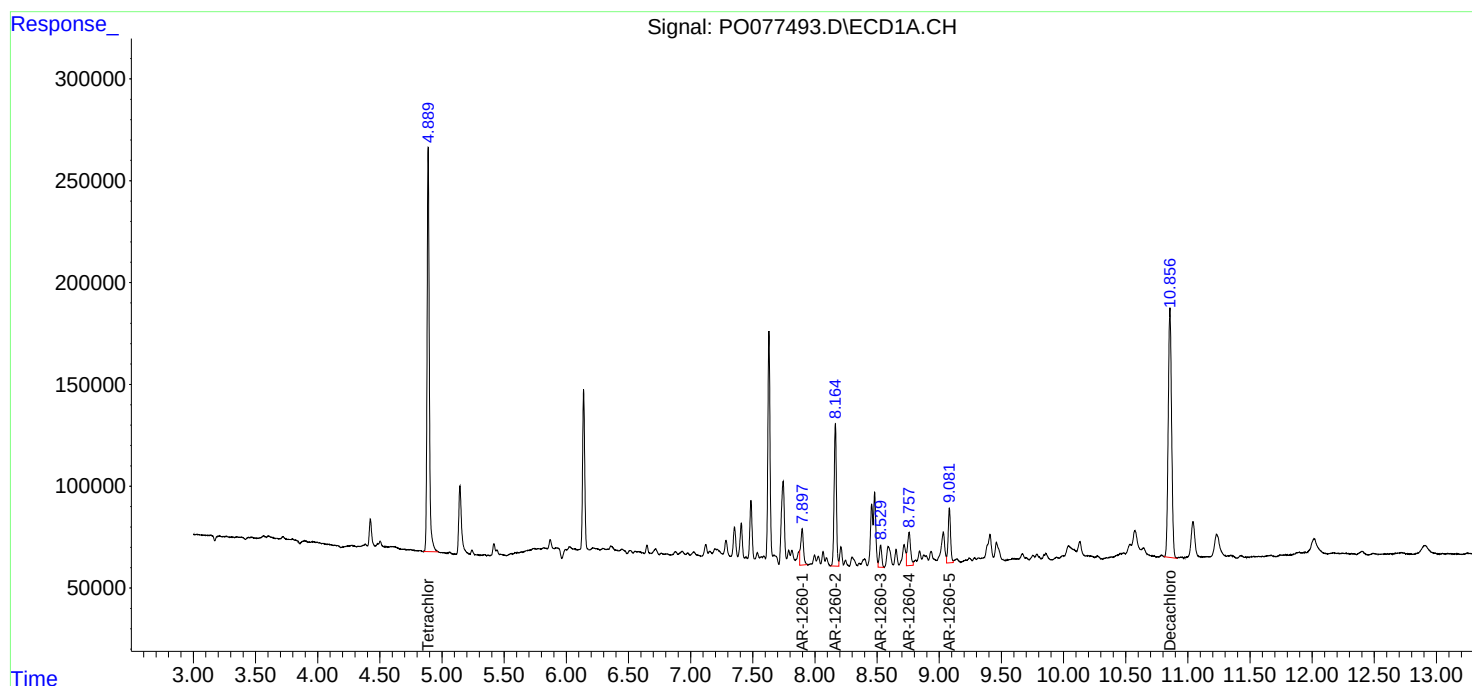

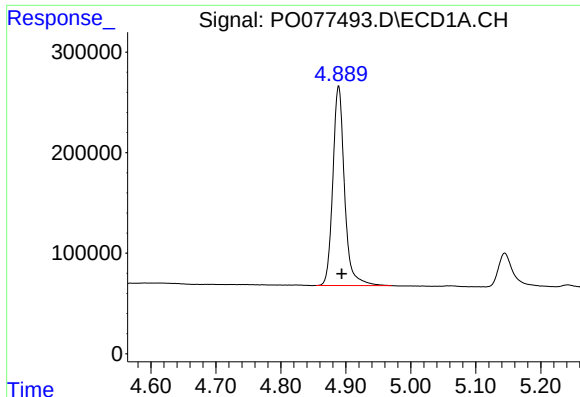


#1 Tetrachloro-m-xylene

R.T.: 4.889 min
Delta R.T.: -0.005 min
Response: 2481331
Conc: 22.61 ng/ml

Instrument :
ECD_O
ClientSampleId :
STOCK-PILE


Manual Integrations
APPROVED

Ankita
5/4/2021 4:39:15 PM

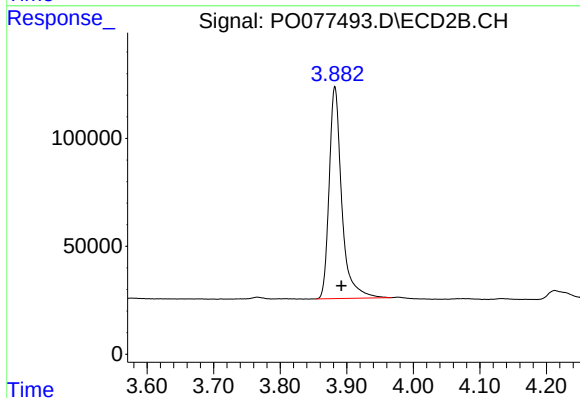


#1 Tetrachloro-m-xylene

R.T.: 3.882 min
Delta R.T.: -0.010 min
Response: 1291164
Conc: 23.13 ng/ml

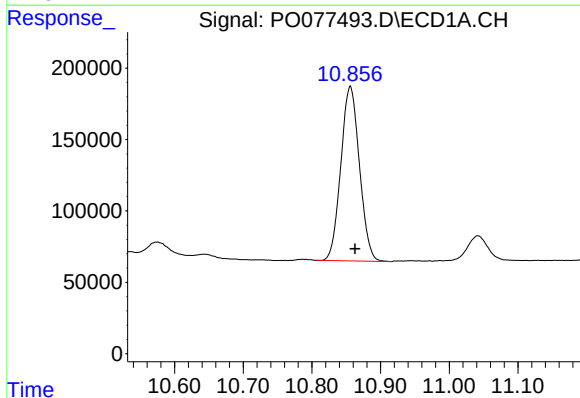


#2 Decachlorobiphenyl

R.T.: 10.856 min
Delta R.T.: -0.007 min
Response: 2301392
Conc: 20.93 ng/ml

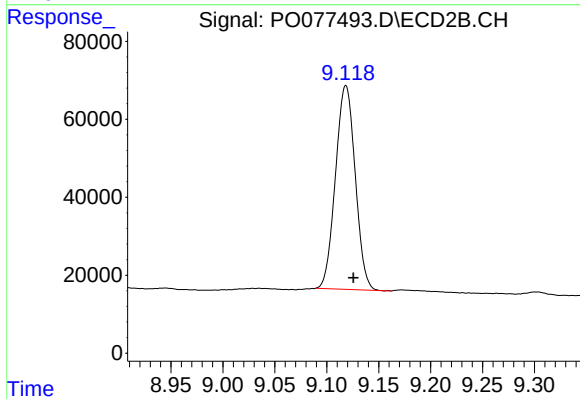

#2 Decachlorobiphenyl

R.T.: 9.118 min
Delta R.T.: -0.007 min
Response: 691982
Conc: 20.34 ng/ml

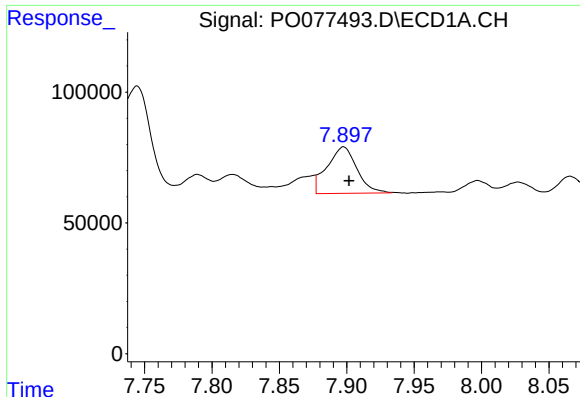


#31 AR-1260-1

R.T.: 7.897 min
Delta R.T.: -0.004 min
Response: 272675
Conc: 44.10 ng/ml m

Instrument :
ECD_O
ClientSampleId :
STOCK-PILE


Manual Integrations
APPROVED

Ankita
5/4/2021 4:39:15 PM

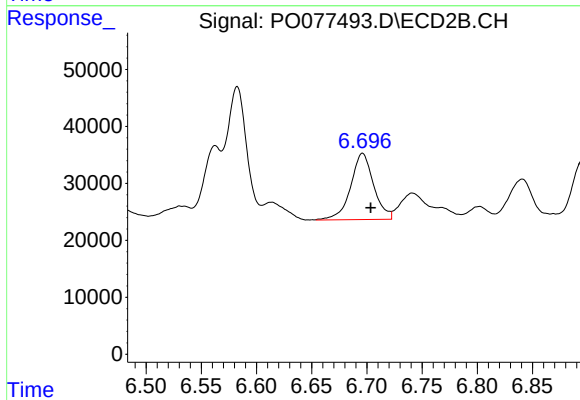


#31 AR-1260-1

R.T.: 6.696 min
Delta R.T.: -0.008 min
Response: 168556
Conc: 53.56 ng/ml

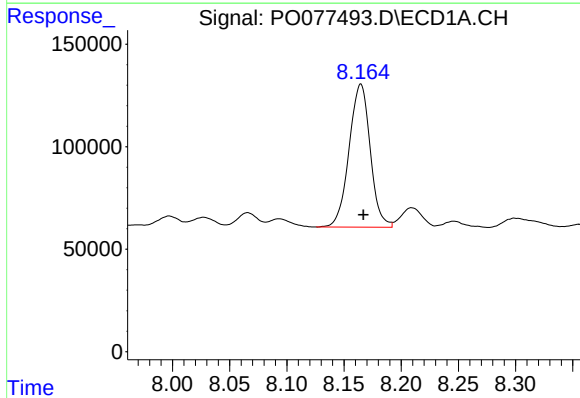


#32 AR-1260-2

R.T.: 8.165 min
Delta R.T.: -0.002 min
Response: 898163
Conc: 119.90 ng/ml

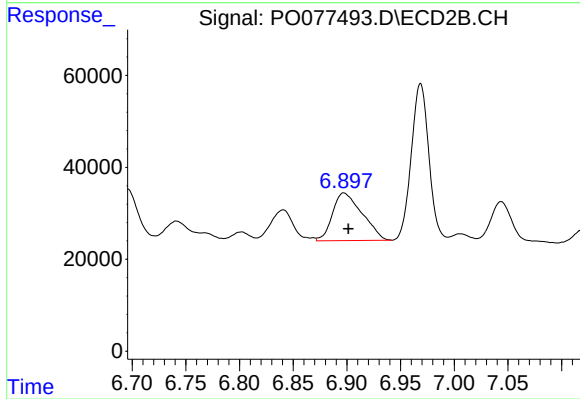

#32 AR-1260-2

R.T.: 6.897 min
Delta R.T.: -0.004 min
Response: 199256
Conc: 53.58 ng/ml

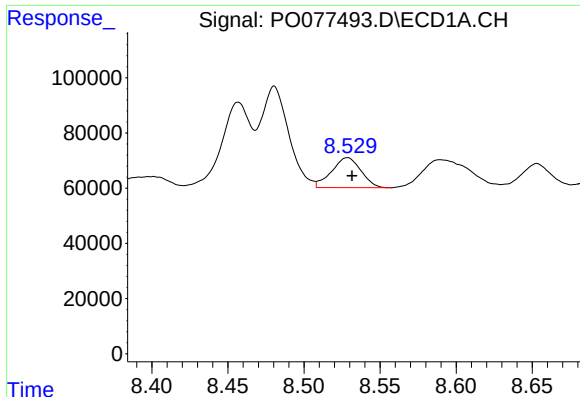


#33 AR-1260-3

R.T.: 8.529 min
Delta R.T.: -0.003 min
Response: 145345
Conc: 29.03 ng/ml

Instrument :
ECD_O
ClientSampleId :
STOCK-PILE


Manual Integrations
APPROVED

Ankita
5/4/2021 4:39:15 PM

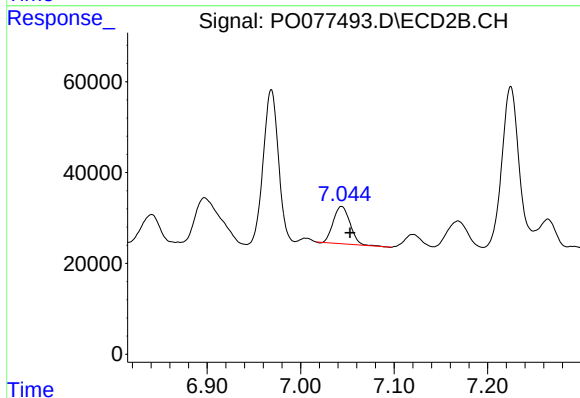


#33 AR-1260-3

R.T.: 7.044 min
Delta R.T.: -0.009 min
Response: 102508
Conc: 29.80 ng/ml

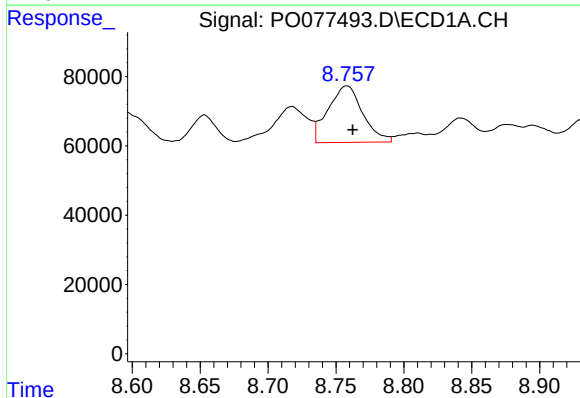


#34 AR-1260-4

R.T.: 8.758 min
Delta R.T.: -0.004 min
Response: 289767
Conc: 52.91 ng/ml

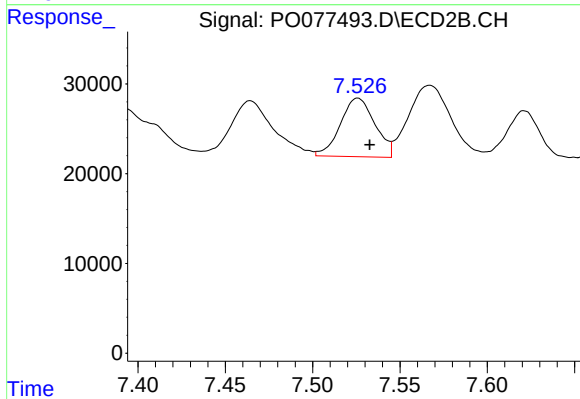

#34 AR-1260-4

R.T.: 7.526 min
Delta R.T.: -0.007 min
Response: 89773
Conc: 37.57 ng/ml

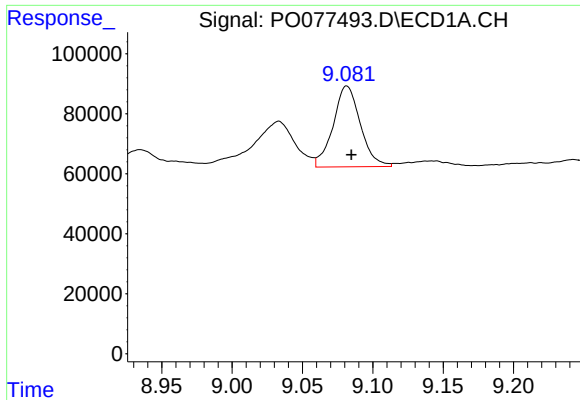


#35 AR-1260-5

R.T.: 9.082 min
Delta R.T.: -0.003 min
Response: 362466
Conc: 33.41 ng/ml

Instrument :
ECD_O
ClientSampleId :
STOCK-PILE

Manual Integrations
APPROVED

Ankita
5/4/2021 4:39:15 PM

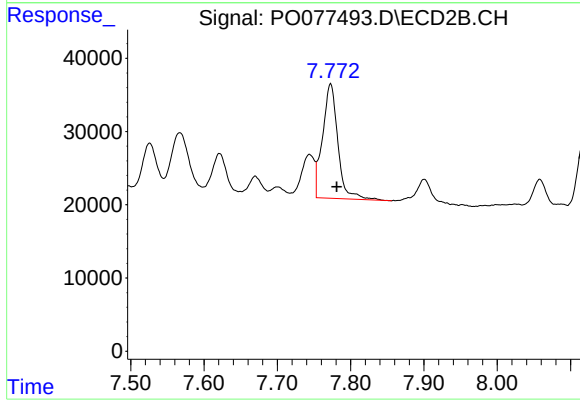

#35 AR-1260-5

R.T.: 7.773 min
Delta R.T.: -0.008 min
Response: 226616
Conc: 43.24 ng/ml