

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0050421\
 Data File : P0077504.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 May 2021 13:09
 Operator : DD\AJ
 Sample : M2253-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 COMP-41772-75

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 04 17:38:22 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Apr 29 05:54:04 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.891	3.885	2026661	1072174	18.469	19.207
2) SA Decachlor...	10.876	9.139	1672879	493845	15.213	14.517

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO050421\
Data File : PO077504.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 May 2021 13:09
Operator : DD\AJ
Sample : M2253-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
COMP-41772-75

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 04 17:38:22 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO042821.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Apr 29 05:54:04 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

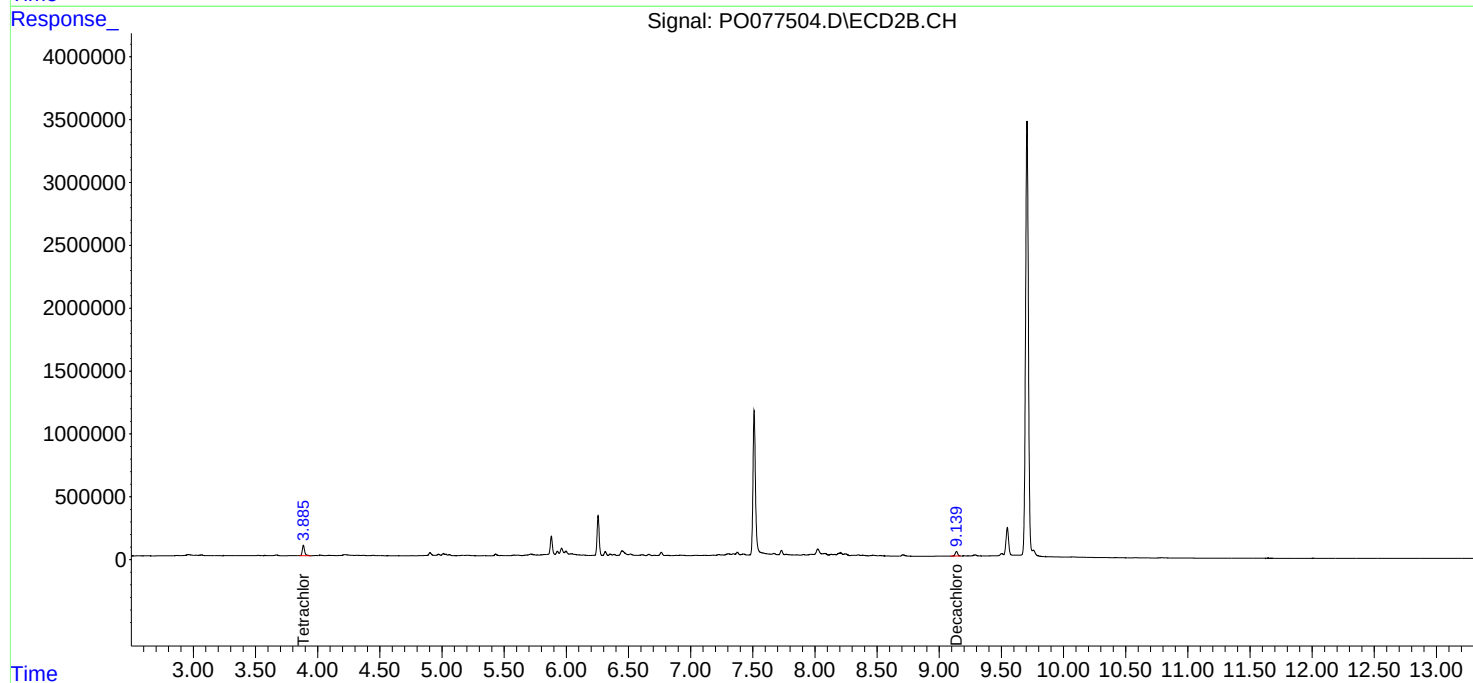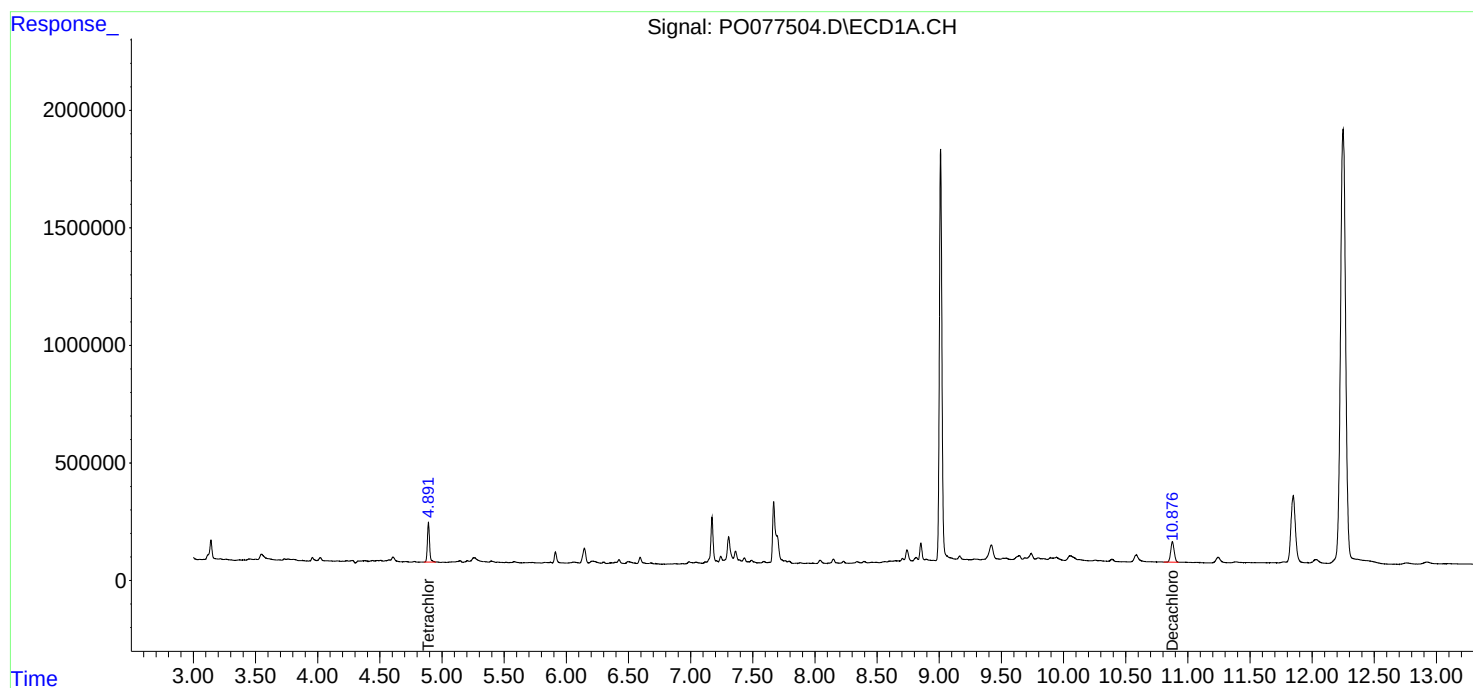


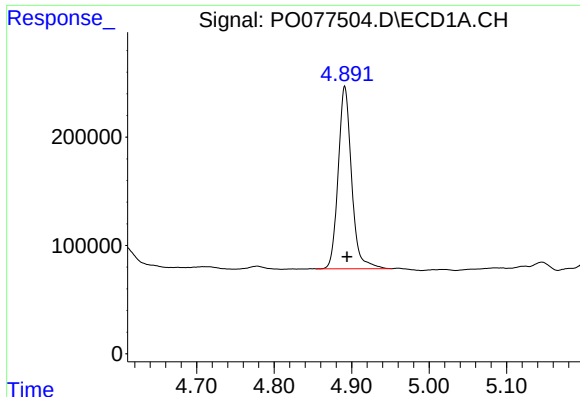

#1 Tetrachloro-m-xylene


R.T.: 4.891 min
Delta R.T.: -0.003 min
Response: 2026661
Conc: 18.47 ng/ml

Instrument :
ECD_O
ClientSampleId :
COMP-41772-75

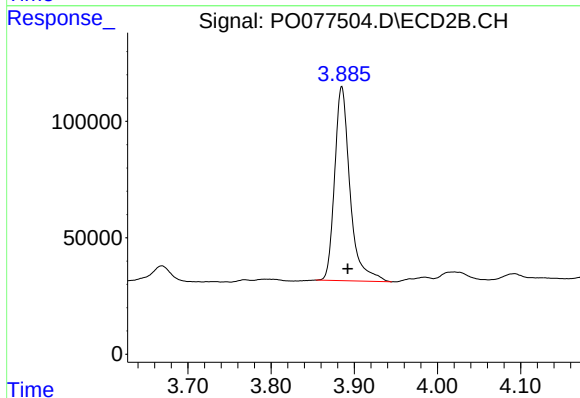


#1 Tetrachloro-m-xylene

R.T.: 3.885 min
Delta R.T.: -0.007 min
Response: 1072174
Conc: 19.21 ng/ml

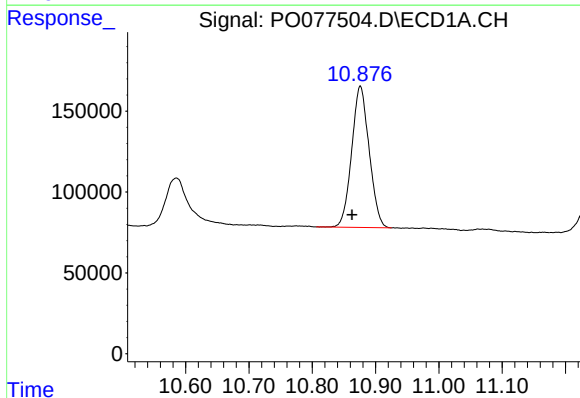

#2 Decachlorobiphenyl

R.T.: 10.876 min
Delta R.T.: 0.013 min
Response: 1672879
Conc: 15.21 ng/ml

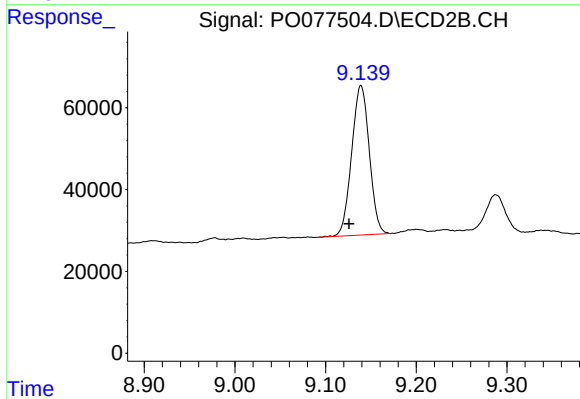

#2 Decachlorobiphenyl

R.T.: 9.139 min
Delta R.T.: 0.013 min
Response: 493845
Conc: 14.52 ng/ml