

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0050421\
 Data File : P0077506.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 May 2021 13:44
 Operator : DD\AJ
 Sample : M2253-03
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 31069

Manual Integrations
 APPROVED

Ankita
 5/5/2021 10:41:50 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 04 17:42:18 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Apr 29 05:54:04 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.891	3.886	1647736	908071	15.015m	16.267
2) SA Decachlor...	10.888f	9.148f	1521000	458183	13.832	13.469

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0050421\
Data File : P0077506.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 May 2021 13:44
Operator : DD\AJ
Sample : M2253-03
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
31069


Manual Integrations
APPROVED

Ankita
5/5/2021 10:41:50 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 04 17:42:18 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042821.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Apr 29 05:54:04 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

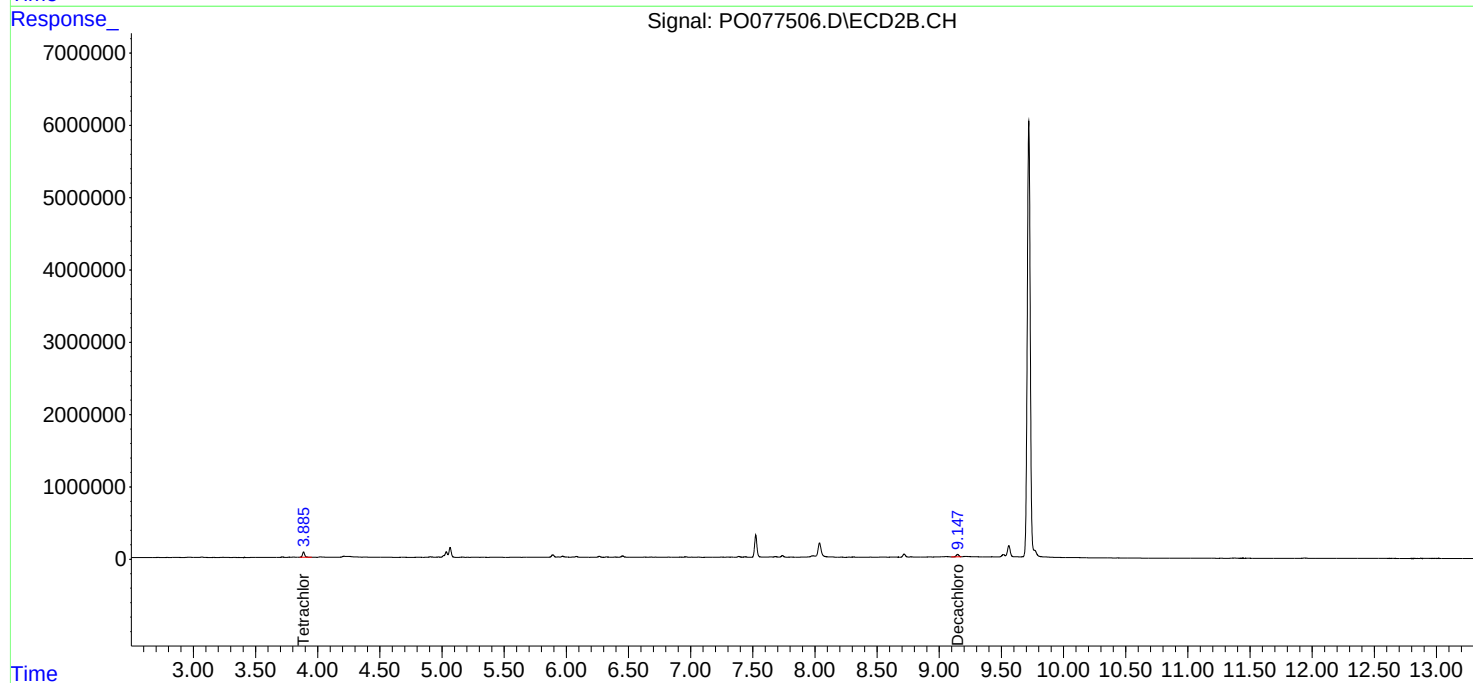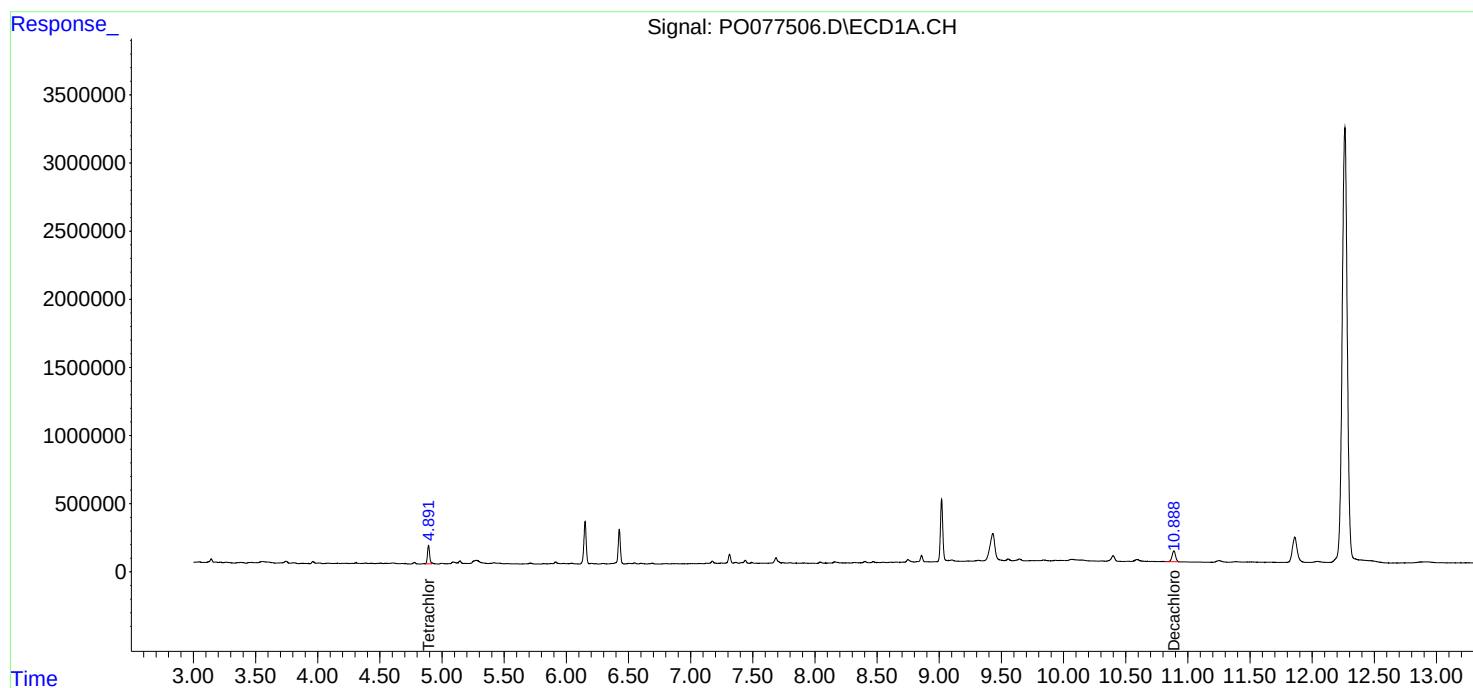

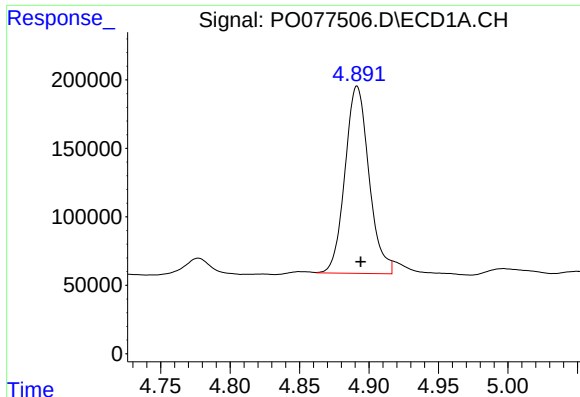


#1 Tetrachloro-m-xylene

R.T.: 4.891 min
Delta R.T.: -0.003 min
Response: 1647736
Conc: 15.02 ng/ml m

Instrument :
ECD_O
ClientSampleId :
31069


Manual Integrations
APPROVED

Ankita
5/5/2021 10:41:50 AM

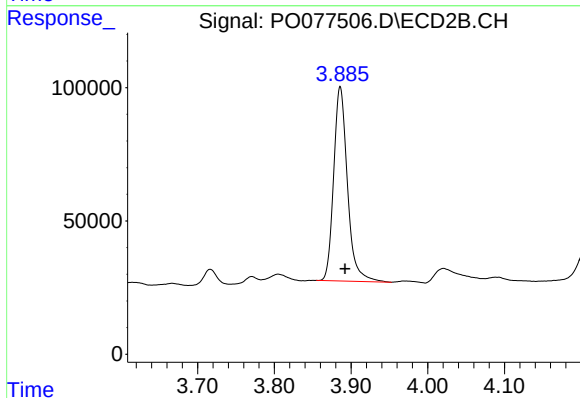


#1 Tetrachloro-m-xylene

R.T.: 3.886 min
Delta R.T.: -0.006 min
Response: 908071
Conc: 16.27 ng/ml

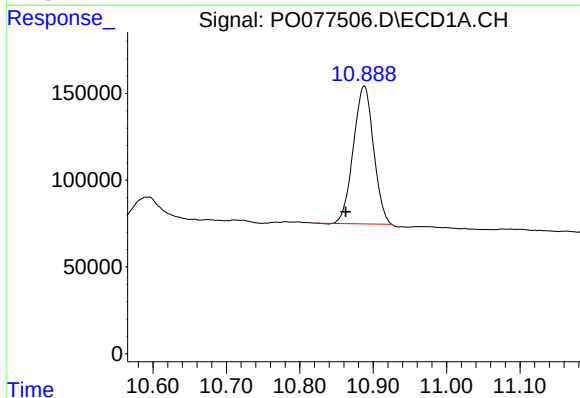

#2 Decachlorobiphenyl

R.T.: 10.888 min
Delta R.T.: 0.025 min
Response: 1521000
Conc: 13.83 ng/ml

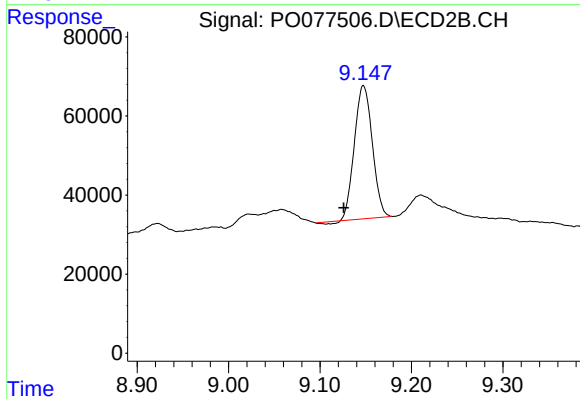

#2 Decachlorobiphenyl

R.T.: 9.148 min
Delta R.T.: 0.022 min
Response: 458183
Conc: 13.47 ng/ml