

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0050421\
 Data File : P0077507.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 May 2021 14:01
 Operator : DD\AJ
 Sample : M2254-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-1

Manual Integrations
 APPROVED

Ankita
 5/5/2021 10:41:51 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 04 17:44:22 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Apr 29 05:54:04 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.891	3.884	1428028	840577	13.013m	15.058
2) SA Decachlor...	10.858	9.120	1697746	553168	15.439	16.261
Target Compounds						
31) L7 AR-1260-1	7.901	6.699	1469108	910804	237.624	289.434
32) L7 AR-1260-2	8.168	6.897	1875054	1098686	250.320	295.455
33) L7 AR-1260-3	8.532	7.048	1104743	955183	220.671	277.687 #
34) L7 AR-1260-4	8.762	7.528	1336381	639850	244.036	267.798
35) L7 AR-1260-5	9.083	7.776	3004681	1601858	276.972	305.648

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0050421\
Data File : P0077507.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 May 2021 14:01
Operator : DD\AJ
Sample : M2254-01
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
TP-1


Manual Integrations
APPROVED

Ankita
5/5/2021 10:41:51 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 04 17:44:22 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042821.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Apr 29 05:54:04 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

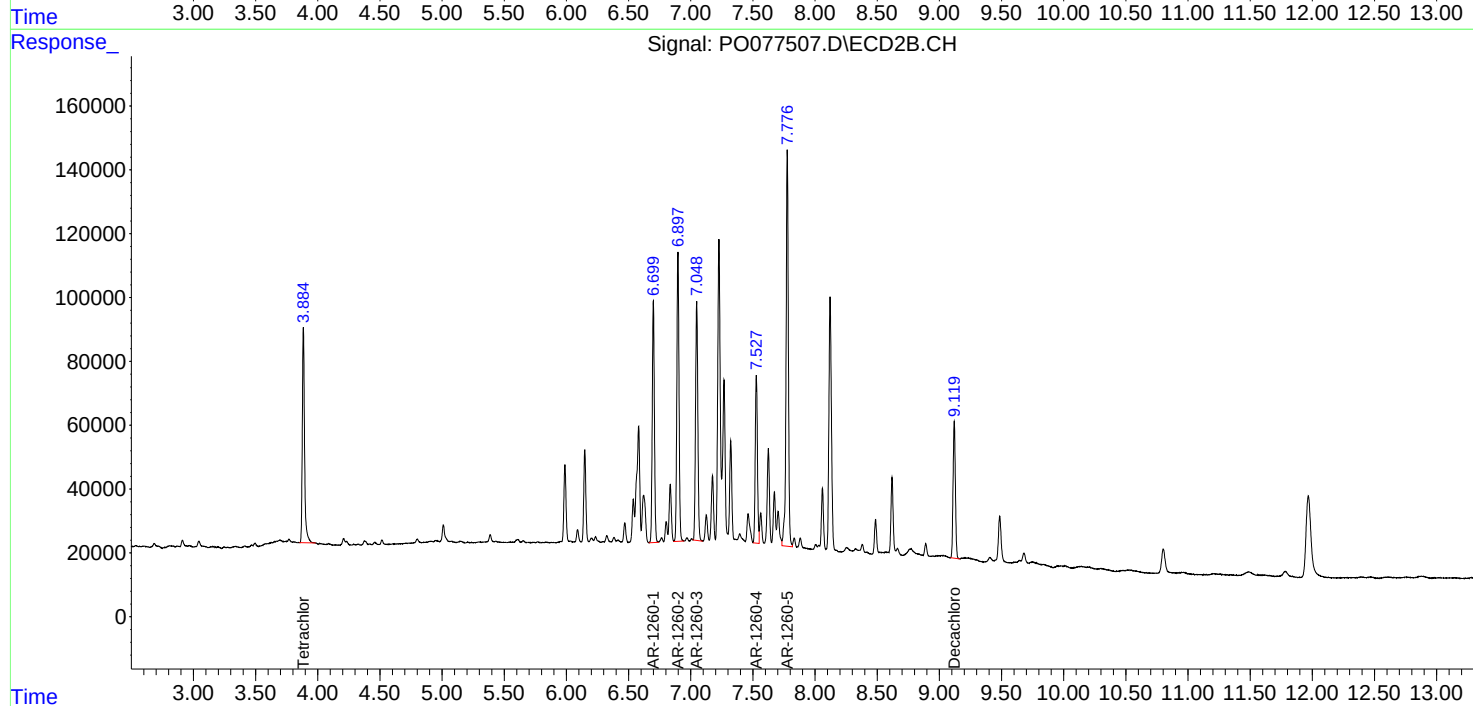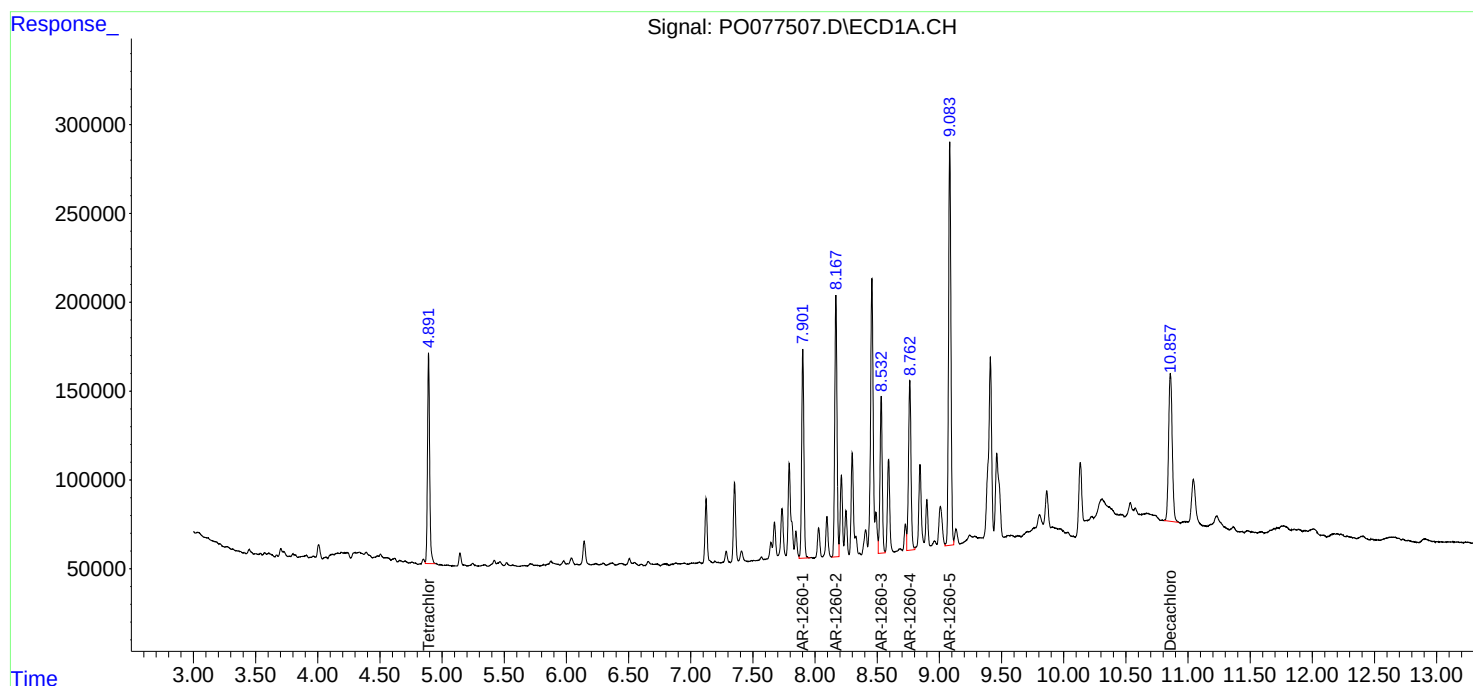

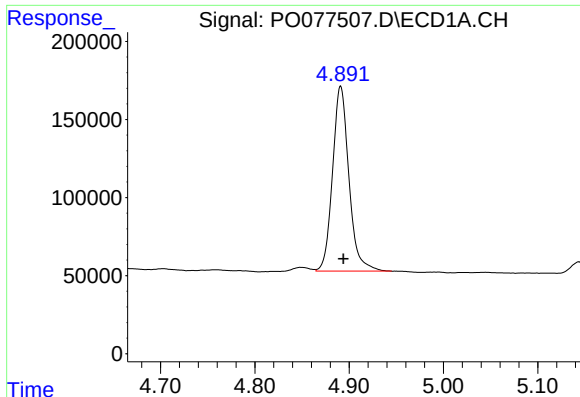


#1 Tetrachloro-m-xylene

R.T.: 4.891 min
Delta R.T.: -0.003 min
Response: 1428028
Conc: 13.01 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TP-1


Manual Integrations
APPROVED

Ankita
5/5/2021 10:41:51 AM

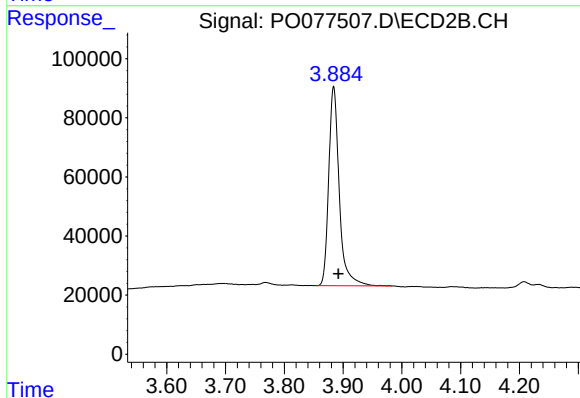


#1 Tetrachloro-m-xylene

R.T.: 3.884 min
Delta R.T.: -0.008 min
Response: 840577
Conc: 15.06 ng/ml

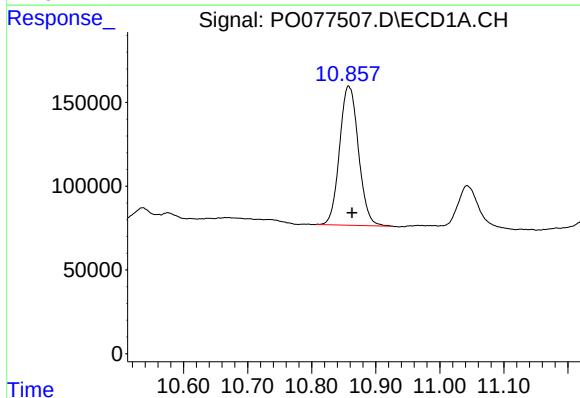


#2 Decachlorobiphenyl

R.T.: 10.858 min
Delta R.T.: -0.005 min
Response: 1697746
Conc: 15.44 ng/ml

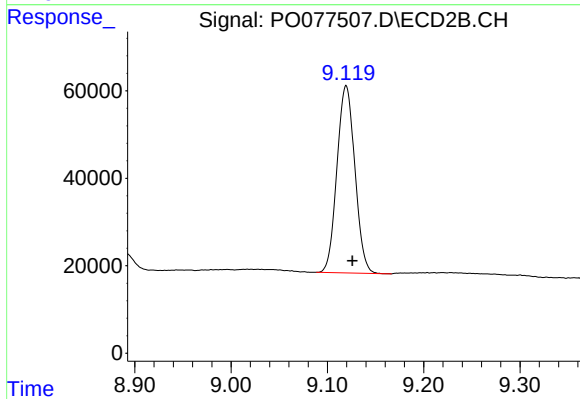

#2 Decachlorobiphenyl

R.T.: 9.120 min
Delta R.T.: -0.006 min
Response: 553168
Conc: 16.26 ng/ml

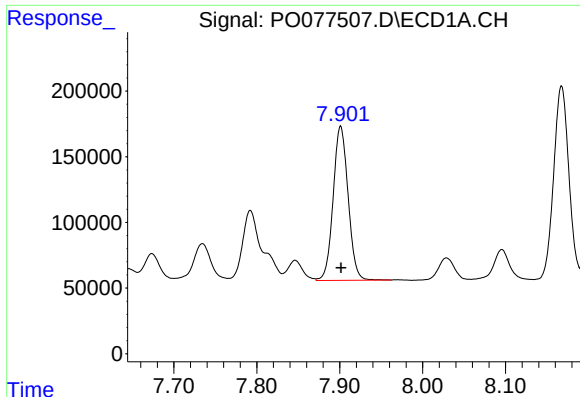


#31 AR-1260-1

R.T.: 7.901 min
Delta R.T.: 0.000 min
Response: 1469108
Conc: 237.62 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-1


Manual Integrations
APPROVED

Ankita
5/5/2021 10:41:51 AM

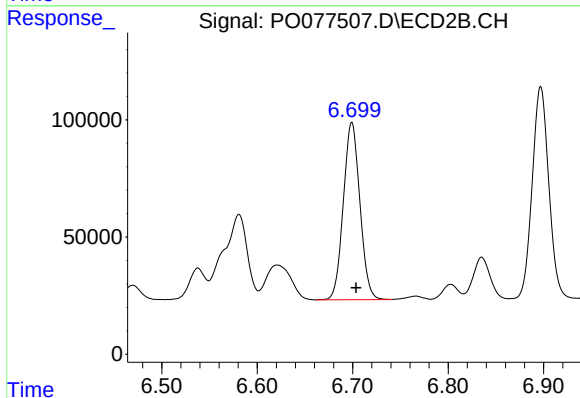


#31 AR-1260-1

R.T.: 6.699 min
Delta R.T.: -0.004 min
Response: 910804
Conc: 289.43 ng/ml

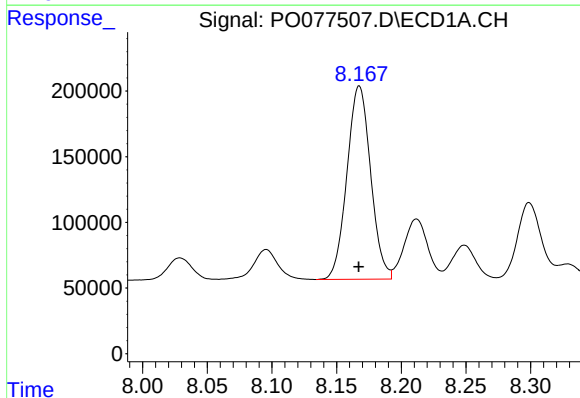


#32 AR-1260-2

R.T.: 8.168 min
Delta R.T.: 0.000 min
Response: 1875054
Conc: 250.32 ng/ml

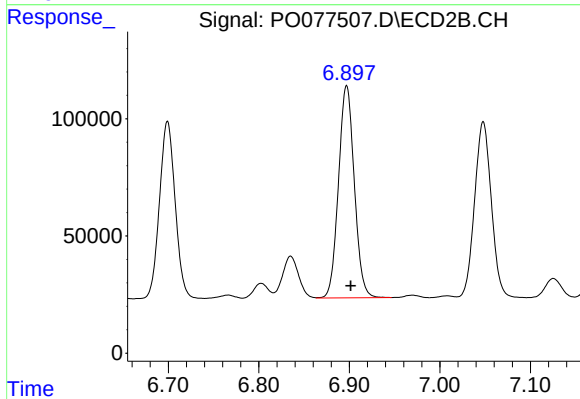

#32 AR-1260-2

R.T.: 6.897 min
Delta R.T.: -0.005 min
Response: 1098686
Conc: 295.45 ng/ml

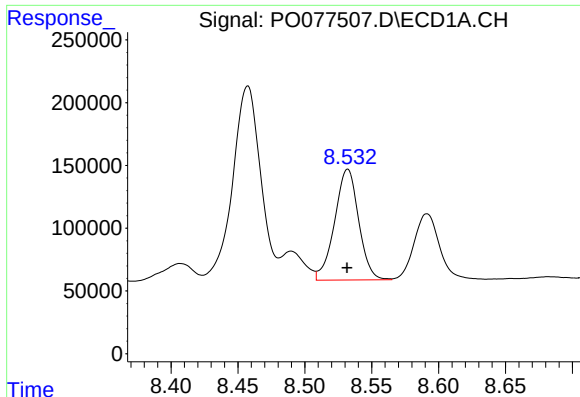


#33 AR-1260-3

R.T.: 8.532 min
Delta R.T.: 0.000 min
Response: 1104743
Conc: 220.67 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-1


Manual Integrations
APPROVED

Ankita
5/5/2021 10:41:51 AM

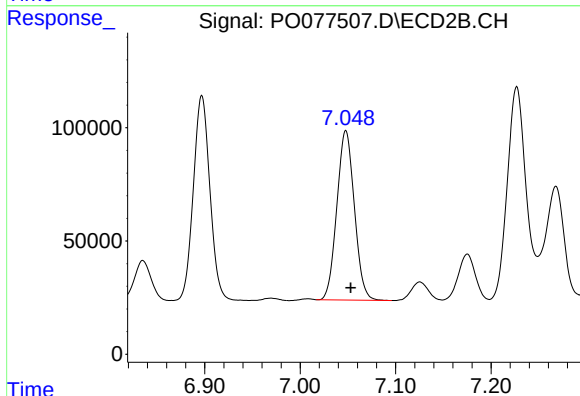


#33 AR-1260-3

R.T.: 7.048 min
Delta R.T.: -0.005 min
Response: 955183
Conc: 277.69 ng/ml

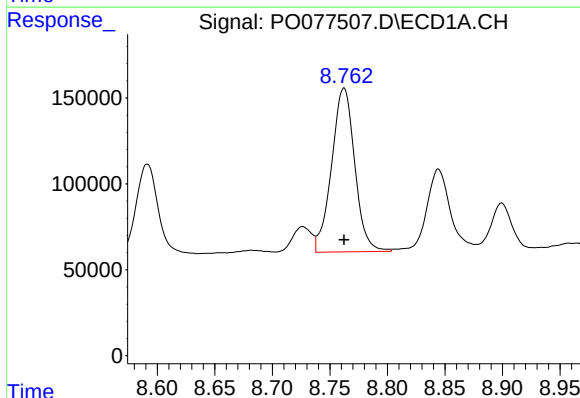


#34 AR-1260-4

R.T.: 8.762 min
Delta R.T.: 0.000 min
Response: 1336381
Conc: 244.04 ng/ml

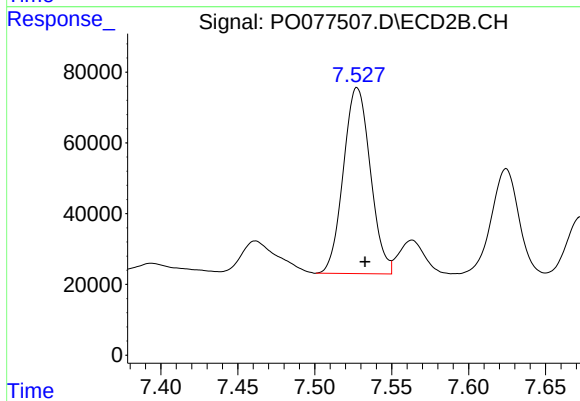

#34 AR-1260-4

R.T.: 7.528 min
Delta R.T.: -0.005 min
Response: 639850
Conc: 267.80 ng/ml

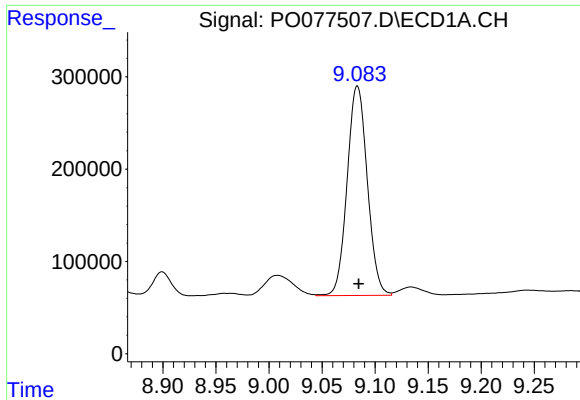


#35 AR-1260-5

R.T.: 9.083 min
Delta R.T.: -0.001 min
Response: 3004681
Conc: 276.97 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-1

Manual Integrations
APPROVED

Ankita
5/5/2021 10:41:51 AM

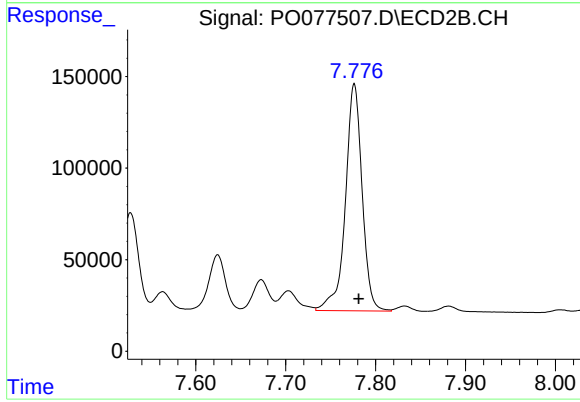

#35 AR-1260-5

R.T.: 7.776 min
Delta R.T.: -0.005 min
Response: 1601858
Conc: 305.65 ng/ml