

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0050423\
 Data File : P0094730.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 May 2023 13:24
 Operator : YP/AJ
 Sample : 02598-04
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ETGI-328

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/05/2023
 Supervised By :Ankita Jodhani 05/05/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 04 18:22:42 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042623.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon May 01 11:12:50 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.415	3.617	69327418	26636504	20.126	19.907
2) SA Decachlor...	10.255	8.629	44526314	18339379	18.347m	16.293m
Target Compounds						
26) L6 AR-1254-1	6.463	5.501	21419931	8760625	169.063	120.851m#
27) L6 AR-1254-2	6.682	5.646	18862375	3530461	98.686	54.107m#
28) L6 AR-1254-3	7.049	6.050	17776861	7219812	94.249	72.707m
29) L6 AR-1254-4	7.337	6.281	6239332	2759374	55.089m	55.904
30) L6 AR-1254-5	7.760	6.698	10842444	6836340	77.420m	81.258

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO050423\
Data File : PO094730.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 May 2023 13:24
Operator : YP/AJ
Sample : 02598-04
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
ETGI-328


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/05/2023
Supervised By :Ankita Jodhani 05/05/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 04 18:22:42 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO042623.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon May 01 11:12:50 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

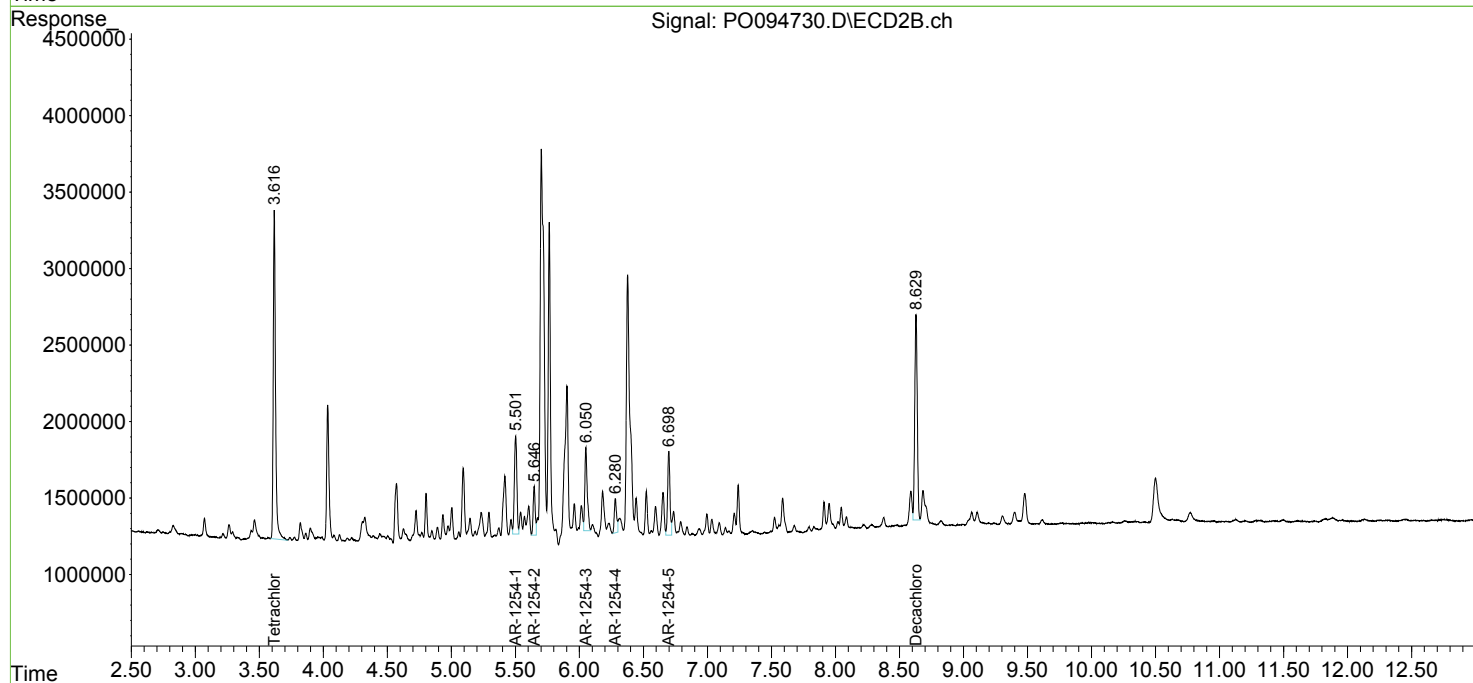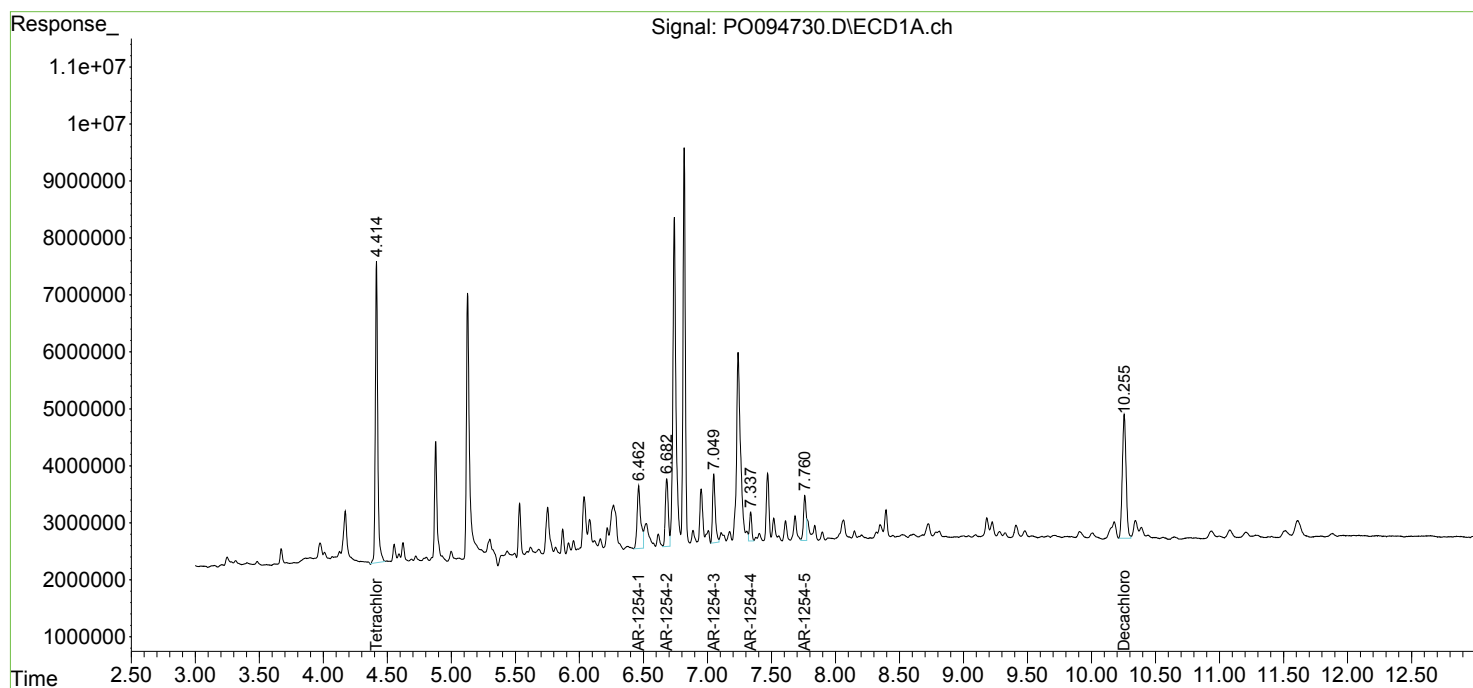

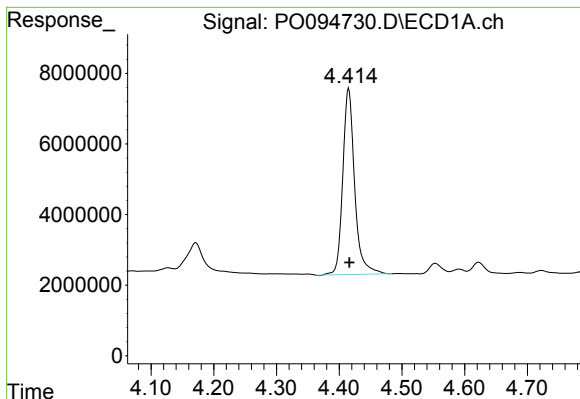


#1 Tetrachloro-m-xylene

R.T.: 4.415 min
Delta R.T.: 0.000 min
Response: 69327418
Conc: 20.13 ng/ml

Instrument :
ECD_O
ClientSampleId :
ETGI-328


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/05/2023
Supervised By :Ankita Jodhani 05/05/2023

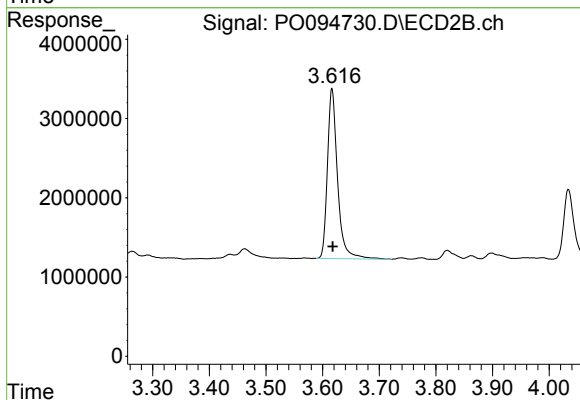


#1 Tetrachloro-m-xylene

R.T.: 3.617 min
Delta R.T.: -0.001 min
Response: 26636504
Conc: 19.91 ng/ml

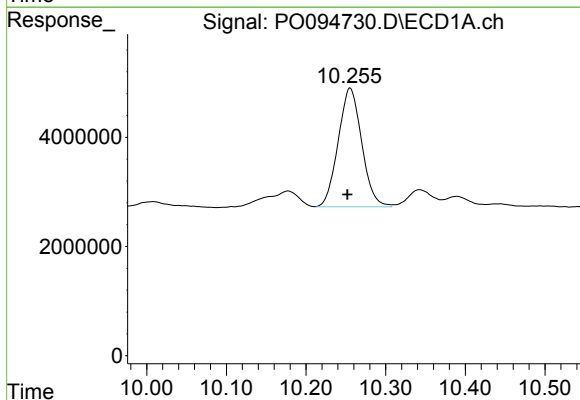


#2 Decachlorobiphenyl

R.T.: 10.255 min
Delta R.T.: 0.003 min
Response: 44526314
Conc: 18.35 ng/ml m

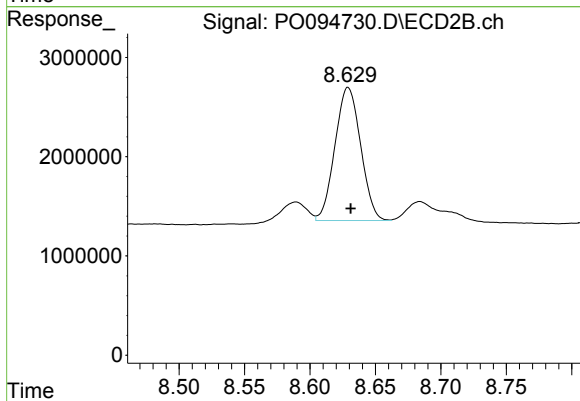

#2 Decachlorobiphenyl

R.T.: 8.629 min
Delta R.T.: -0.003 min
Response: 18339379
Conc: 16.29 ng/ml m

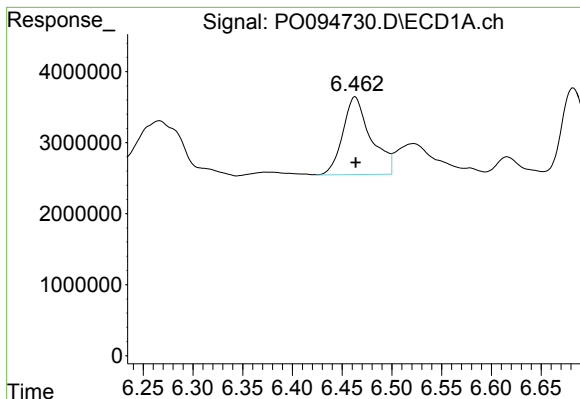


#26 AR-1254-1

R.T.: 6.463 min
Delta R.T.: 0.000 min
Response: 21419931
Conc: 169.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
ETGI-328


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/05/2023
Supervised By :Ankita Jodhani 05/05/2023

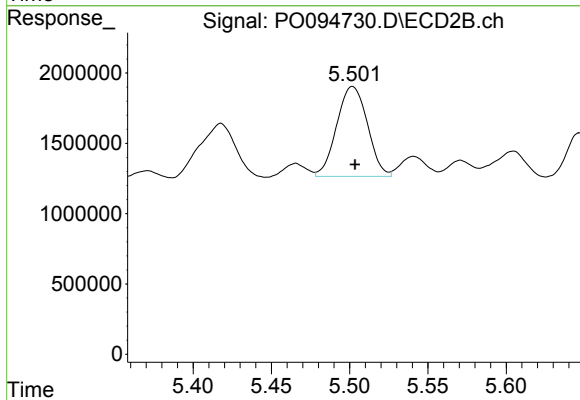


#26 AR-1254-1

R.T.: 5.501 min
Delta R.T.: -0.002 min
Response: 8760625
Conc: 120.85 ng/ml m

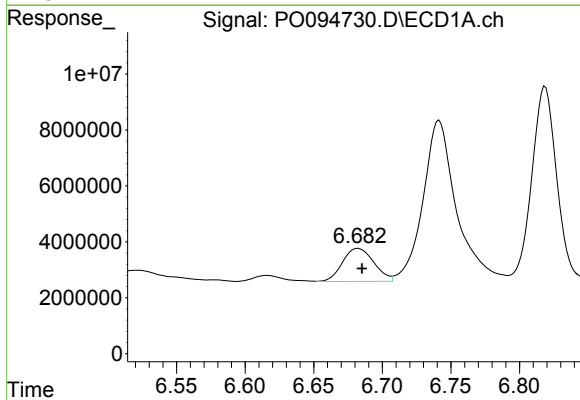


#27 AR-1254-2

R.T.: 6.682 min
Delta R.T.: -0.003 min
Response: 18862375
Conc: 98.69 ng/ml

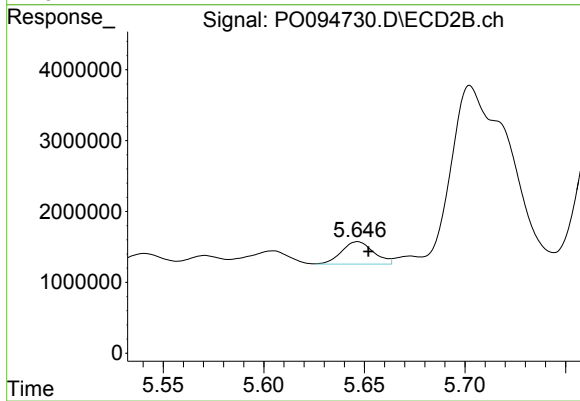

#27 AR-1254-2

R.T.: 5.646 min
Delta R.T.: -0.006 min
Response: 3530461
Conc: 54.11 ng/ml m

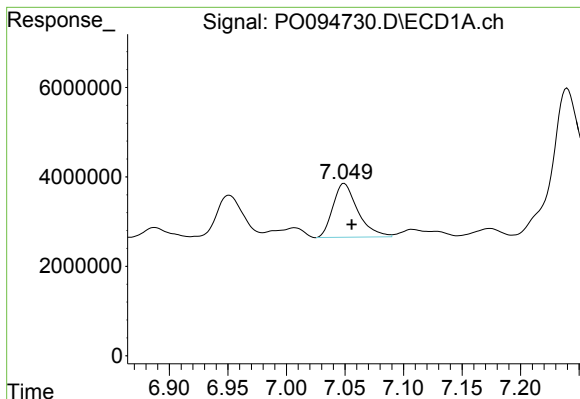


#28 AR-1254-3

R.T.: 7.049 min
Delta R.T.: -0.006 min
Response: 17776861
Conc: 94.25 ng/ml

Instrument :
ECD_O
ClientSampleId :
ETGI-328


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/05/2023
Supervised By :Ankita Jodhani 05/05/2023

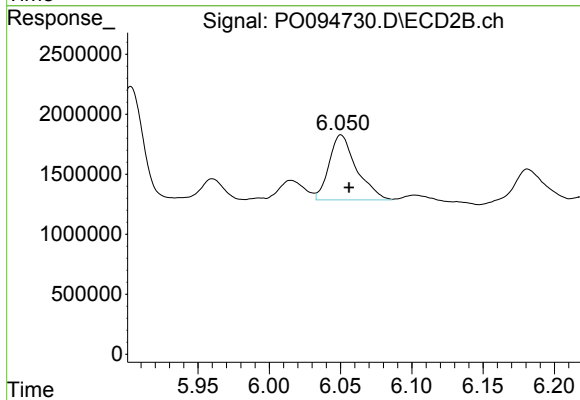


#28 AR-1254-3

R.T.: 6.050 min
Delta R.T.: -0.006 min
Response: 7219812
Conc: 72.71 ng/ml m

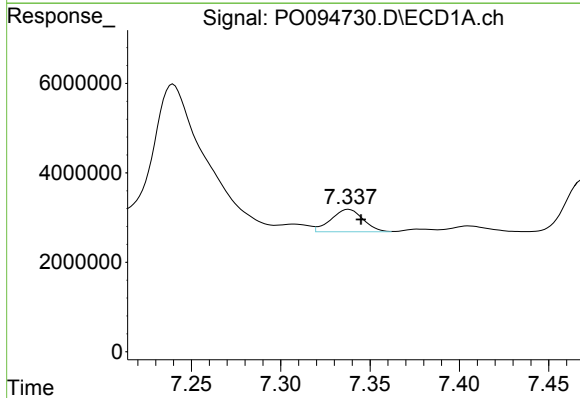


#29 AR-1254-4

R.T.: 7.337 min
Delta R.T.: -0.008 min
Response: 6239332
Conc: 55.09 ng/ml m

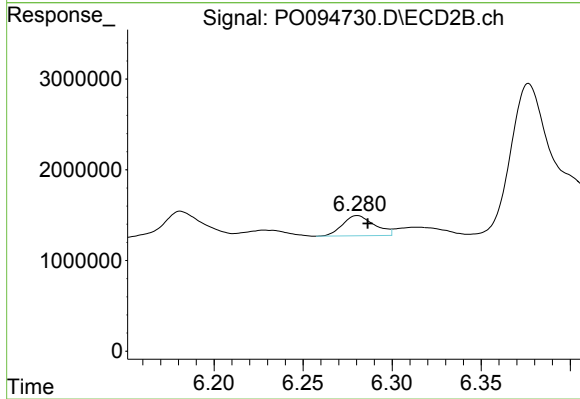

#29 AR-1254-4

R.T.: 6.281 min
Delta R.T.: -0.006 min
Response: 2759374
Conc: 55.90 ng/ml

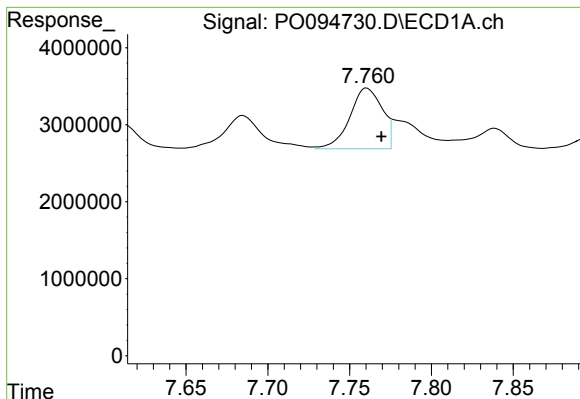


#30 AR-1254-5

R.T.: 7.760 min
Delta R.T.: -0.010 min
Response: 10842444
Conc: 77.42 ng/ml

Instrument :
ECD_O
ClientSampleId :
ETGI-328

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/05/2023
Supervised By :Ankita Jodhani 05/05/2023

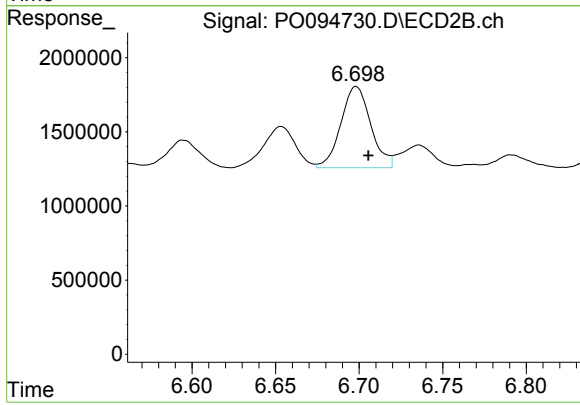

#30 AR-1254-5

R.T.: 6.698 min
Delta R.T.: -0.007 min
Response: 6836340
Conc: 81.26 ng/ml