

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0050423\
 Data File : P0094753.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 May 2023 20:08
 Operator : YP/AJ
 Sample : 02588-14
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PILE-A-UNK-05022023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 04 21:16:19 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042623.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon May 01 11:12:50 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.414	3.616	65769888	26943378	19.094	20.136
2) SA Decachlor...	10.252	8.627	49609359	21214308	20.442	18.847

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO050423\
Data File : PO094753.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 May 2023 20:08
Operator : YP/AJ
Sample : 02588-14
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PILE-A-UNK-05022023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 04 21:16:19 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO042623.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon May 01 11:12:50 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

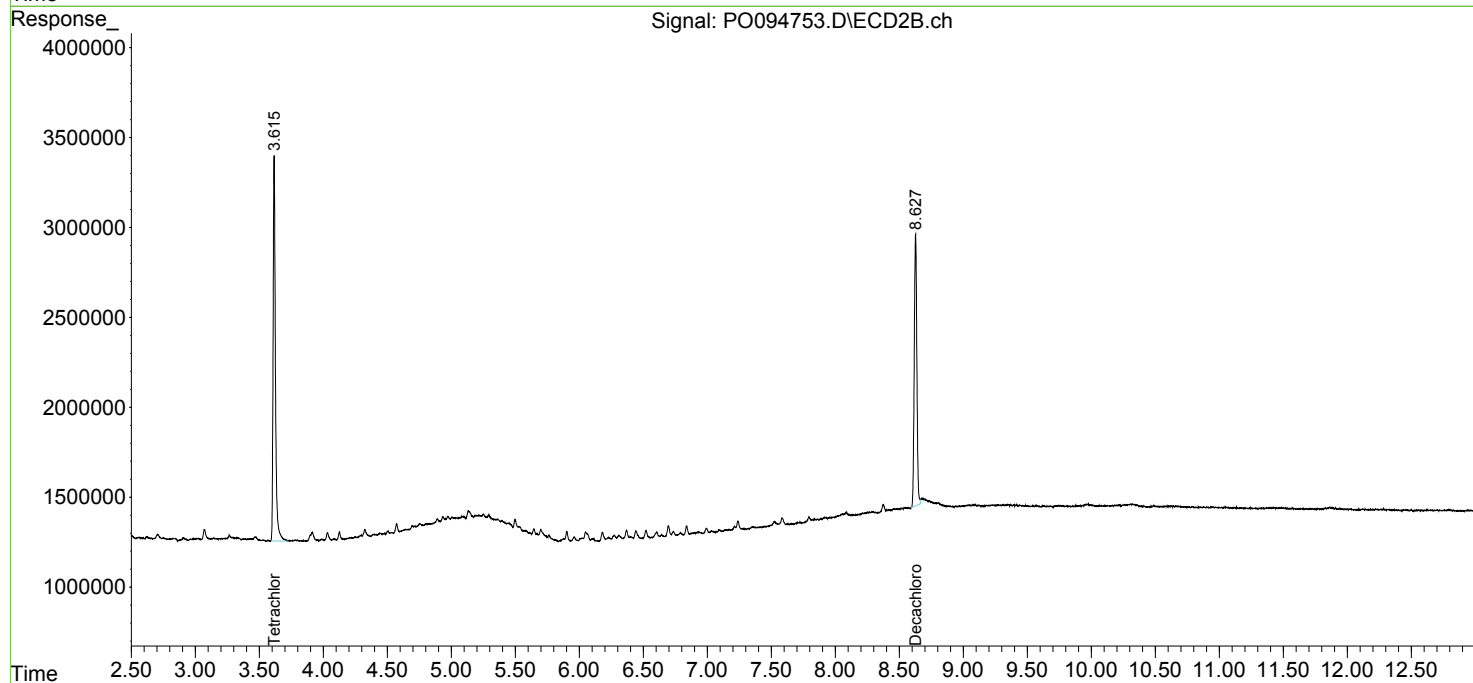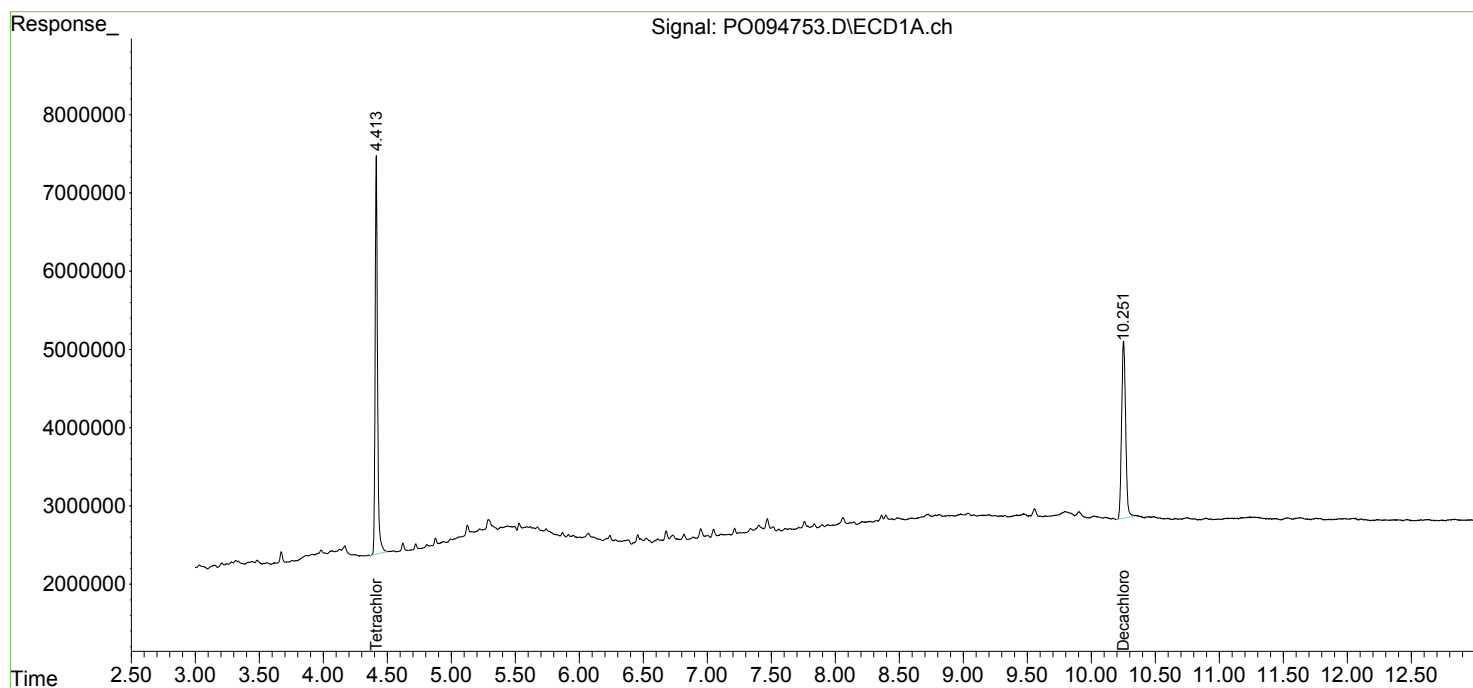


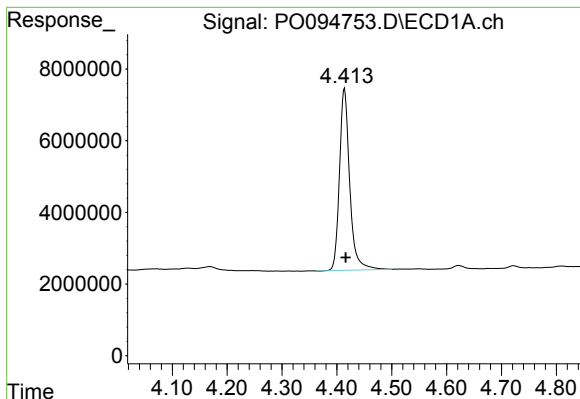

#1 Tetrachloro-m-xylene


R.T.: 4.414 min
Delta R.T.: -0.002 min
Response: 65769888
Conc: 19.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
PILE-A-UNK-05022023

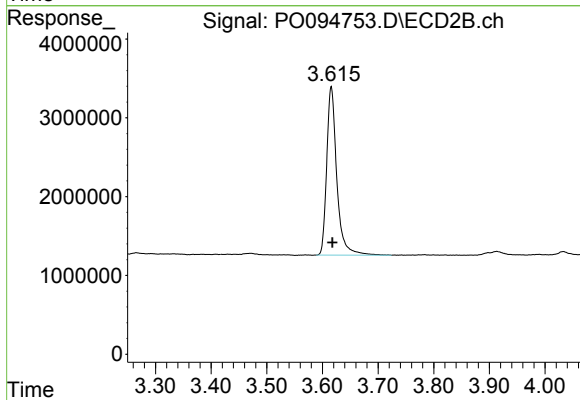


#1 Tetrachloro-m-xylene

R.T.: 3.616 min
Delta R.T.: -0.002 min
Response: 26943378
Conc: 20.14 ng/ml

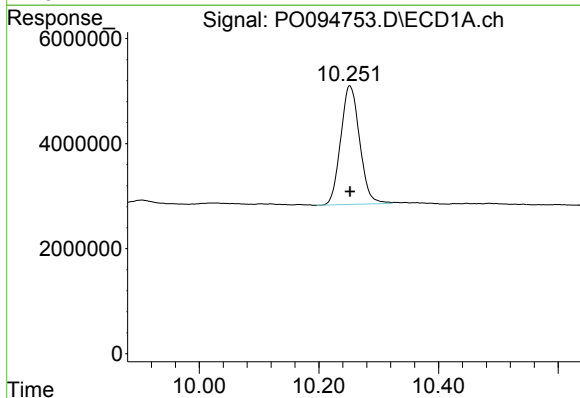

#2 Decachlorobiphenyl

R.T.: 10.252 min
Delta R.T.: 0.000 min
Response: 49609359
Conc: 20.44 ng/ml

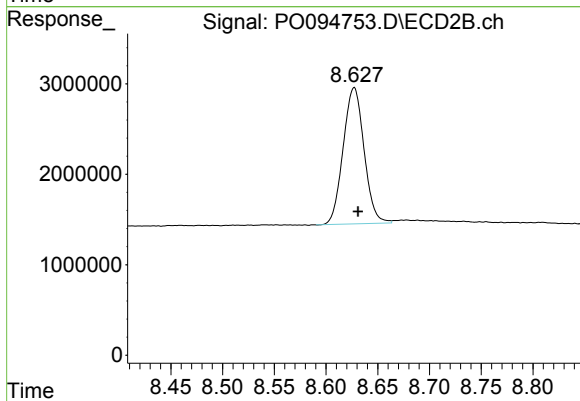

#2 Decachlorobiphenyl

R.T.: 8.627 min
Delta R.T.: -0.004 min
Response: 21214308
Conc: 18.85 ng/ml