

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0050521\
 Data File : P0077528.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 May 2021 10:53
 Operator : DD\AJ
 Sample : M2252-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 STONE-1

Manual Integrations
 APPROVED

Ankita
 5/6/2021 4:14:54 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 05 12:30:49 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Apr 29 05:54:04 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.891	3.886	1586578	578723	14.458m	10.367 #
2) SA Decachlor...	10.866	9.132	1484487	481625	13.500m	14.158m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0050521\
Data File : P0077528.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 May 2021 10:53
Operator : DD\AJ
Sample : M2252-01
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
STONE-1


Manual Integrations
APPROVED

Ankita
5/6/2021 4:14:54 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 05 12:30:49 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042821.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Apr 29 05:54:04 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

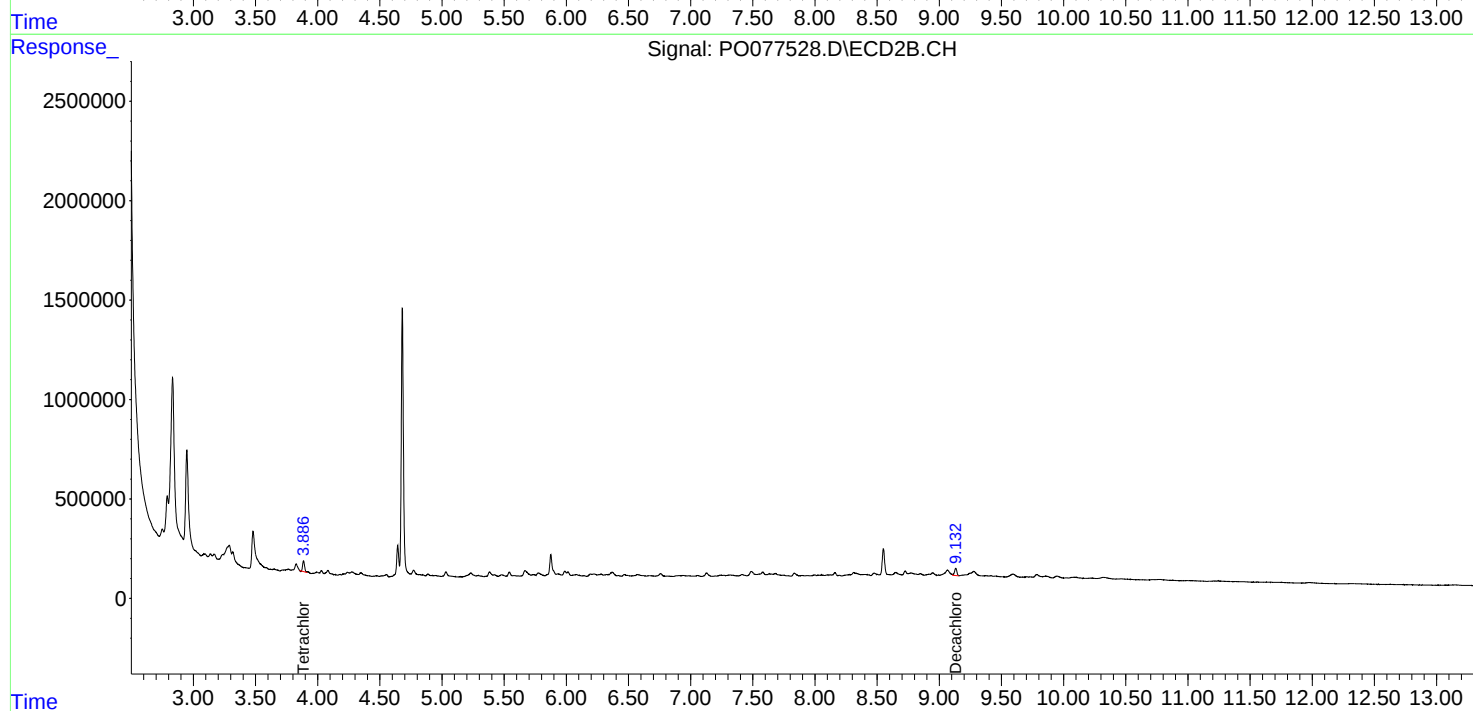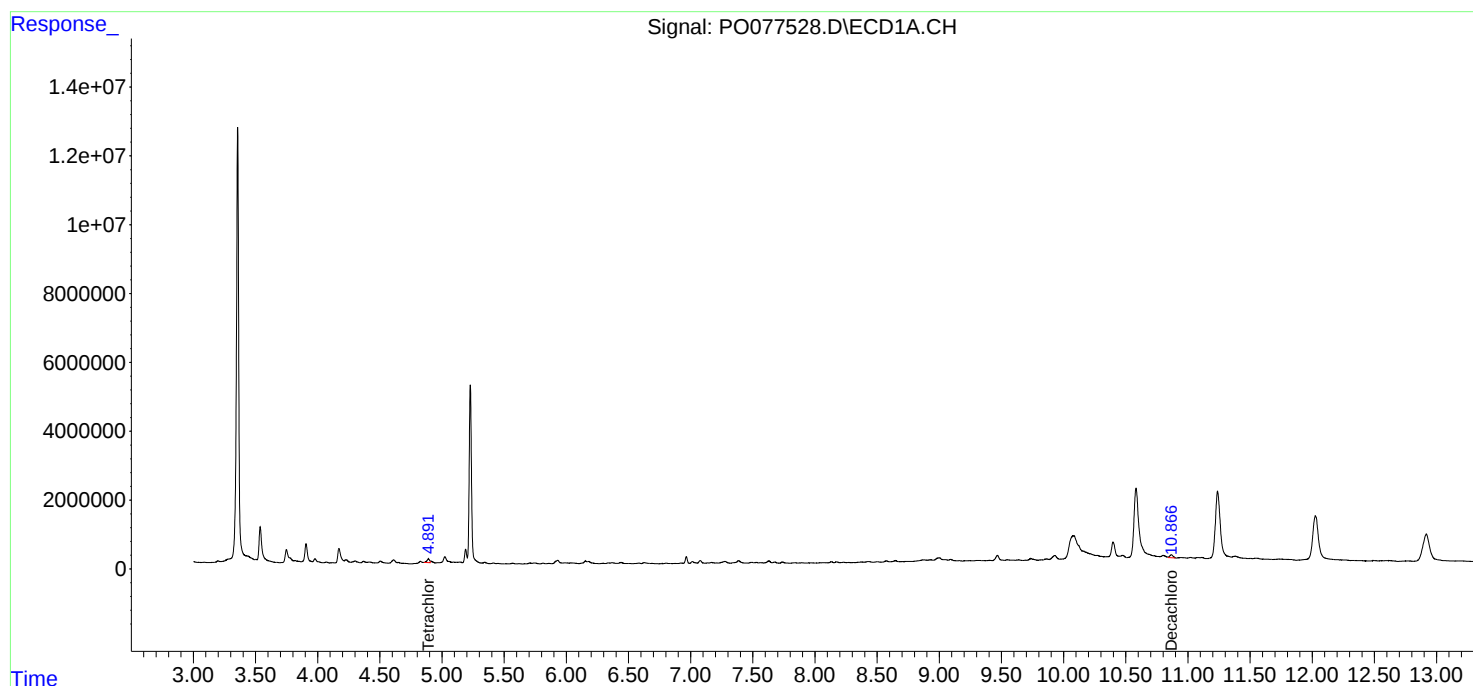

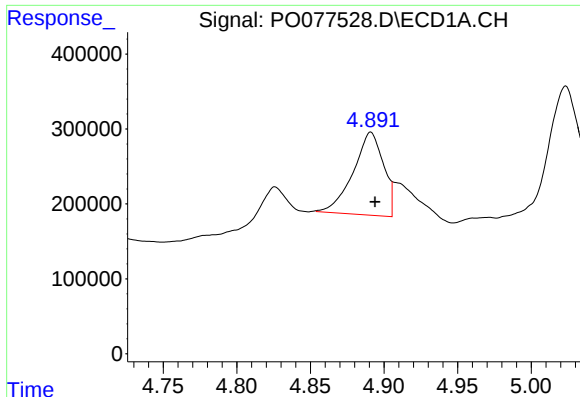


#1 Tetrachloro-m-xylene

R.T.: 4.891 min
Delta R.T.: -0.003 min
Response: 1586578
Conc: 14.46 ng/ml m

Instrument :
ECD_O
ClientSampleId :
STONE-1


Manual Integrations
APPROVED

Ankita
5/6/2021 4:14:54 PM

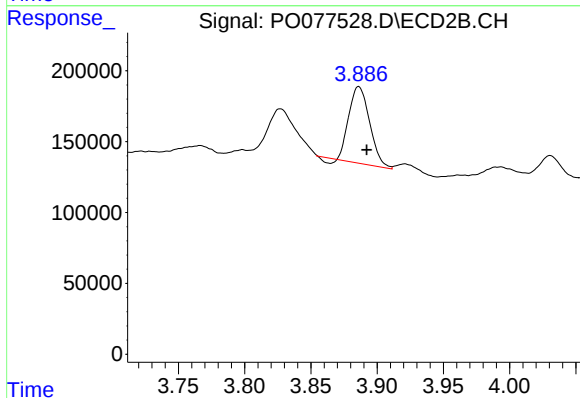


#1 Tetrachloro-m-xylene

R.T.: 3.886 min
Delta R.T.: -0.006 min
Response: 578723
Conc: 10.37 ng/ml

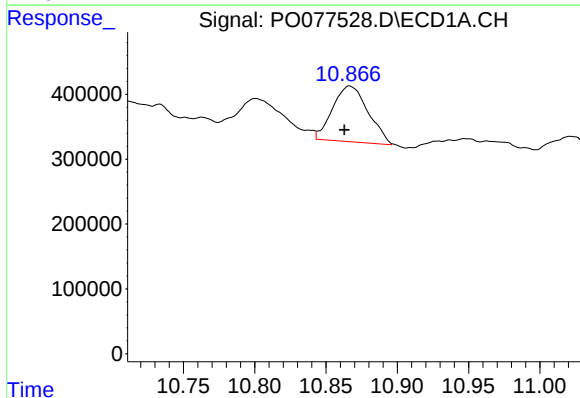

#2 Decachlorobiphenyl

R.T.: 10.866 min
Delta R.T.: 0.003 min
Response: 1484487
Conc: 13.50 ng/ml m

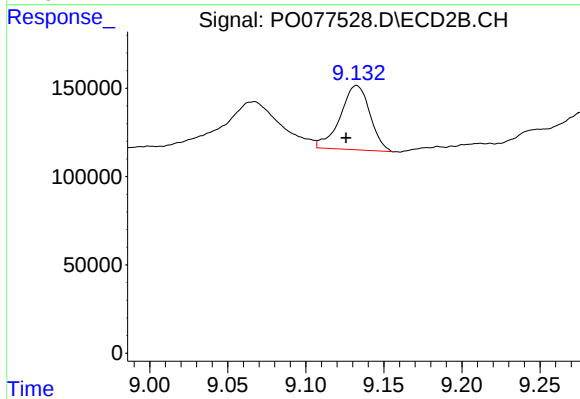

#2 Decachlorobiphenyl

R.T.: 9.132 min
Delta R.T.: 0.006 min
Response: 481625
Conc: 14.16 ng/ml m