

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0050521\
 Data File : P0077532.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 May 2021 12:02
 Operator : DD\AJ
 Sample : M2273-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 HIA632R-1-1

Manual Integrations
 APPROVED

Ankita
 5/6/2021 4:14:58 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 05 12:32:35 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Apr 29 05:54:04 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.894	3.887	2039833	948711	18.589	16.995m
2) SA Decachlor...	10.876	9.139	1692088	524978	15.388	15.432

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0050521\
Data File : P0077532.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 May 2021 12:02
Operator : DD\AJ
Sample : M2273-01
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
HIA632R-1-1


Manual Integrations
APPROVED

Ankita
5/6/2021 4:14:58 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 05 12:32:35 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042821.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Apr 29 05:54:04 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

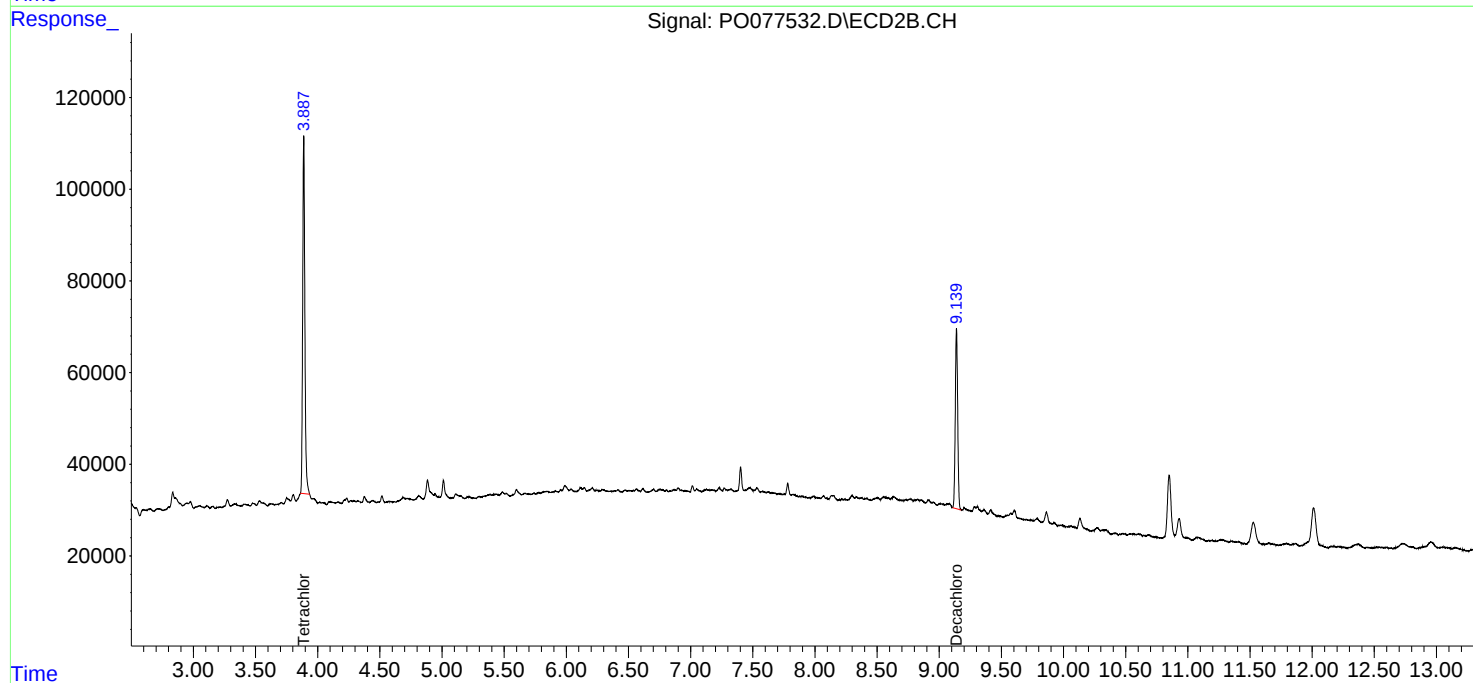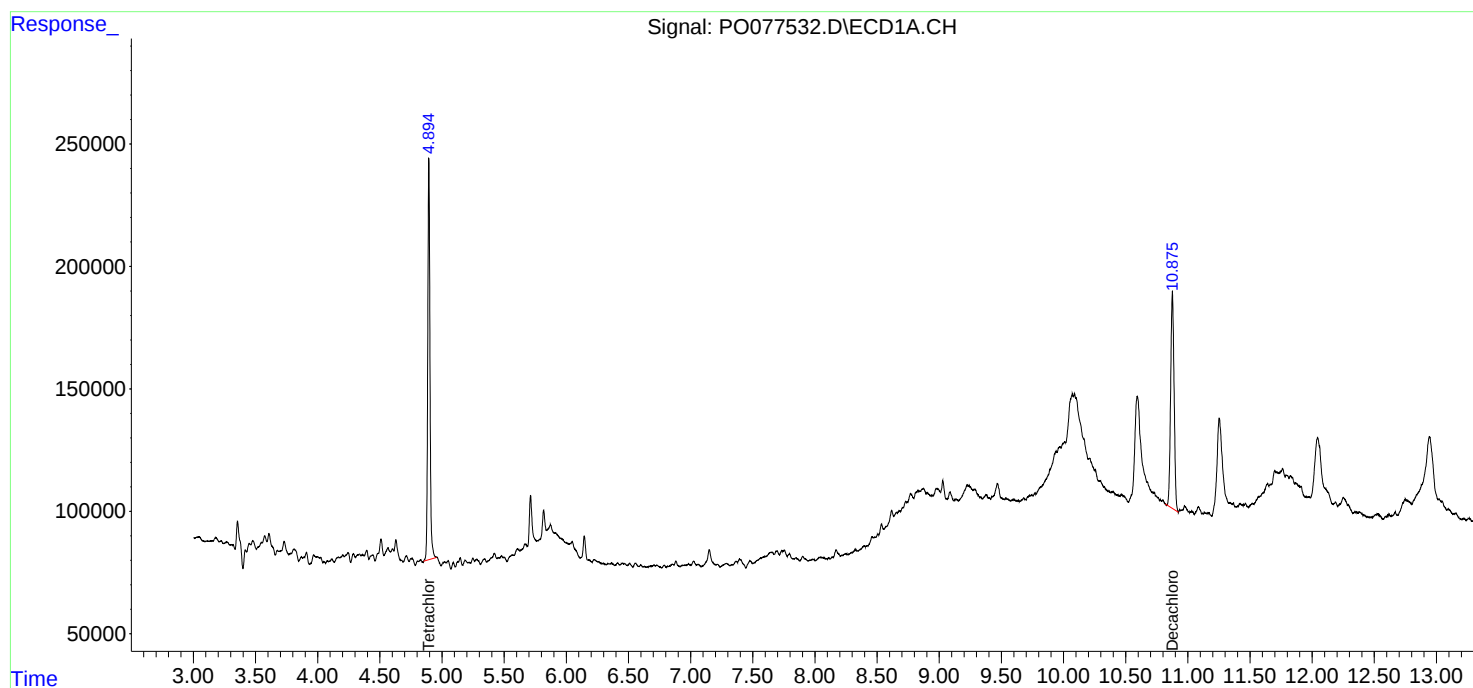

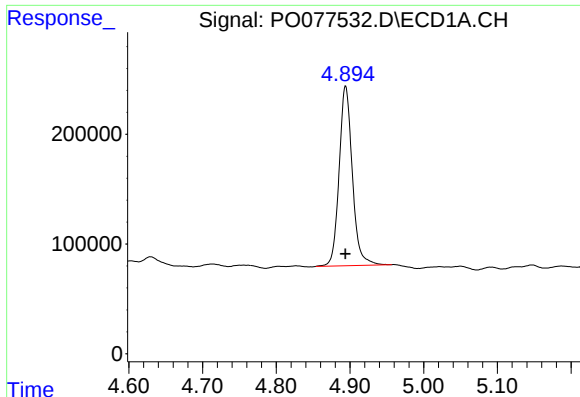


#1 Tetrachloro-m-xylene

R.T.: 4.894 min
Delta R.T.: 0.000 min
Response: 2039833
Conc: 18.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
HIA632R-1-1


Manual Integrations
APPROVED

Ankita
5/6/2021 4:14:58 PM

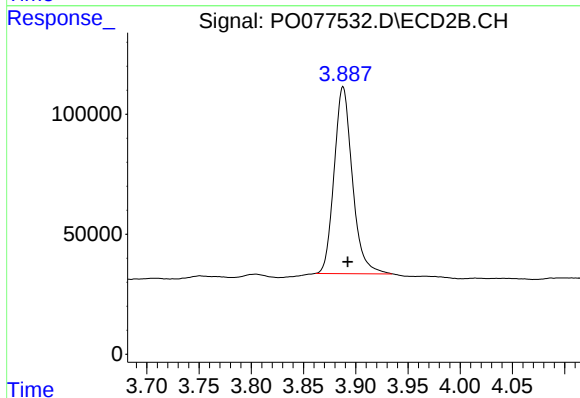


#1 Tetrachloro-m-xylene

R.T.: 3.887 min
Delta R.T.: -0.005 min
Response: 948711
Conc: 17.00 ng/ml m

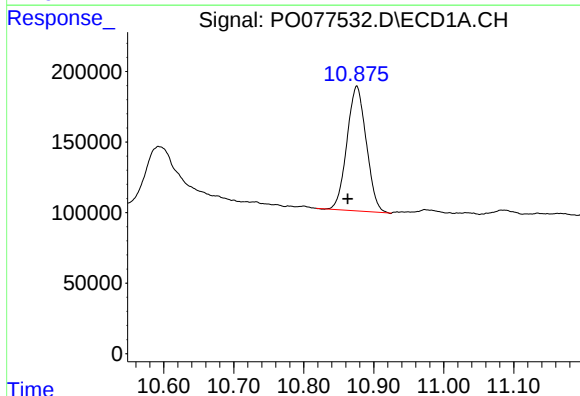

#2 Decachlorobiphenyl

R.T.: 10.876 min
Delta R.T.: 0.013 min
Response: 1692088
Conc: 15.39 ng/ml

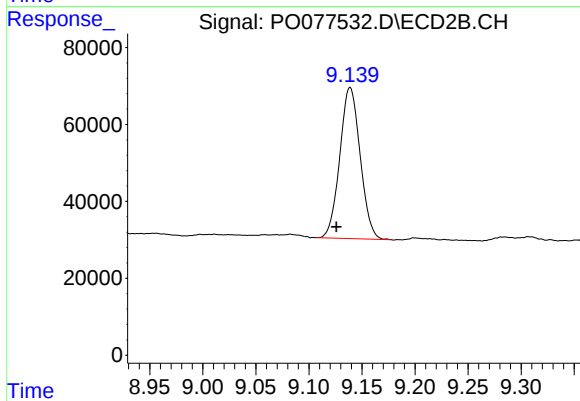

#2 Decachlorobiphenyl

R.T.: 9.139 min
Delta R.T.: 0.013 min
Response: 524978
Conc: 15.43 ng/ml