

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0050521\
 Data File : P0077535.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 May 2021 12:53
 Operator : DD\AJ
 Sample : M2273-06
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FCA557N-1-2

Manual Integrations
 APPROVED

Ankita
 5/6/2021 4:15:01 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 05 13:22:23 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Apr 29 05:54:04 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.899	3.890	1294129	840579	11.793	15.058m#
2) SA Decachlor...	10.891f	9.151f	1415905	480356	12.876	14.120m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0050521\
Data File : P0077535.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 May 2021 12:53
Operator : DD\AJ
Sample : M2273-06
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
FCA557N-1-2


Manual Integrations
APPROVED

Ankita
5/6/2021 4:15:01 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 05 13:22:23 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042821.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Apr 29 05:54:04 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

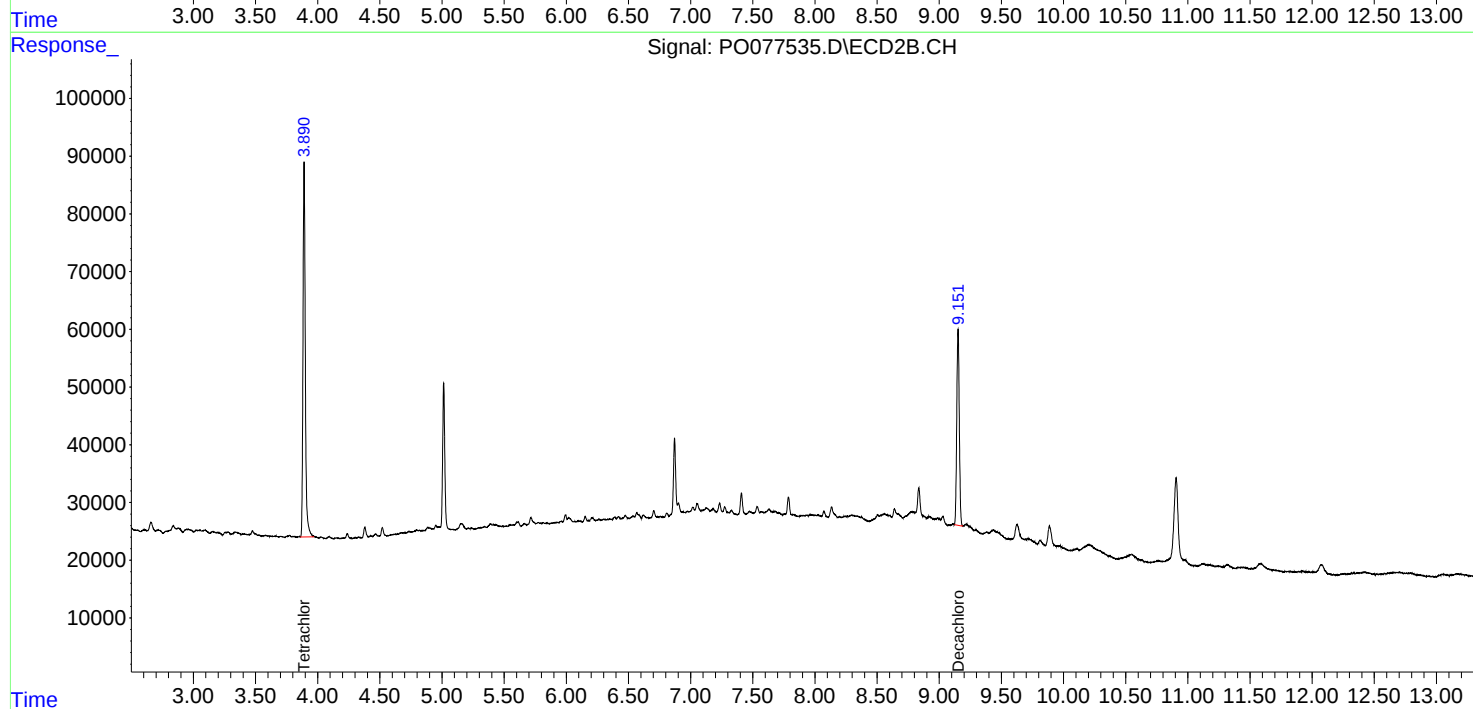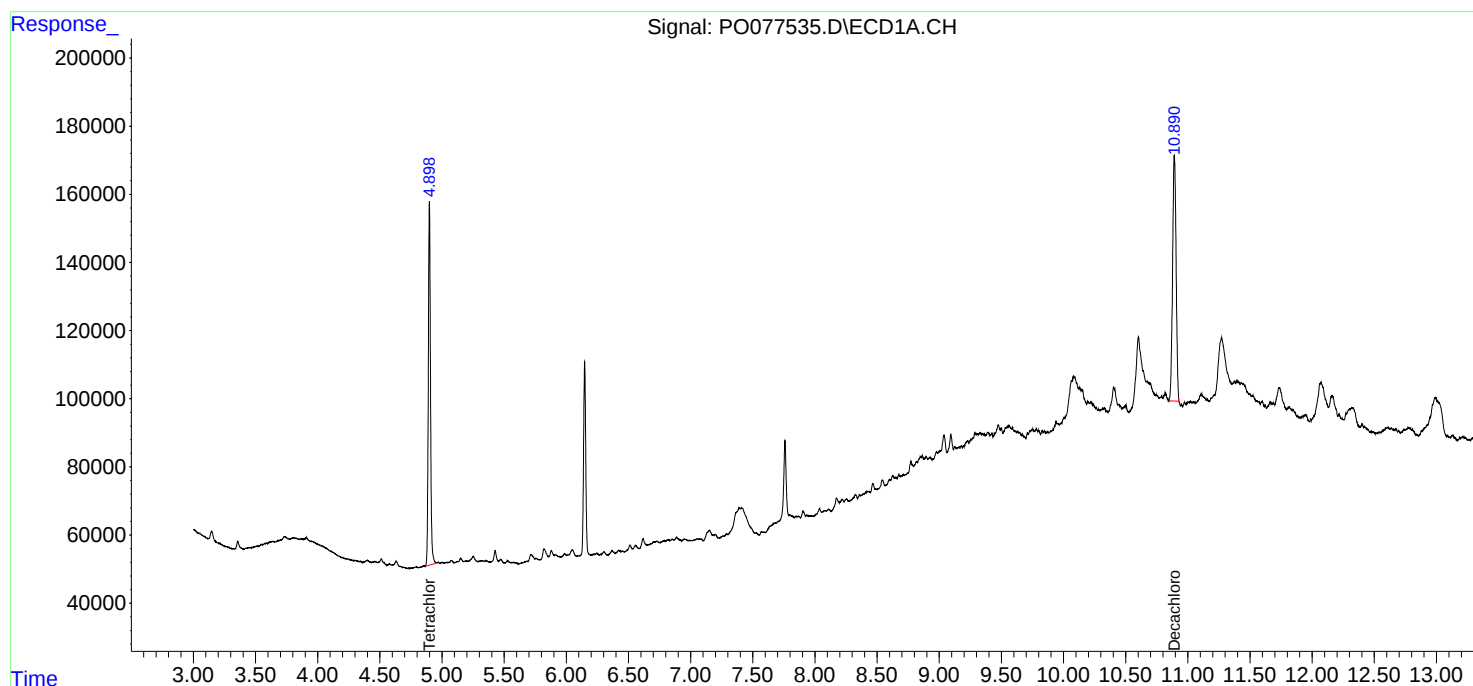

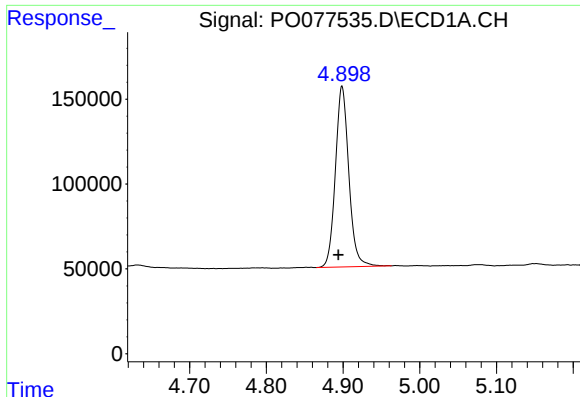


#1 Tetrachloro-m-xylene

R.T.: 4.899 min
Delta R.T.: 0.005 min
Response: 1294129
Conc: 11.79 ng/ml

Instrument :
ECD_O
ClientSampleId :
FCA557N-1-2


Manual Integrations
APPROVED

Ankita
5/6/2021 4:15:01 PM

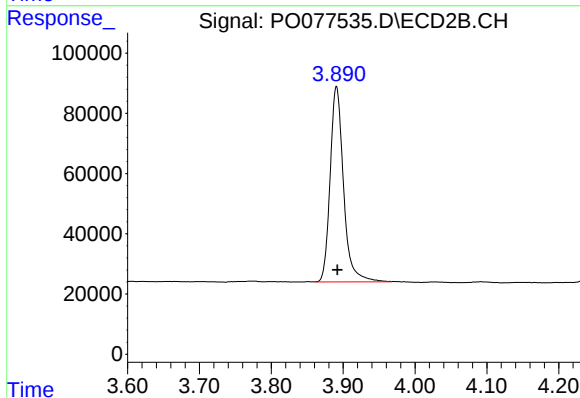


#1 Tetrachloro-m-xylene

R.T.: 3.890 min
Delta R.T.: -0.002 min
Response: 840579
Conc: 15.06 ng/ml m

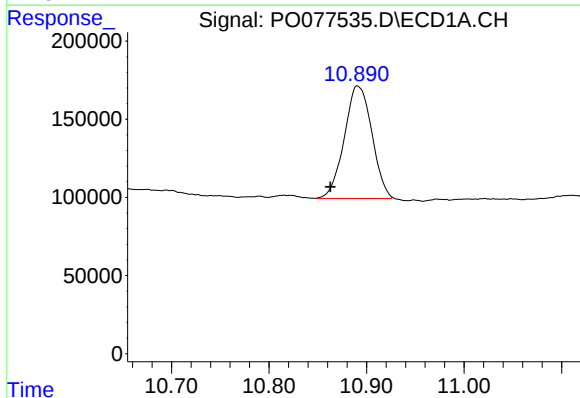

#2 Decachlorobiphenyl

R.T.: 10.891 min
Delta R.T.: 0.028 min
Response: 1415905
Conc: 12.88 ng/ml

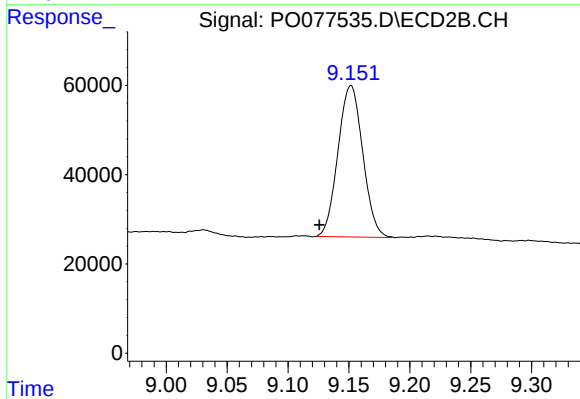

#2 Decachlorobiphenyl

R.T.: 9.151 min
Delta R.T.: 0.026 min
Response: 480356
Conc: 14.12 ng/ml m