

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0050619\
 Data File : P0055882.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 May 2019 10:59
 Operator : SM/SJ
 Sample : K2538-06RE 10X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 NB-20523RE

Manual Integrations
 APPROVED

Ankita
 5/7/2019 1:14:43 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 07 01:15:36 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 03 15:20:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.274	3.585	123602	120788	4.130	4.277m
2) SA Decachlor...	9.826	8.537	101348	96738	2.709	3.577 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0050619\
Data File : P0055882.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 May 2019 10:59
Operator : SM/SJ
Sample : K2538-06RE 10X
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
NB-20523RE


Manual Integrations
APPROVED

Ankita
5/7/2019 1:14:43 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 07 01:15:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 03 15:20:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

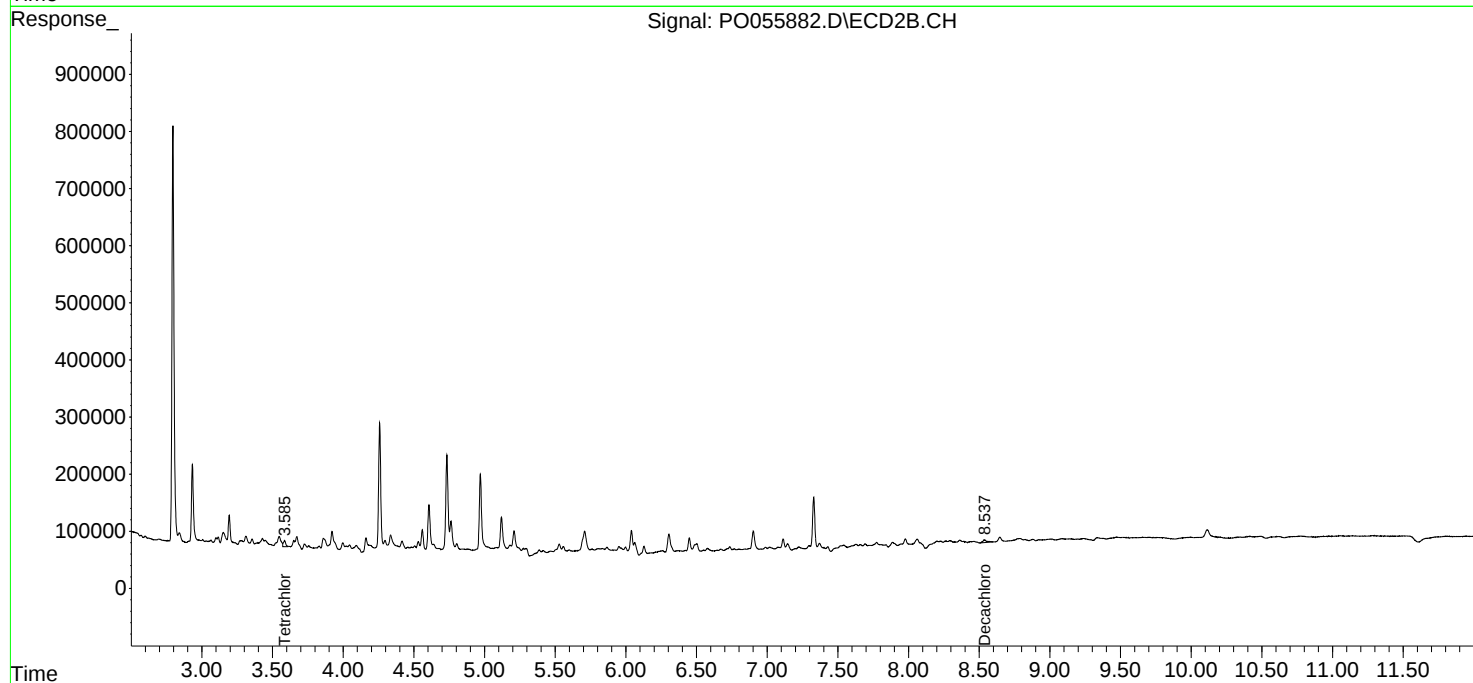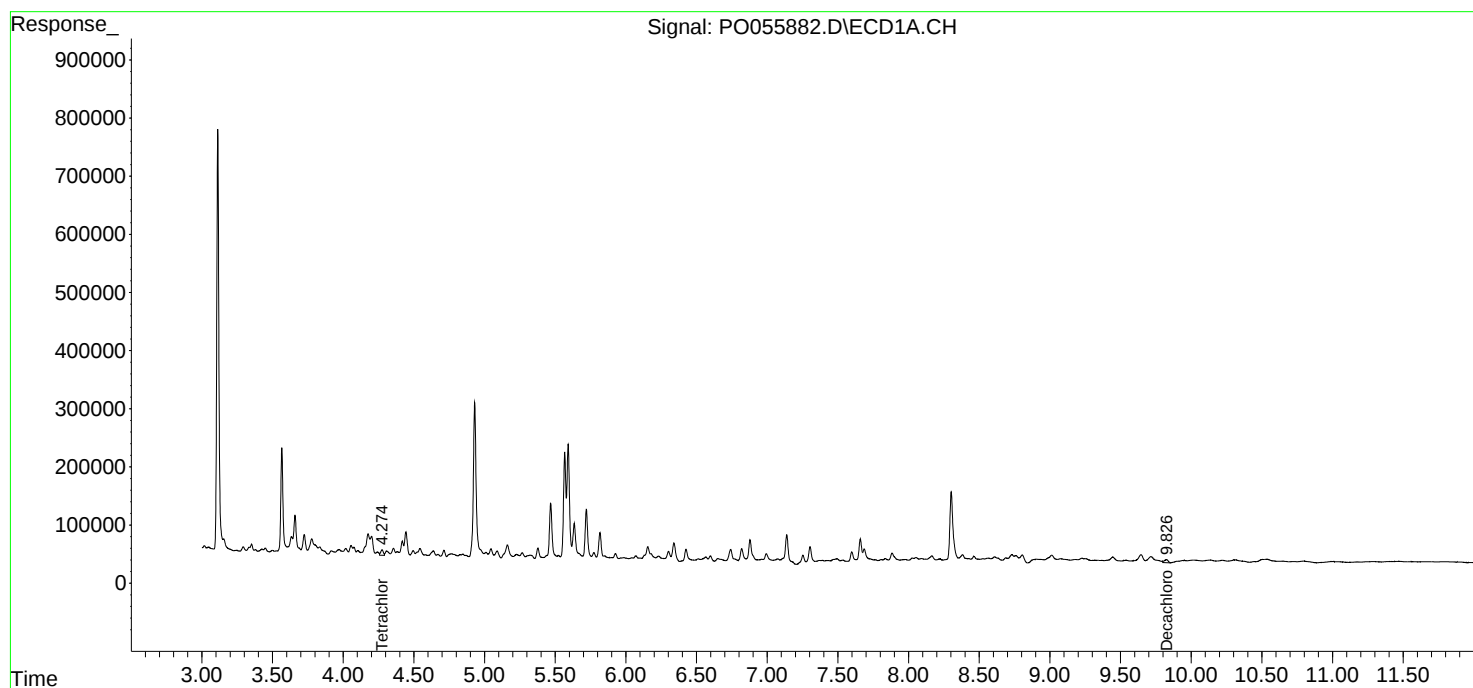

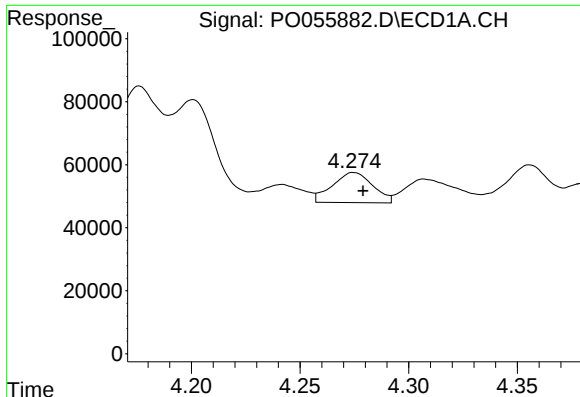


#1 Tetrachloro-m-xylene

R.T.: 4.274 min
Delta R.T.: -0.005 min
Response: 123602
Conc: 4.13 ng/ml

Instrument :
ECD_O
ClientSampleId :
NB-20523RE


Manual Integrations
APPROVED

Ankita
5/7/2019 1:14:43 PM

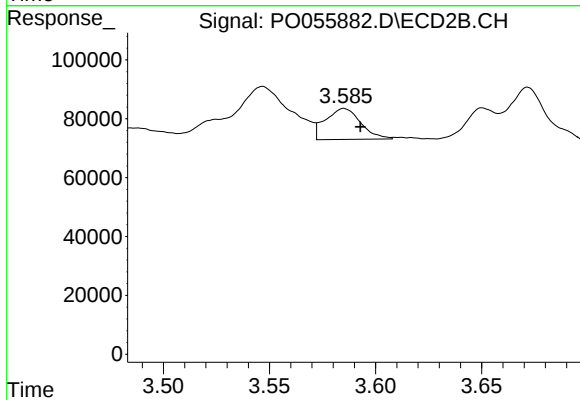


#1 Tetrachloro-m-xylene

R.T.: 3.585 min
Delta R.T.: -0.008 min
Response: 120788
Conc: 4.28 ng/ml m

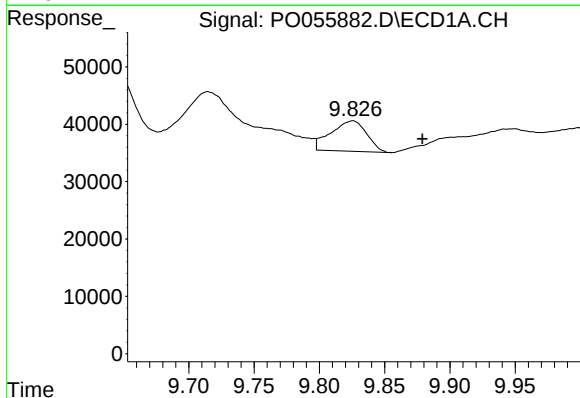

#2 Decachlorobiphenyl

R.T.: 9.826 min
Delta R.T.: -0.053 min
Response: 101348
Conc: 2.71 ng/ml

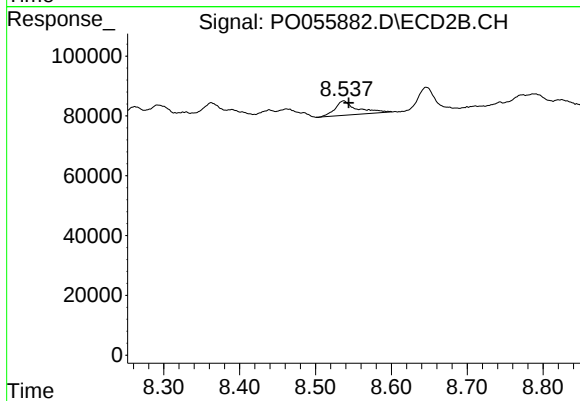

#2 Decachlorobiphenyl

R.T.: 8.537 min
Delta R.T.: -0.006 min
Response: 96738
Conc: 3.58 ng/ml