

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0050619\
 Data File : P0055914.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 May 2019 2:46
 Operator : SM/SJ
 Sample : K2672-12
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-06-COMP

Manual Integrations
 APPROVED

Ankita
 5/7/2019 1:15:16 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 07 03:53:56 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 03 15:20:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.274	3.589	1004041	858781	33.551	30.406m
2) SA Decachlor...	9.869	8.537	986754	649301	26.372	24.010

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0050619\
Data File : P0055914.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 May 2019 2:46
Operator : SM/SJ
Sample : K2672-12
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SB-06-COMP


Manual Integrations
APPROVED

Ankita
5/7/2019 1:15:16 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 07 03:53:56 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0050319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 03 15:20:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

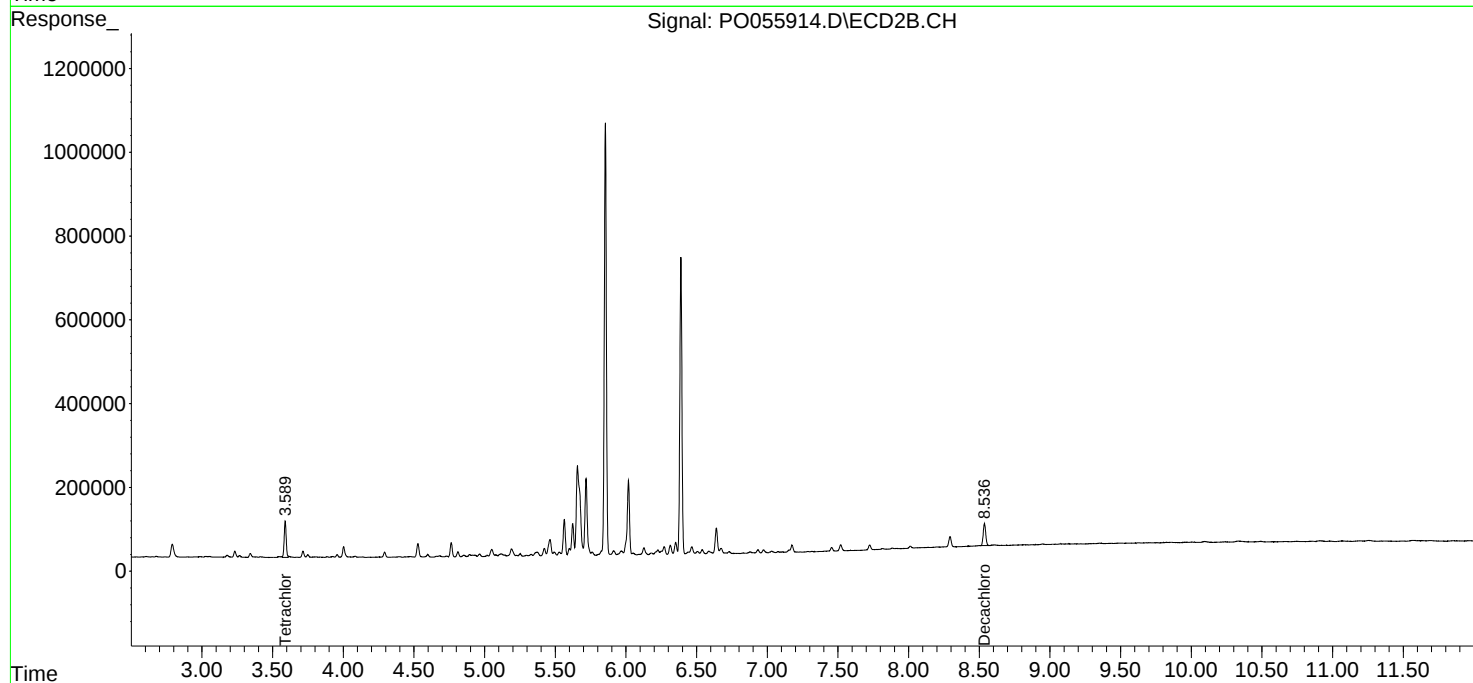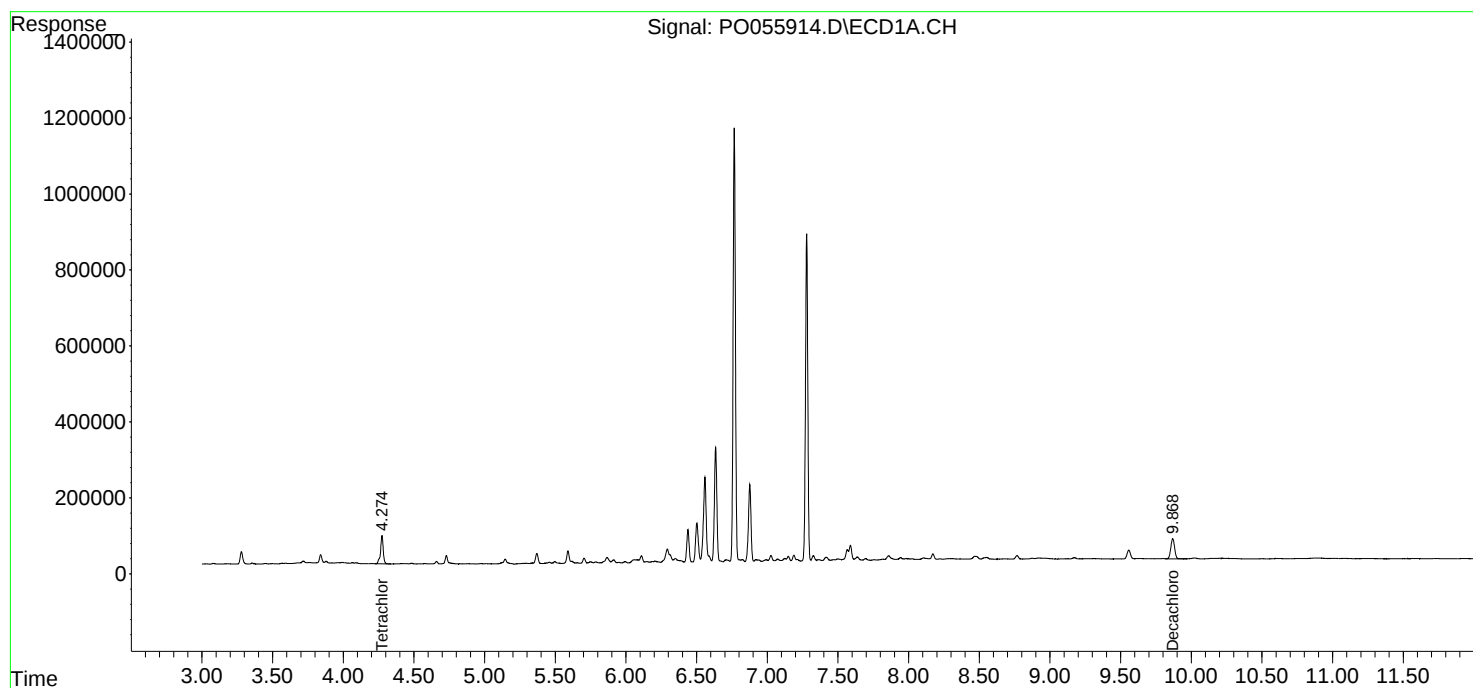

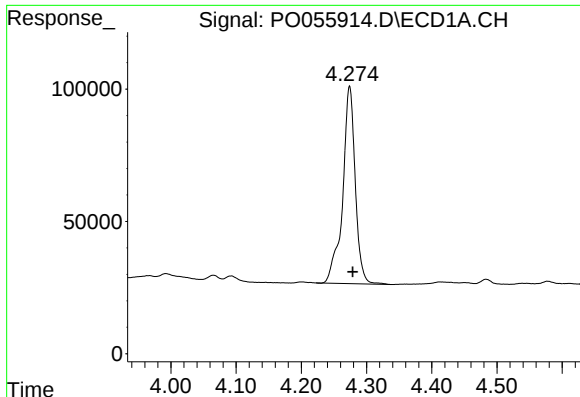


#1 Tetrachloro-m-xylene

R.T.: 4.274 min
Delta R.T.: -0.005 min
Response: 1004041
Conc: 33.55 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-06-COMP


Manual Integrations
APPROVED

Ankita
5/7/2019 1:15:16 PM

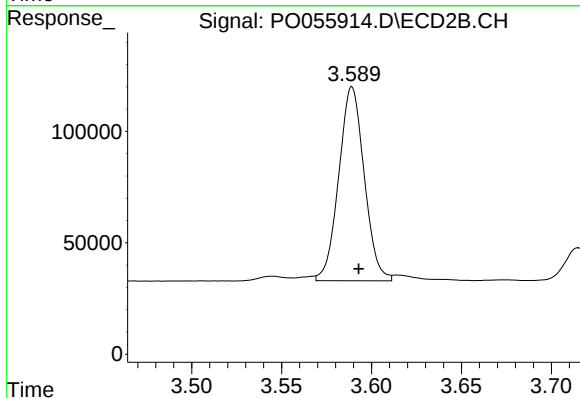


#1 Tetrachloro-m-xylene

R.T.: 3.589 min
Delta R.T.: -0.004 min
Response: 858781
Conc: 30.41 ng/ml m

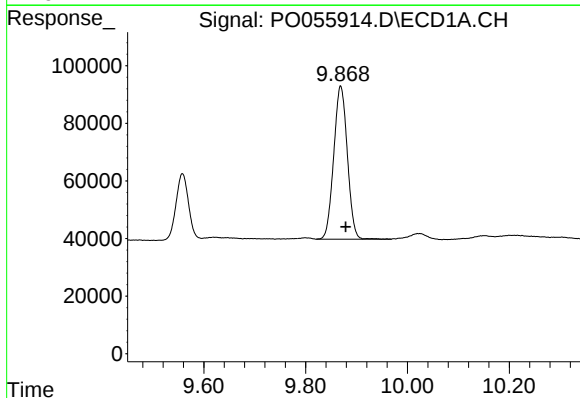

#2 Decachlorobiphenyl

R.T.: 9.869 min
Delta R.T.: -0.010 min
Response: 986754
Conc: 26.37 ng/ml

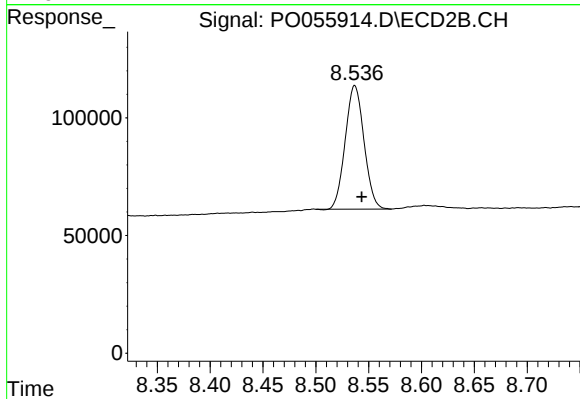

#2 Decachlorobiphenyl

R.T.: 8.537 min
Delta R.T.: -0.007 min
Response: 649301
Conc: 24.01 ng/ml