

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0050724\
 Data File : P0103430.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 May 2024 17:32
 Operator : YP/AJ
 Sample : PB160753BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB160753BL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/08/2024
 Supervised By :Ankita Jodhani 05/08/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 08 01:21:04 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue May 07 04:55:35 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.452	3.592	162.0E6	54811224	21.056	21.757
2) SA Decachlor...	10.209	8.558	67287253	26098556	14.195m	20.062 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO050724\
Data File : PO103430.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 May 2024 17:32
Operator : YP/AJ
Sample : PB160753BL
Misc :
ALS Vial : 19 Sample Multiplier: 1


Instrument :
ECD_O
ClientSampleId :
PB160753BL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/08/2024
Supervised By :Ankita Jodhani 05/08/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 08 01:21:04 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO050624.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue May 07 04:55:35 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

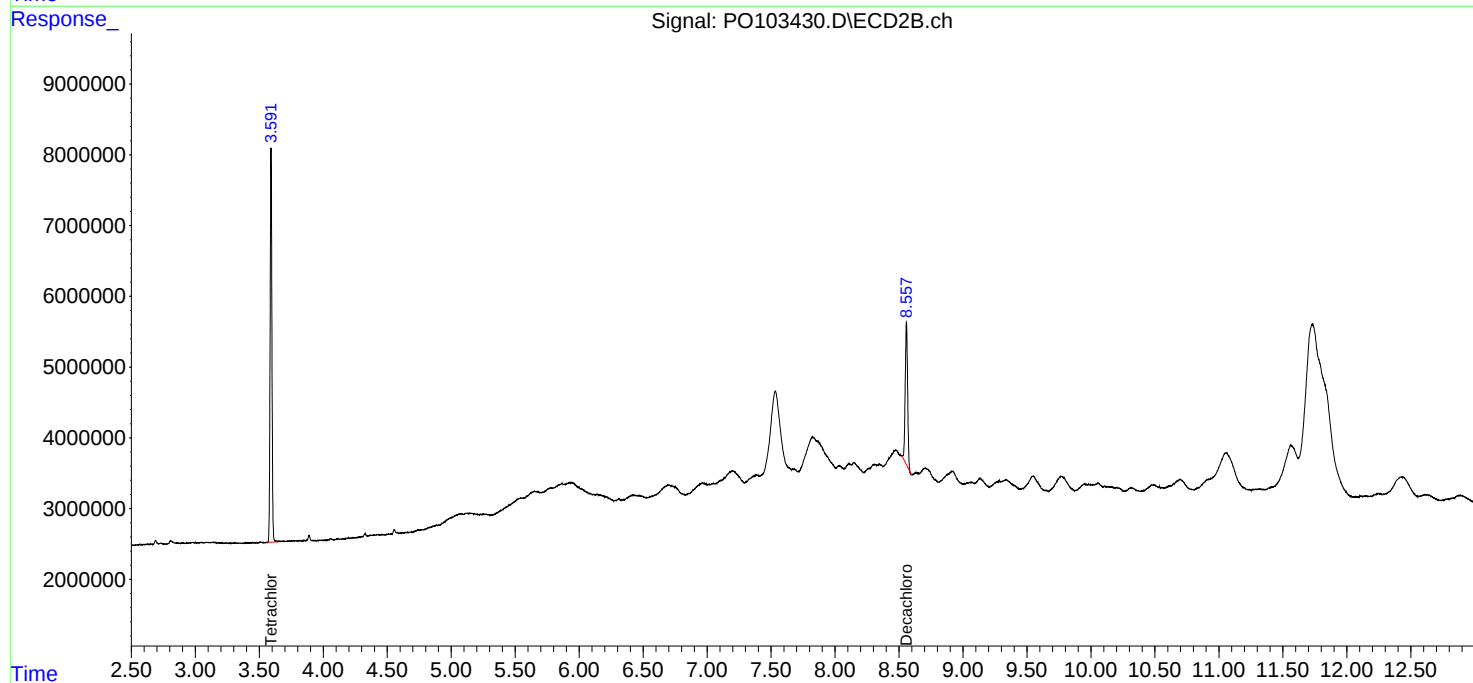

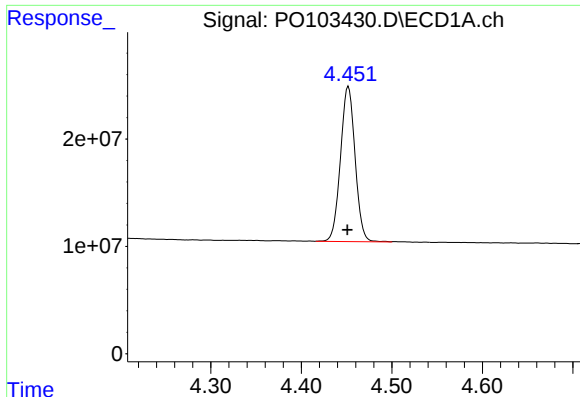


#1 Tetrachloro-m-xylene

R.T.: 4.452 min
Delta R.T.: 0.001 min
Response: 162040500
Conc: 21.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB160753BL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/08/2024
Supervised By :Ankita Jodhani 05/08/2024

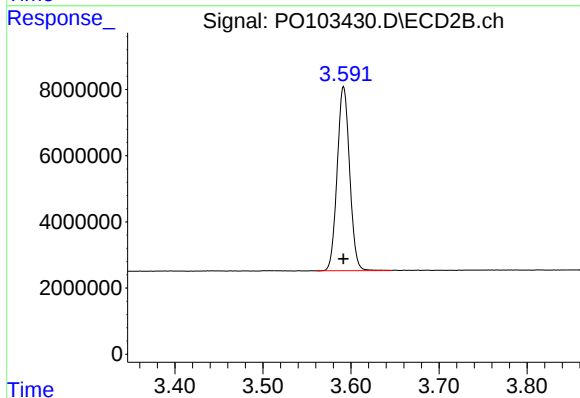


#1 Tetrachloro-m-xylene

R.T.: 3.592 min
Delta R.T.: 0.000 min
Response: 54811224
Conc: 21.76 ng/ml

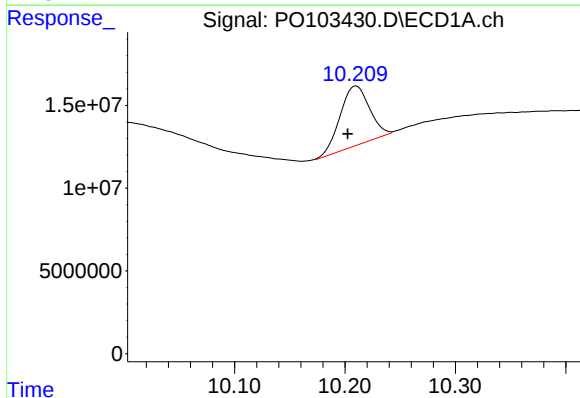

#2 Decachlorobiphenyl

R.T.: 10.209 min
Delta R.T.: 0.007 min
Response: 67287253
Conc: 14.19 ng/ml m

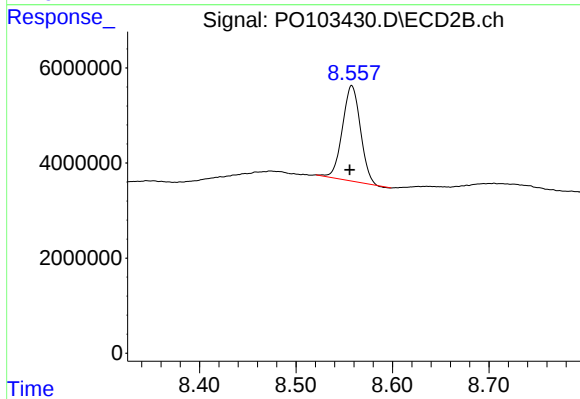

#2 Decachlorobiphenyl

R.T.: 8.558 min
Delta R.T.: 0.002 min
Response: 26098556
Conc: 20.06 ng/ml