

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0050820\
 Data File : P0068260.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 May 2020 19:43
 Operator : DD\AJ
 Sample : L2557-06
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-13A

Manual Integrations
 APPROVED

Sohil
 5/11/2020 9:09:42 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 09 04:14:23 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 08 13:29:29 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.909	3.934	665940	825886	23.744	24.068m
2) SA Decachlor...	10.872	9.212	808256	772054	20.312	20.054

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0050820\
Data File : P0068260.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 May 2020 19:43
Operator : DD\AJ
Sample : L2557-06
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TP-13A


Manual Integrations
APPROVED

Sohil
5/11/2020 9:09:42 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 09 04:14:23 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050820.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 08 13:29:29 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

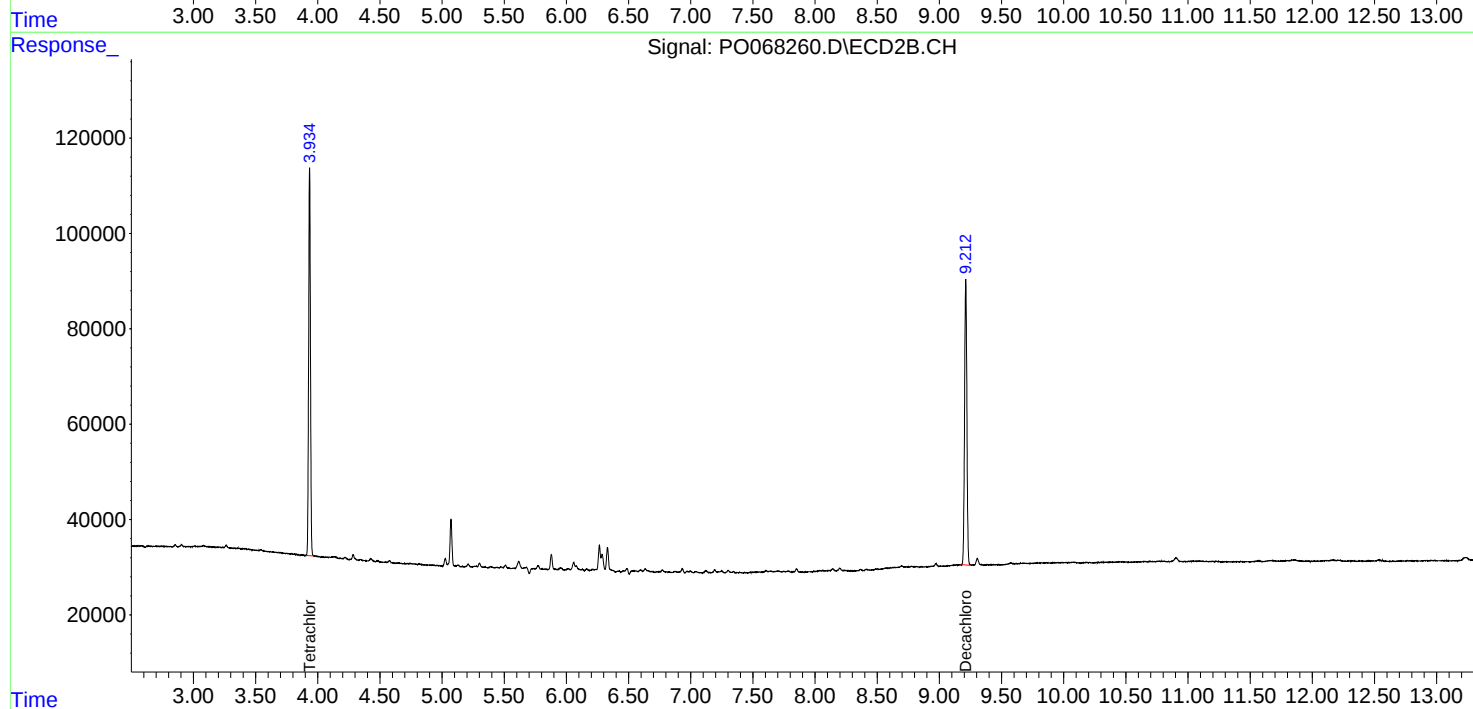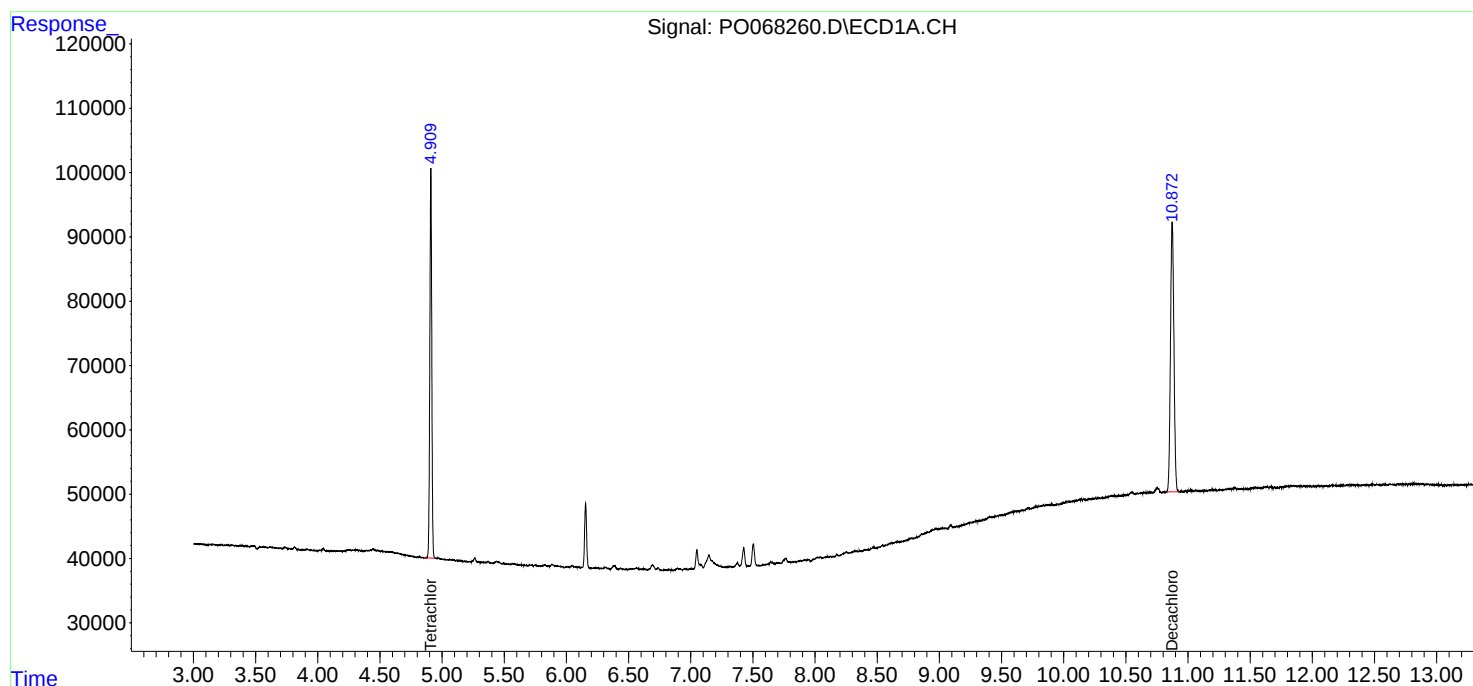

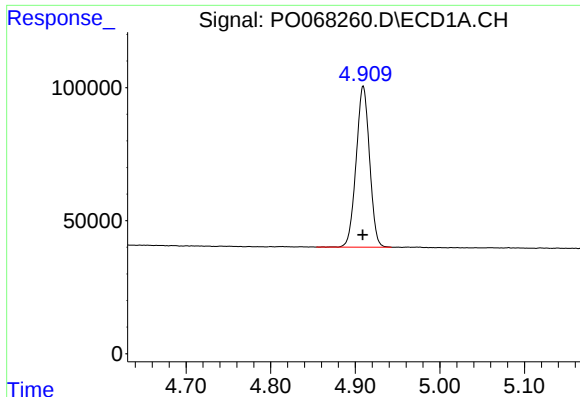


#1 Tetrachloro-m-xylene

R.T.: 4.909 min
Delta R.T.: 0.000 min
Response: 665940
Conc: 23.74 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-13A


Manual Integrations
APPROVED

Sohil
5/11/2020 9:09:42 AM

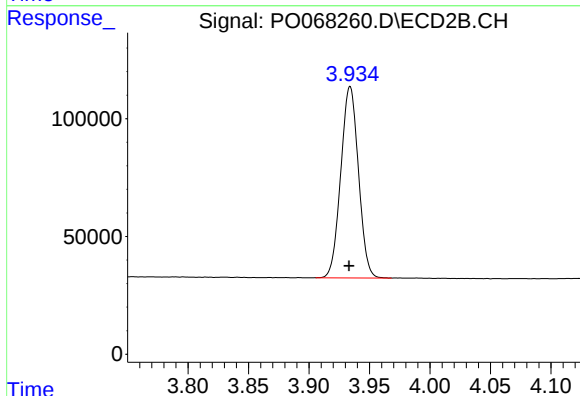


#1 Tetrachloro-m-xylene

R.T.: 3.934 min
Delta R.T.: 0.000 min
Response: 825886
Conc: 24.07 ng/ml m

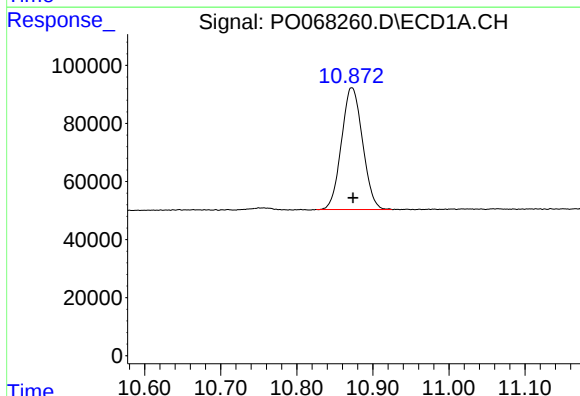

#2 Decachlorobiphenyl

R.T.: 10.872 min
Delta R.T.: -0.001 min
Response: 808256
Conc: 20.31 ng/ml

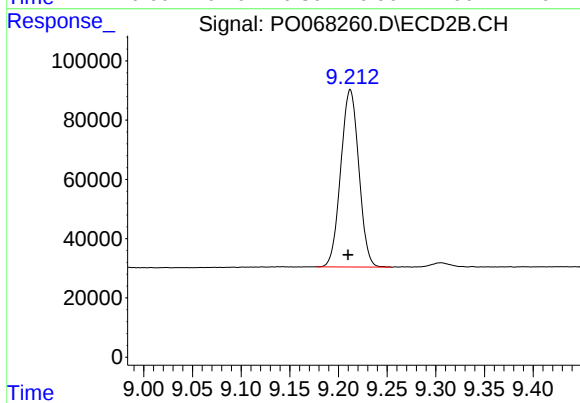

#2 Decachlorobiphenyl

R.T.: 9.212 min
Delta R.T.: 0.002 min
Response: 772054
Conc: 20.05 ng/ml