

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0050823\
 Data File : P0094859.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 May 2023 08:12
 Operator : YP/AJ
 Sample : 02660-02
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 WATER-SAMPLE-API-3-6

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 09 09:00:20 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042623.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon May 01 11:12:50 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.415	3.616	61872197	24261180	17.962	18.132
2) SA Decachlor...	10.256	8.627	35718354	17715702	14.718	15.739

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO050823\
Data File : PO094859.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 May 2023 08:12
Operator : YP/AJ
Sample : 02660-02
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
WATER-SAMPLE-API-3-6

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 09 09:00:20 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO042623.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon May 01 11:12:50 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

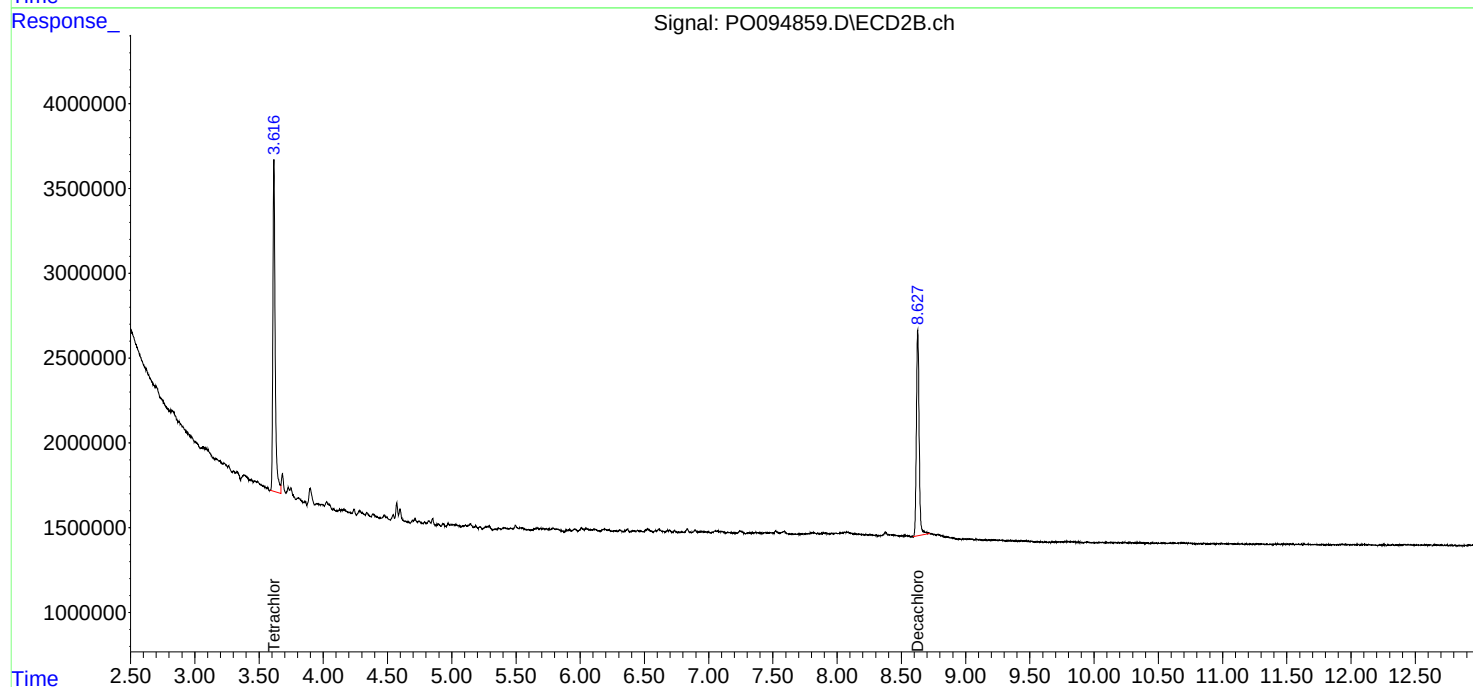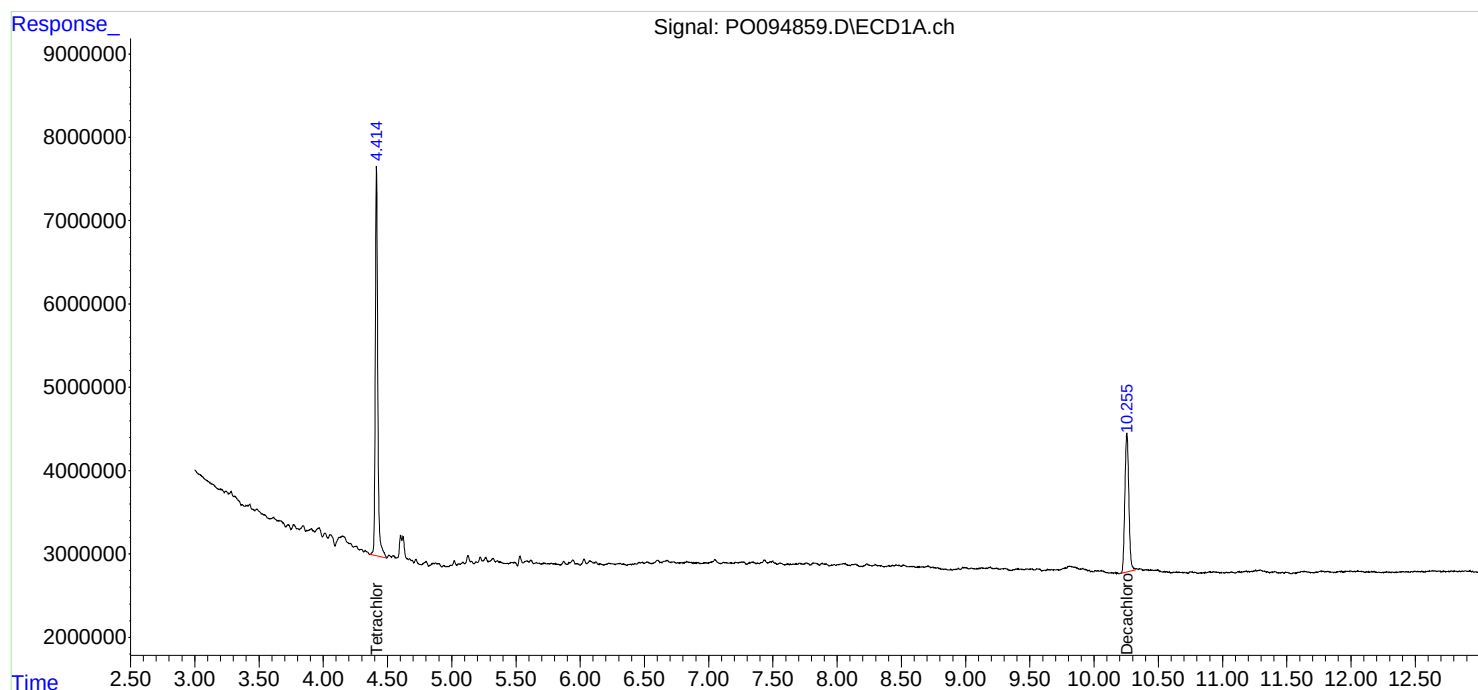


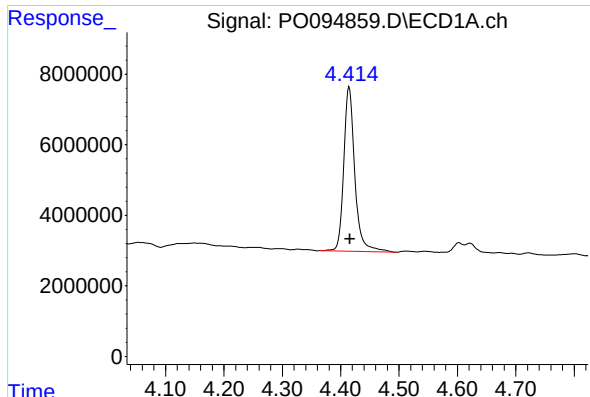

#1 Tetrachloro-m-xylene


R.T.: 4.415 min
Delta R.T.: -0.001 min
Response: 61872197
Conc: 17.96 ng/ml

Instrument :
ECD_O
ClientSampleId :
WATER-SAMPLE-API-3-6

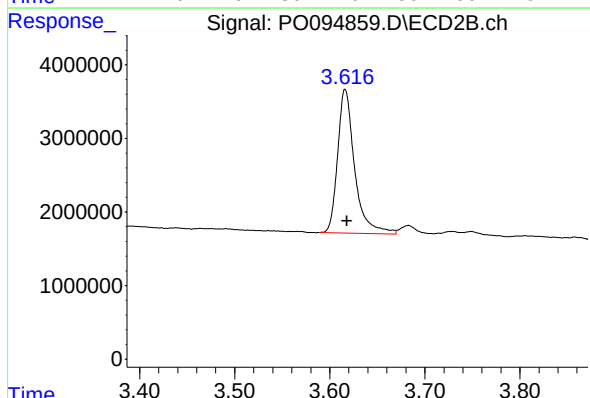


#1 Tetrachloro-m-xylene

R.T.: 3.616 min
Delta R.T.: -0.002 min
Response: 24261180
Conc: 18.13 ng/ml

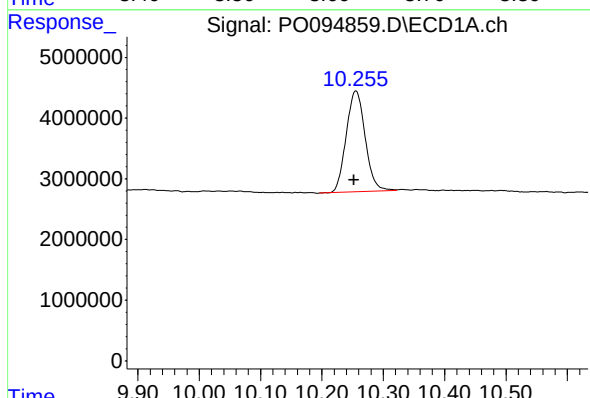

#2 Decachlorobiphenyl

R.T.: 10.256 min
Delta R.T.: 0.003 min
Response: 35718354
Conc: 14.72 ng/ml

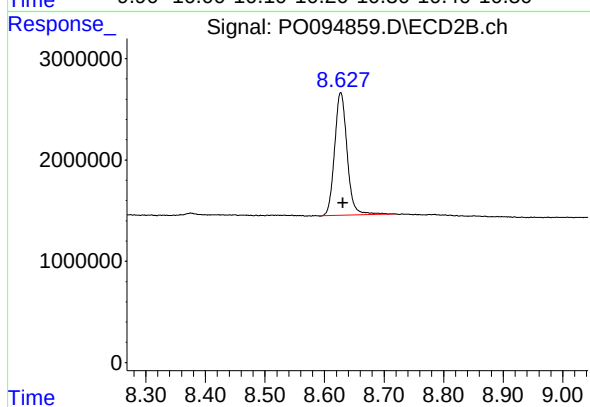

#2 Decachlorobiphenyl

R.T.: 8.627 min
Delta R.T.: -0.004 min
Response: 17715702
Conc: 15.74 ng/ml