

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0050923\
 Data File : P0094868.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 May 2023 11:15
 Operator : YP/AJ
 Sample : 02642-02RE
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TT-052-IDWGW-20230504RE

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/10/2023
 Supervised By :Ankita Jodhani 05/10/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 09 11:56:00 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042623.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon May 01 11:12:50 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.414	3.616	56898747	22801004	16.518	17.040
2) SA Decachlor...	10.254	8.627	16987264	8815752	7.000m	7.832

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO050923\
Data File : PO094868.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 May 2023 11:15
Operator : YP/AJ
Sample : 02642-02RE
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TT-052-IDWGW-20230504RE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/10/2023
Supervised By :Ankita Jodhani 05/10/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 09 11:56:00 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO042623.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon May 01 11:12:50 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

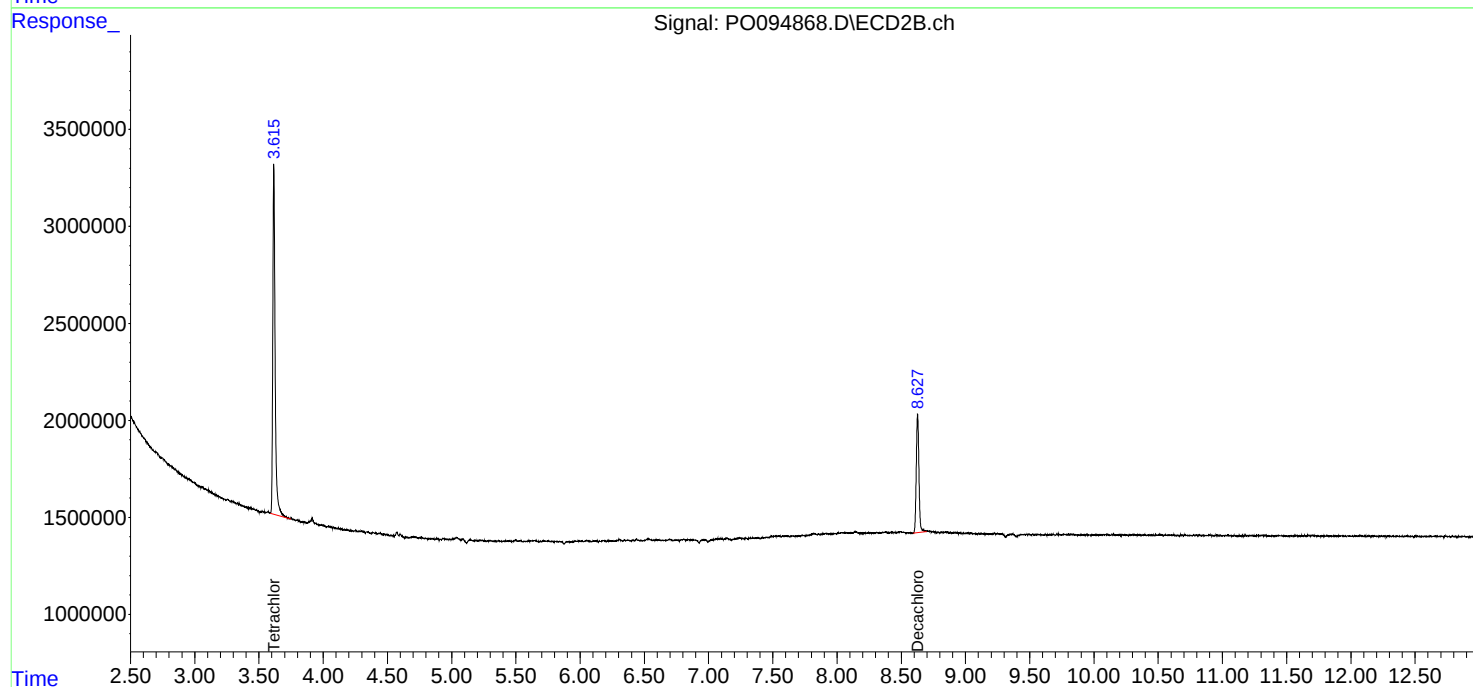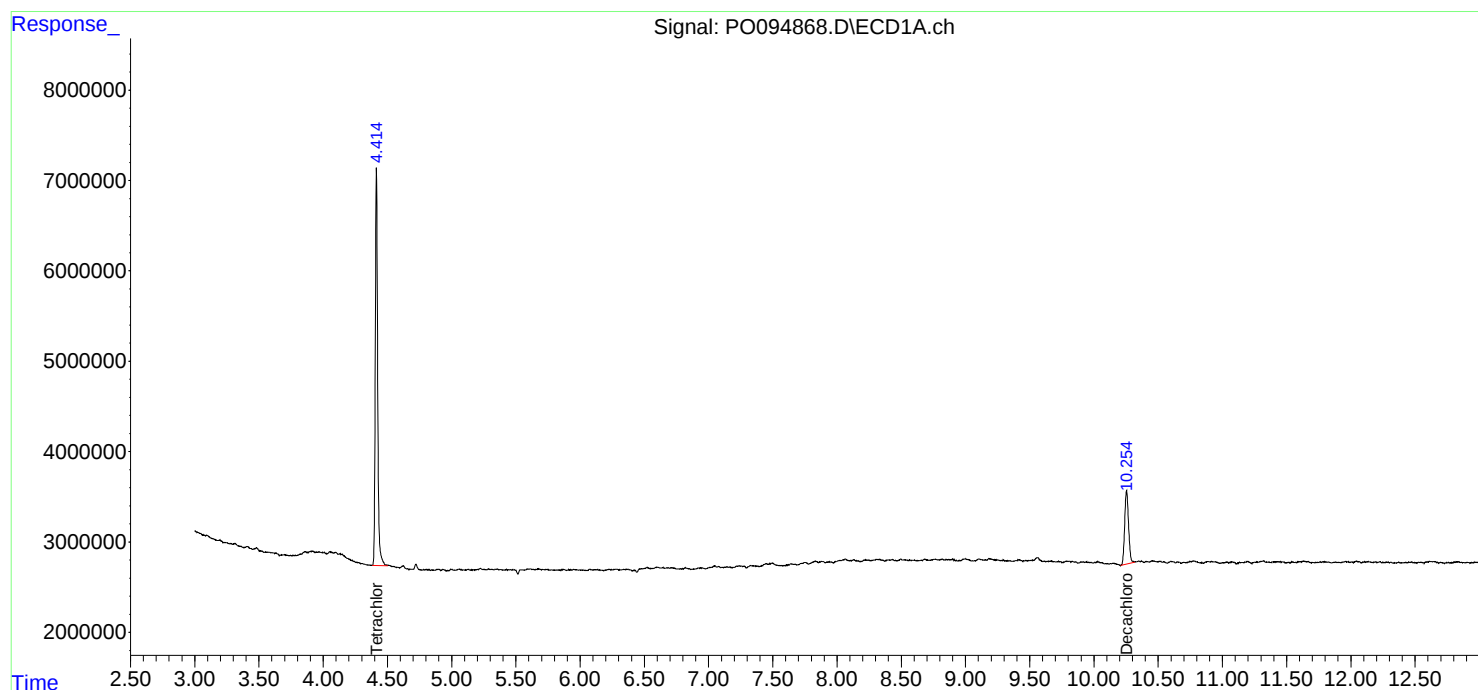

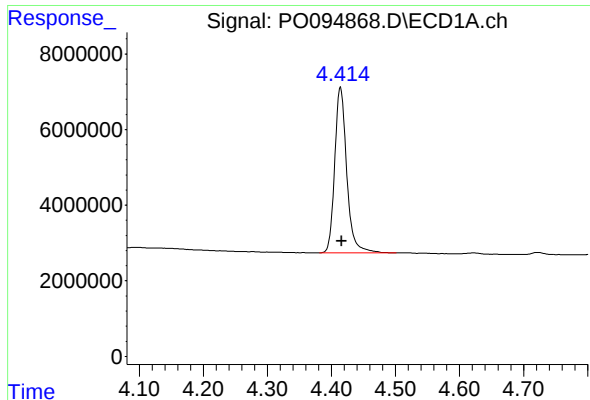


#1 Tetrachloro-m-xylene

R.T.: 4.414 min
Delta R.T.: -0.002 min
Response: 56898747
Conc: 16.52 ng/ml

Instrument :
ECD_O
ClientSampleId :
TT-052-IDWGW-20230504RE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/10/2023
Supervised By :Ankita Jodhani 05/10/2023

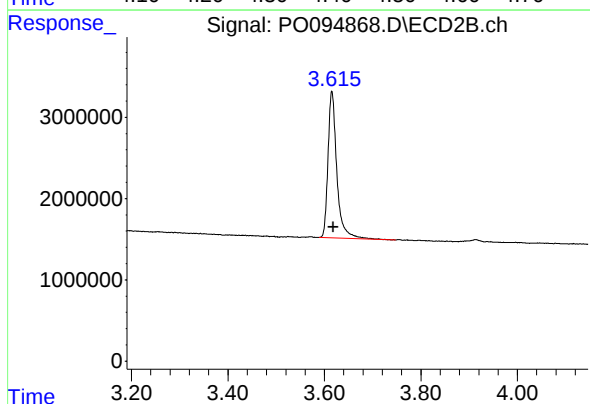


#1 Tetrachloro-m-xylene

R.T.: 3.616 min
Delta R.T.: -0.002 min
Response: 22801004
Conc: 17.04 ng/ml

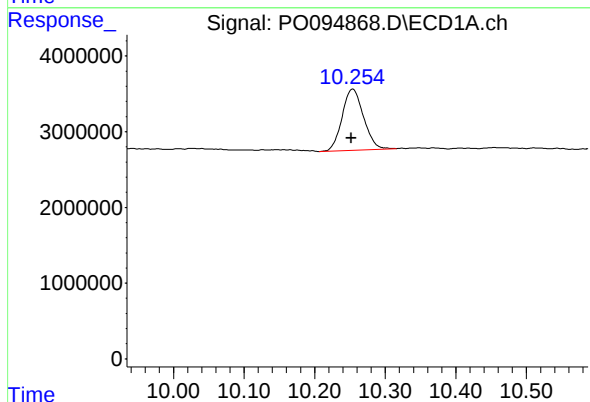

#2 Decachlorobiphenyl

R.T.: 10.254 min
Delta R.T.: 0.001 min
Response: 16987264
Conc: 7.00 ng/ml m

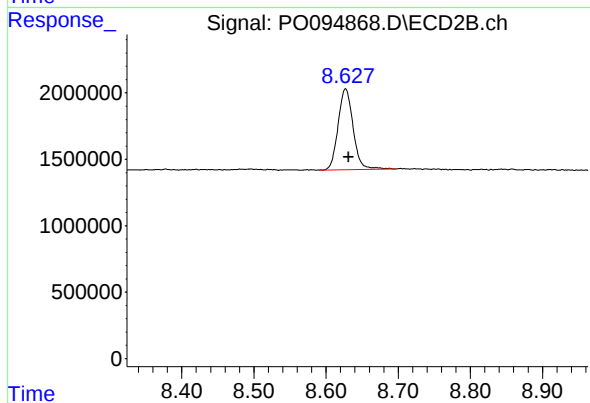

#2 Decachlorobiphenyl

R.T.: 8.627 min
Delta R.T.: -0.004 min
Response: 8815752
Conc: 7.83 ng/ml