

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051023\
 Data File : P0094925.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 May 2023 16:57
 Operator : YP/AJ
 Sample : 02691-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AU-504-COMP-06

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 10 21:34:47 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042623.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon May 01 11:12:50 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.414	3.616	75817558	31116336	22.010	23.255
2) SA Decachlor...	10.253	8.626	48899681	22988460	20.149	20.424

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO051023\
Data File : PO094925.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 May 2023 16:57
Operator : YP/AJ
Sample : 02691-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AU-504-COMP-06

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 10 21:34:47 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO042623.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon May 01 11:12:50 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

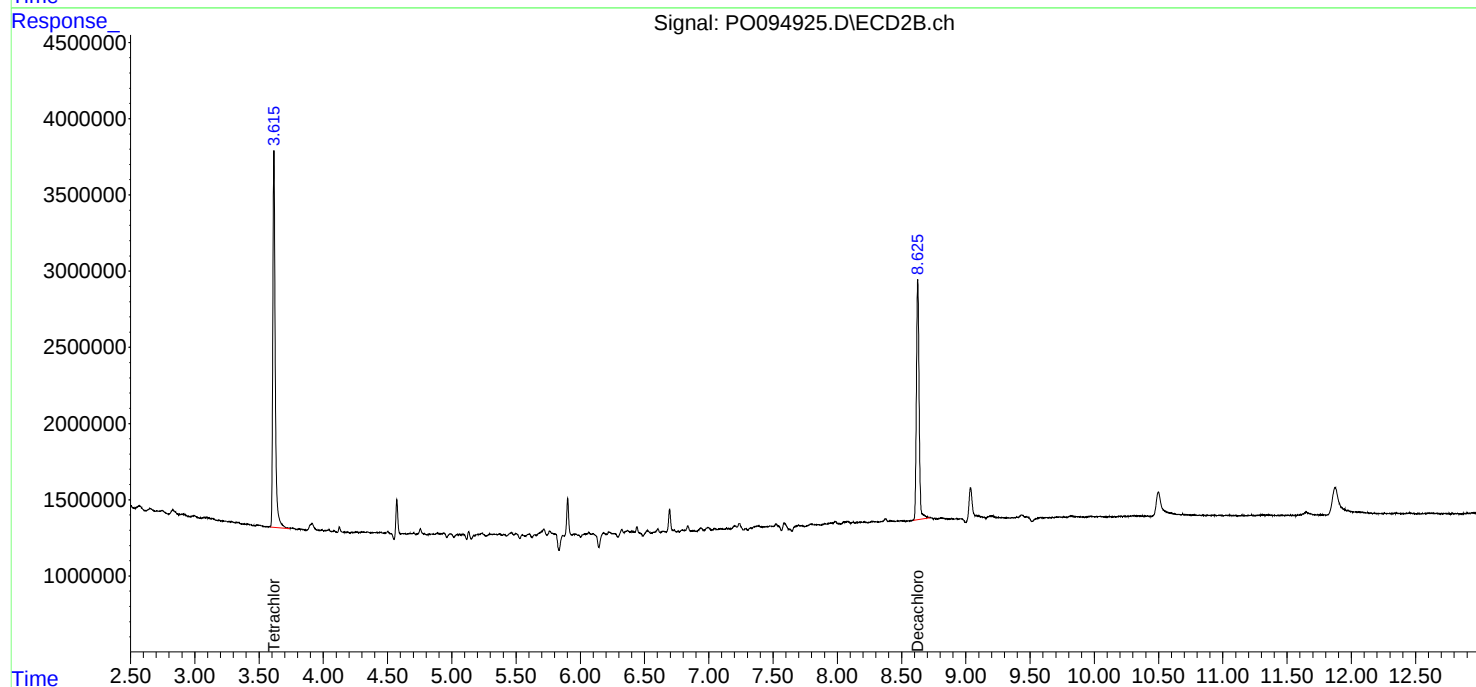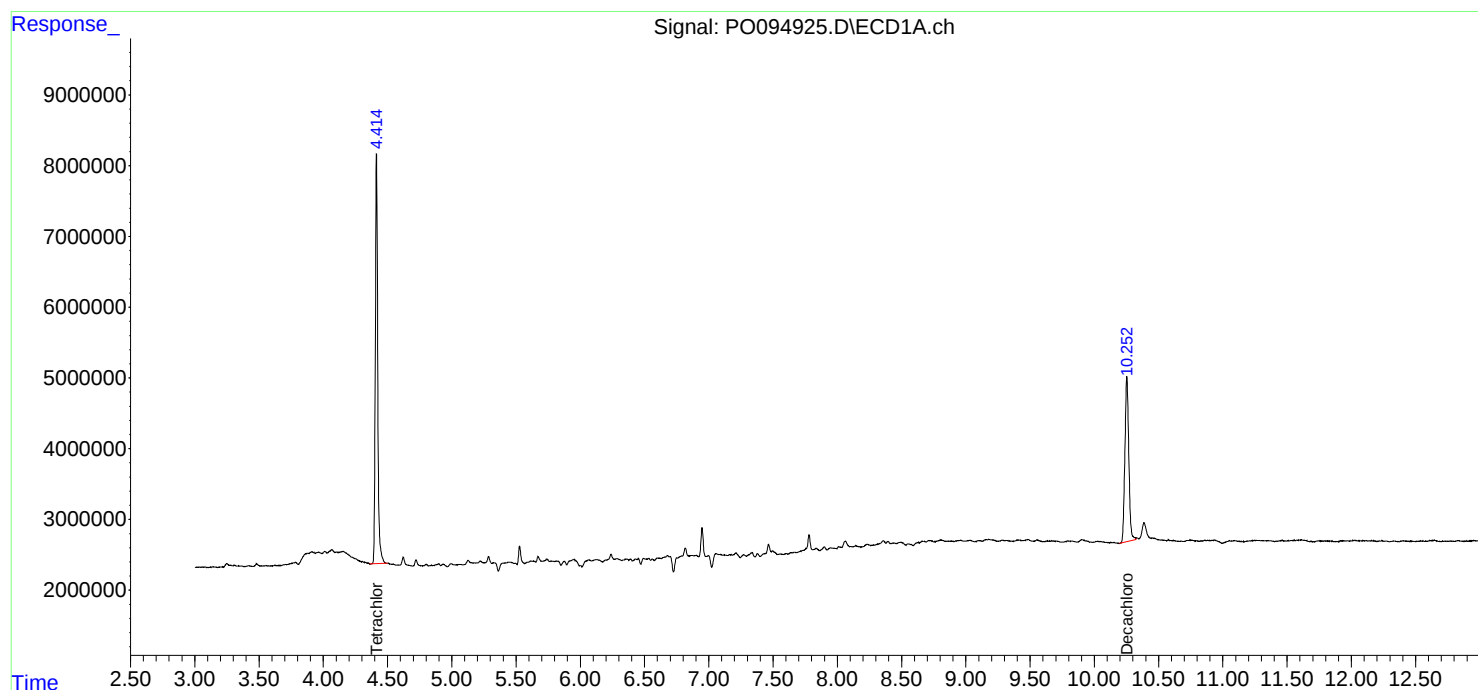


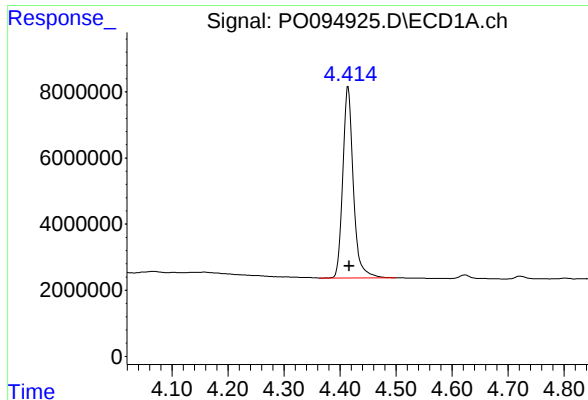

#1 Tetrachloro-m-xylene


R.T.: 4.414 min
Delta R.T.: -0.002 min
Response: 75817558
Conc: 22.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
AU-504-COMP-06

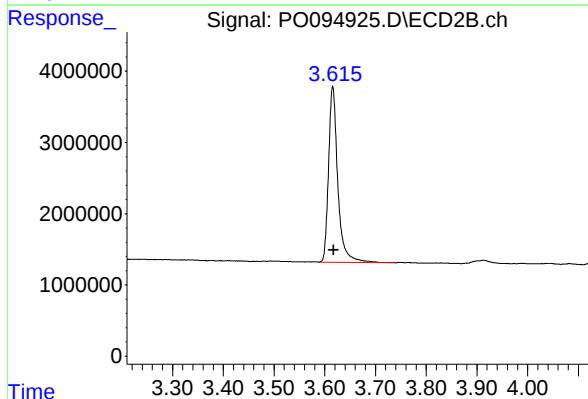


#1 Tetrachloro-m-xylene

R.T.: 3.616 min
Delta R.T.: -0.002 min
Response: 31116336
Conc: 23.25 ng/ml

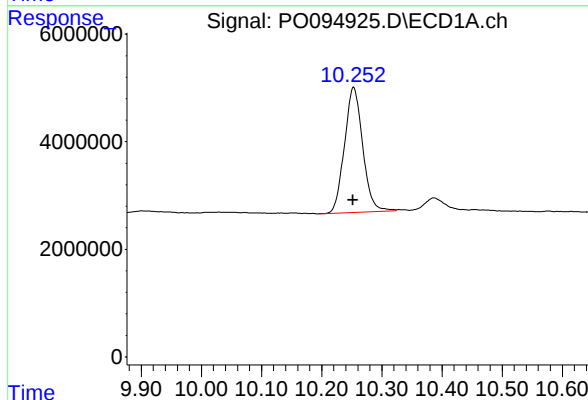

#2 Decachlorobiphenyl

R.T.: 10.253 min
Delta R.T.: 0.000 min
Response: 48899681
Conc: 20.15 ng/ml

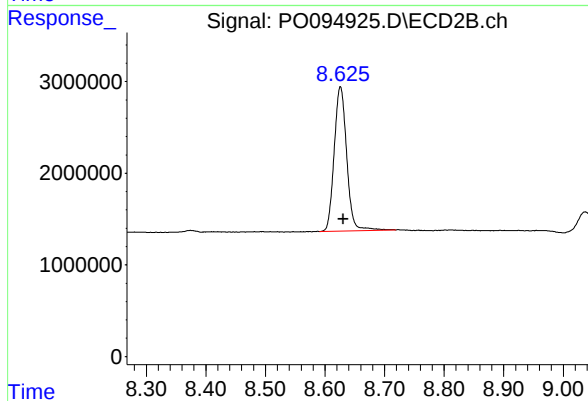

#2 Decachlorobiphenyl

R.T.: 8.626 min
Delta R.T.: -0.005 min
Response: 22988460
Conc: 20.42 ng/ml