

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0051120\
 Data File : P0068278.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 May 2020 13:00
 Operator : DD\AJ
 Sample : L2182-07
 Misc : AR1232 25PPB LOD
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT2-2020

Manual Integrations
 APPROVED

Sohil
 5/12/2020 2:53:36 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 12 00:24:11 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0050820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 08 13:29:29 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.906	3.932	530887	669194	18.929	19.502
2)	SA Decachlor...	10.867	9.208	757620	775488	19.039	20.143
Target Compounds							
11)	L3 AR-1232-1	5.344	4.376	19088	20568	31.079	26.666
12)	L3 AR-1232-2	5.925	5.206	17758	28326	57.624m	35.370 #
13)	L3 AR-1232-3	6.251	5.395	15965	14764	25.041	34.766 #
14)	L3 AR-1232-4	6.425	5.491	7046	13588	22.385	36.191 #
15)	L3 AR-1232-5	6.524	5.675	6085	8489	28.758	20.375m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051120\
Data File : P0068278.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 May 2020 13:00
Operator : DD\AJ
Sample : L2182-07
Misc : AR1232 25PPB LOD
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2020


Manual Integrations
APPROVED

Sohil
5/12/2020 2:53:36 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 12 00:24:11 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050820.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 08 13:29:29 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

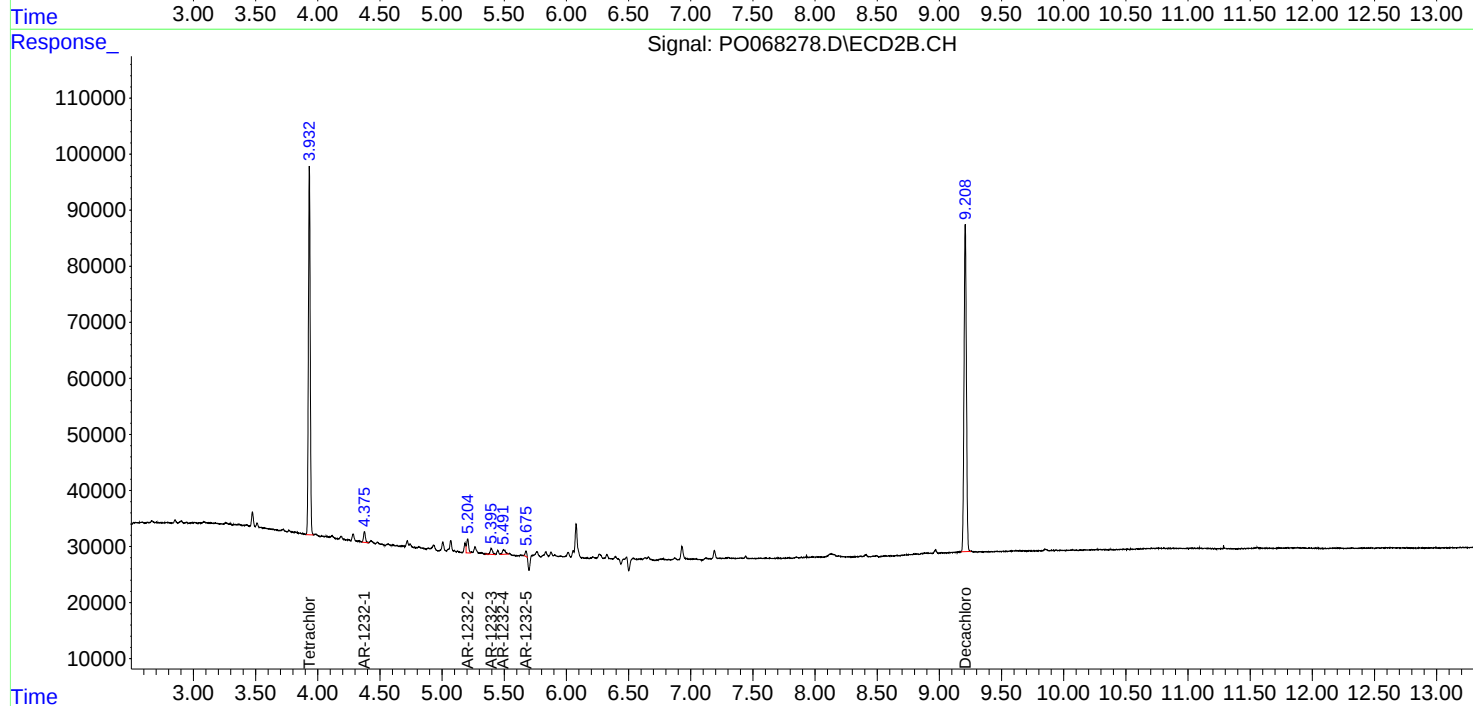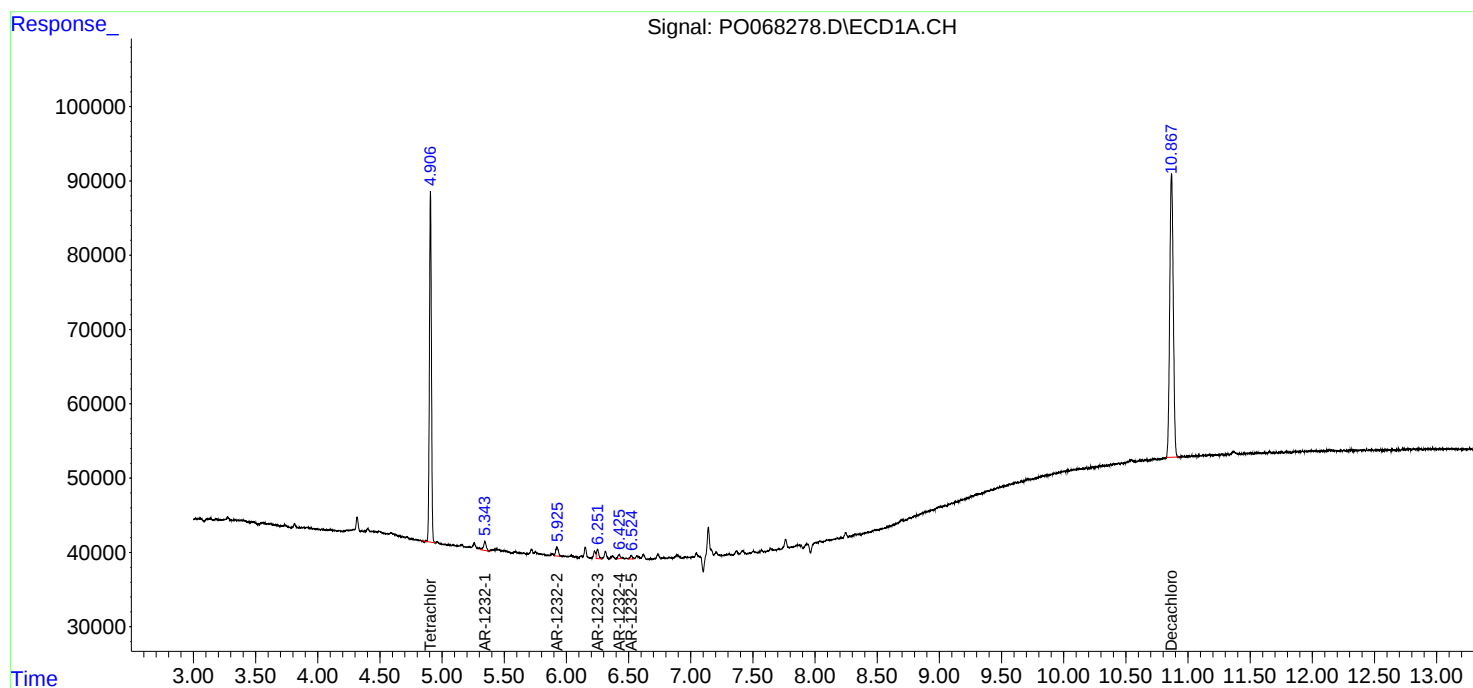

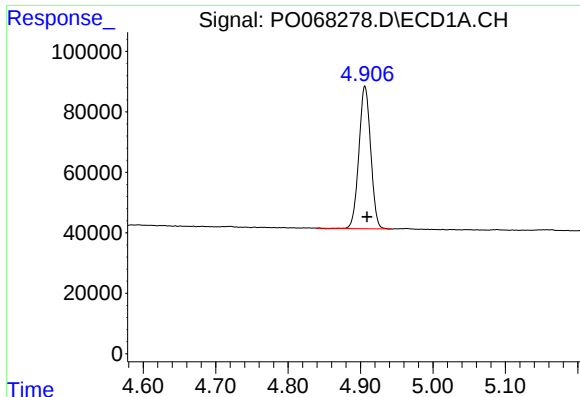


#1 Tetrachloro-m-xylene

R.T.: 4.906 min
Delta R.T.: -0.003 min
Response: 530887
Conc: 18.93 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2020


Manual Integrations
APPROVED

Sohil
5/12/2020 2:53:36 PM

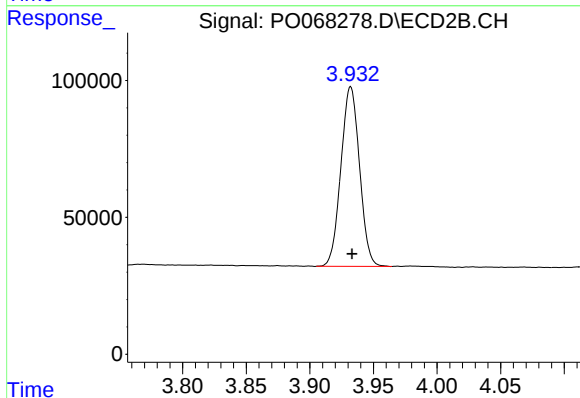


#1 Tetrachloro-m-xylene

R.T.: 3.932 min
Delta R.T.: -0.001 min
Response: 669194
Conc: 19.50 ng/ml

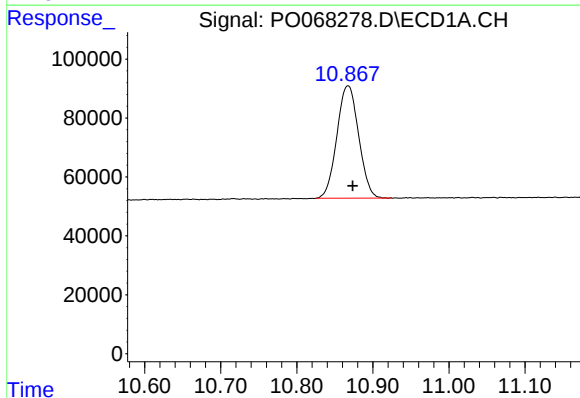


#2 Decachlorobiphenyl

R.T.: 10.867 min
Delta R.T.: -0.006 min
Response: 757620
Conc: 19.04 ng/ml

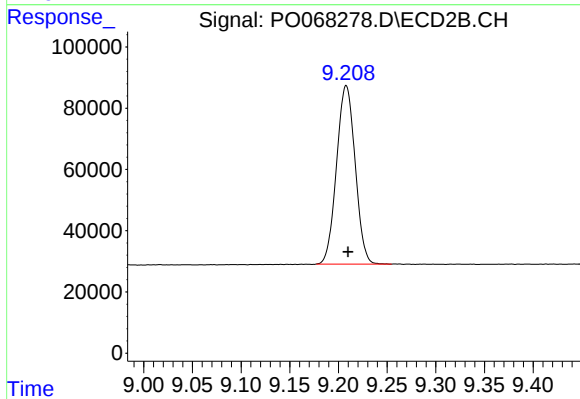

#2 Decachlorobiphenyl

R.T.: 9.208 min
Delta R.T.: -0.002 min
Response: 775488
Conc: 20.14 ng/ml

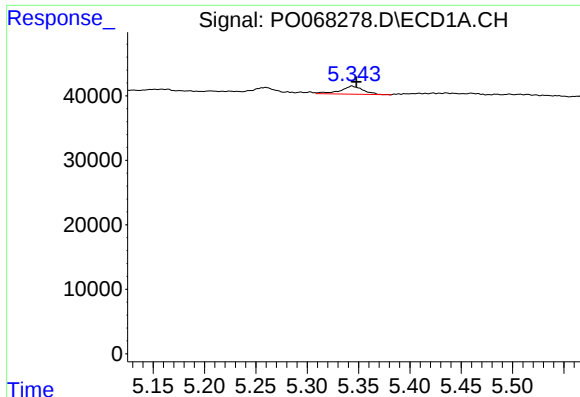


#11 AR-1232-1

R.T.: 5.344 min
Delta R.T.: -0.004 min
Response: 19088
Conc: 31.08 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2020


Manual Integrations
APPROVED

Sohil
5/12/2020 2:53:36 PM

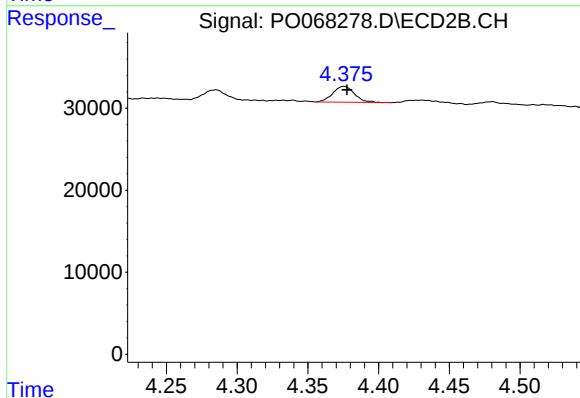


#11 AR-1232-1

R.T.: 4.376 min
Delta R.T.: -0.002 min
Response: 20568
Conc: 26.67 ng/ml

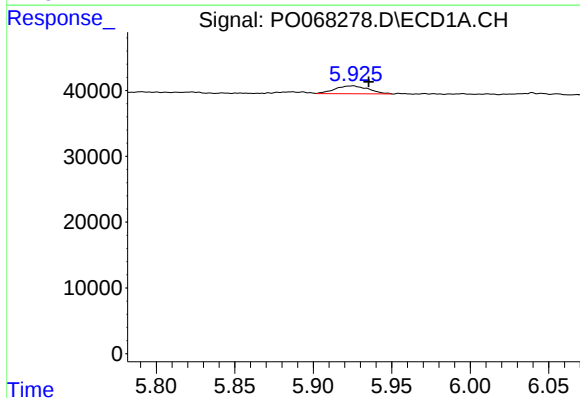


#12 AR-1232-2

R.T.: 5.925 min
Delta R.T.: -0.010 min
Response: 17758
Conc: 57.62 ng/ml m

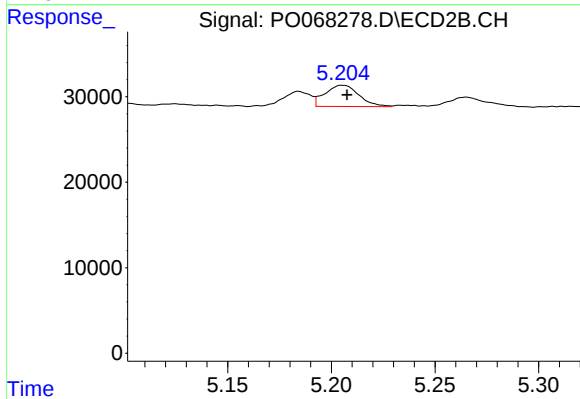

#12 AR-1232-2

R.T.: 5.206 min
Delta R.T.: -0.002 min
Response: 28326
Conc: 35.37 ng/ml

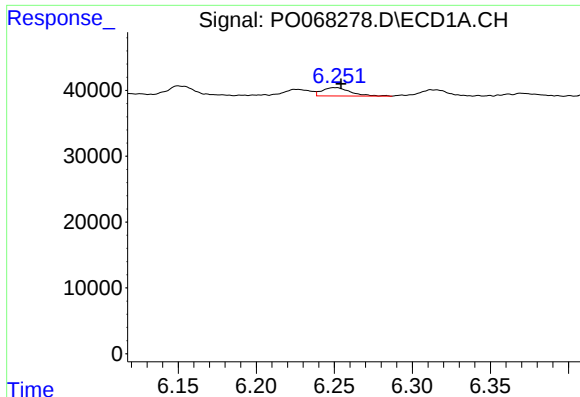


#13 AR-1232-3

R.T.: 6.251 min
Delta R.T.: -0.004 min
Response: 15965
Conc: 25.04 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2020


Manual Integrations
APPROVED

Sohil
5/12/2020 2:53:36 PM

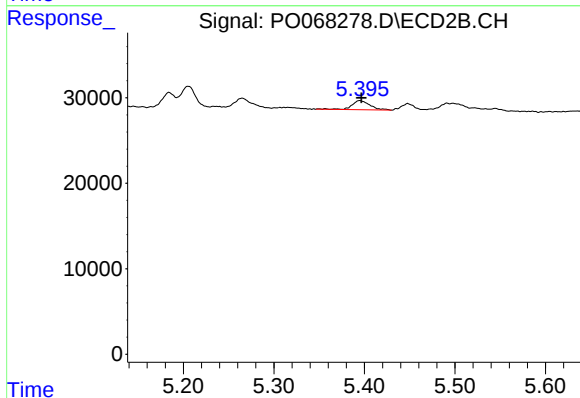


#13 AR-1232-3

R.T.: 5.395 min
Delta R.T.: -0.002 min
Response: 14764
Conc: 34.77 ng/ml

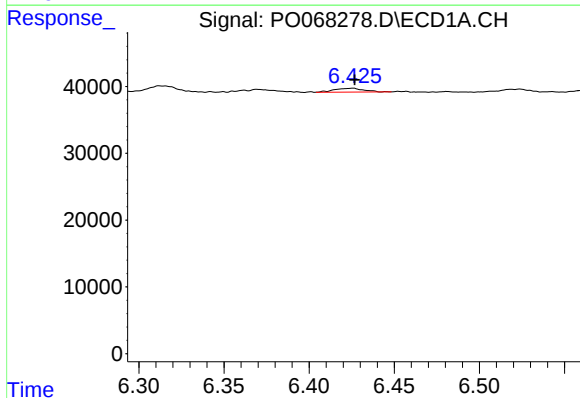


#14 AR-1232-4

R.T.: 6.425 min
Delta R.T.: -0.002 min
Response: 7046
Conc: 22.39 ng/ml

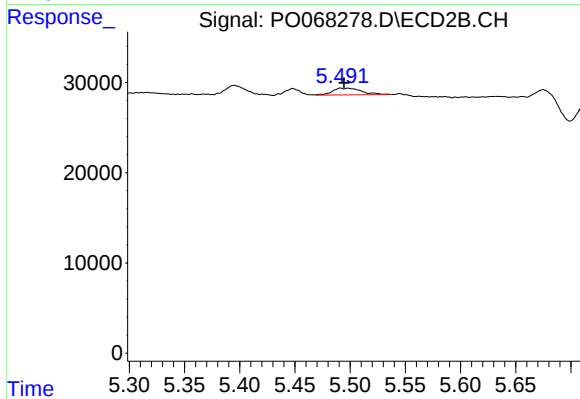

#14 AR-1232-4

R.T.: 5.491 min
Delta R.T.: -0.003 min
Response: 13588
Conc: 36.19 ng/ml

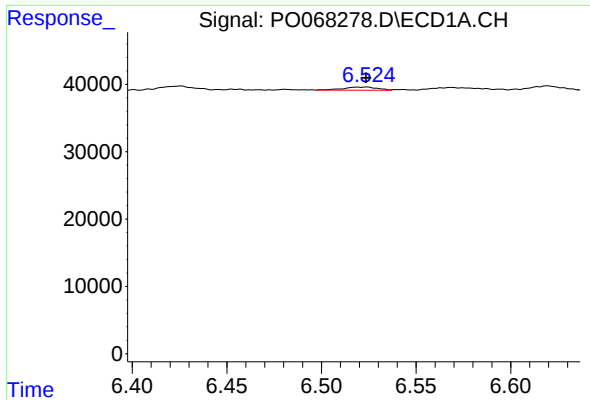


#15 AR-1232-5

R.T.: 6.524 min
Delta R.T.: 0.000 min
Response: 6085
Conc: 28.76 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2020

Manual Integrations
APPROVED

Sohil
5/12/2020 2:53:36 PM

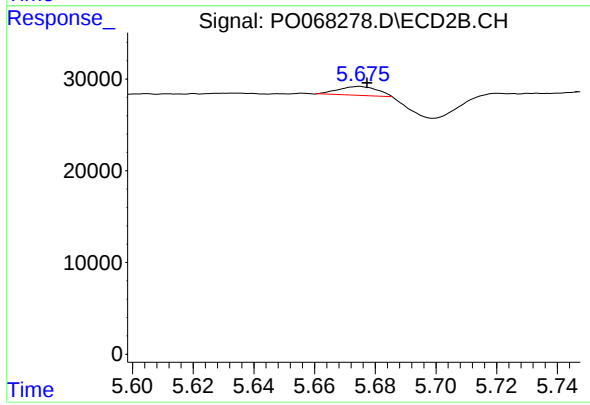

#15 AR-1232-5

R.T.: 5.675 min
Delta R.T.: -0.002 min
Response: 8489
Conc: 20.37 ng/ml m