

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051120\
 Data File : P0068281.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 May 2020 13:51
 Operator : DD\AJ
 Sample : L2182-07
 Misc : AR1254 25PPB LOD
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT2-2020

Manual Integrations
 APPROVED

Sohil
 5/12/2020 2:53:39 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 12 00:25:21 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 08 13:29:29 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.907	3.932	631742	784136	22.525	22.852
2)	SA Decachlor...	10.868	9.209	866815	889392	21.783	23.102
Target Compounds							
26)	L6 AR-1254-1	7.136	6.054	38510	52541	32.382m	25.928m
27)	L6 AR-1254-2	7.363	6.213	52363	50084	28.365	27.951m
28)	L6 AR-1254-3	7.744	6.631	59980	80124	30.981	27.846m
29)	L6 AR-1254-4	8.039	6.872	44938	60375	28.077	31.295
30)	L6 AR-1254-5	8.466	7.299	34732	68252	21.142	25.308

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO051120\
Data File : PO068281.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 May 2020 13:51
Operator : DD\AJ
Sample : L2182-07
Misc : AR1254 25PPB LOD
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
LOD-MDL-WATER-01-QT2-2020


Manual Integrations
APPROVED

Sohil
5/12/2020 2:53:39 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 12 00:25:21 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO050820.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 08 13:29:29 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

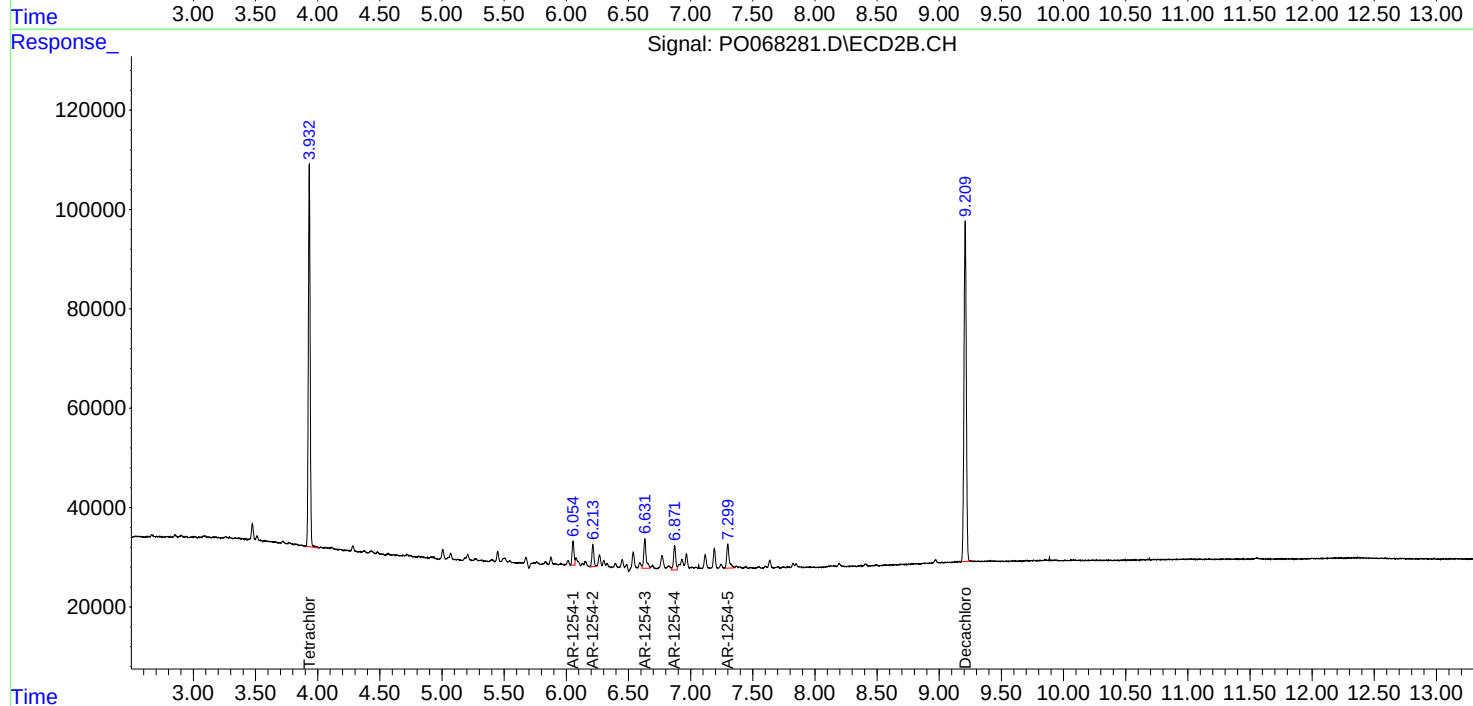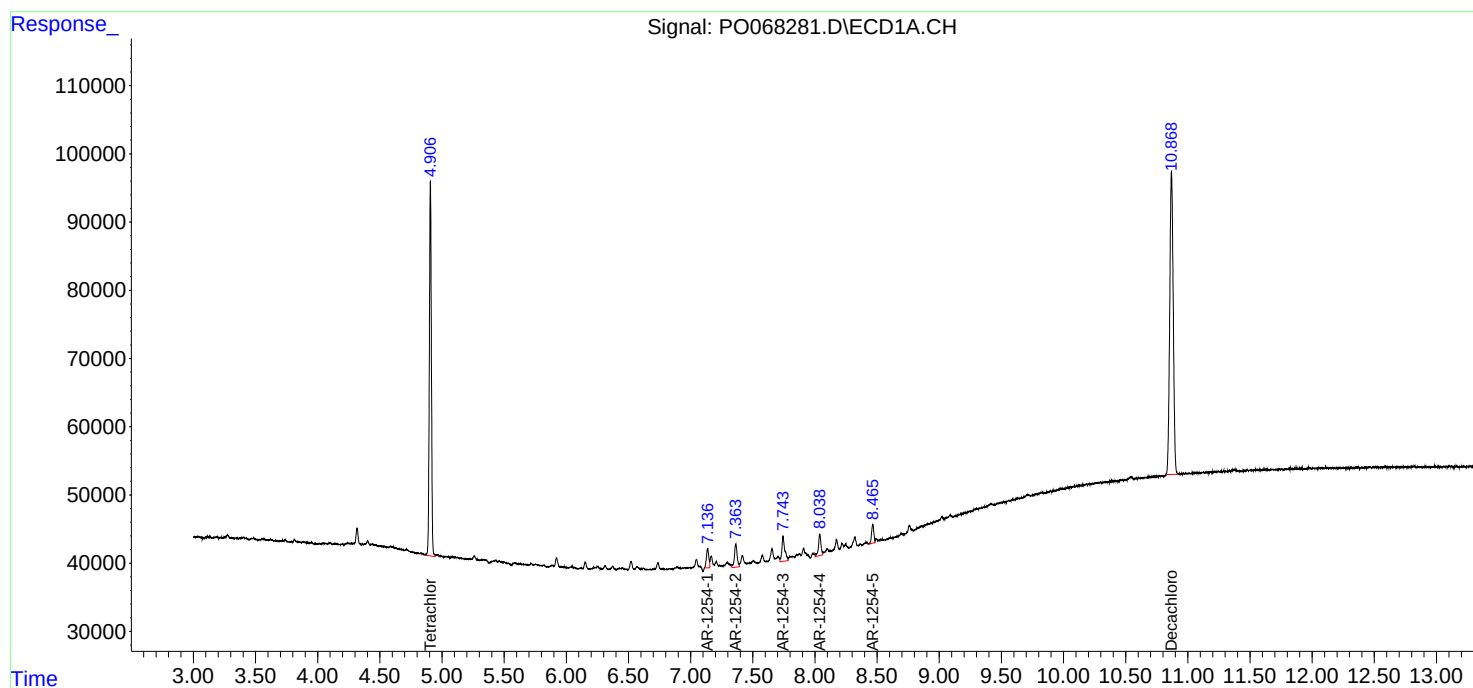

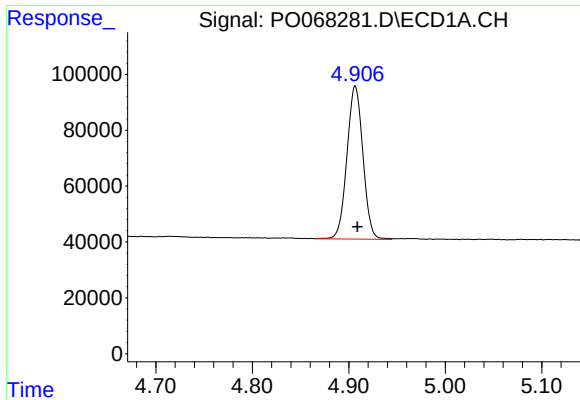


#1 Tetrachloro-m-xylene

R.T.: 4.907 min
Delta R.T.: -0.002 min
Response: 631742
Conc: 22.52 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2020


Manual Integrations
APPROVED

Sohil
5/12/2020 2:53:39 PM

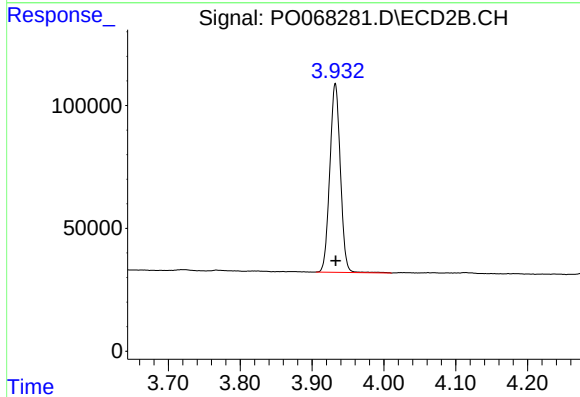


#1 Tetrachloro-m-xylene

R.T.: 3.932 min
Delta R.T.: 0.000 min
Response: 784136
Conc: 22.85 ng/ml

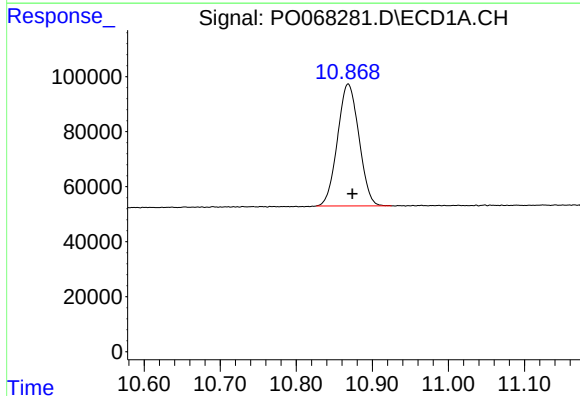


#2 Decachlorobiphenyl

R.T.: 10.868 min
Delta R.T.: -0.005 min
Response: 866815
Conc: 21.78 ng/ml

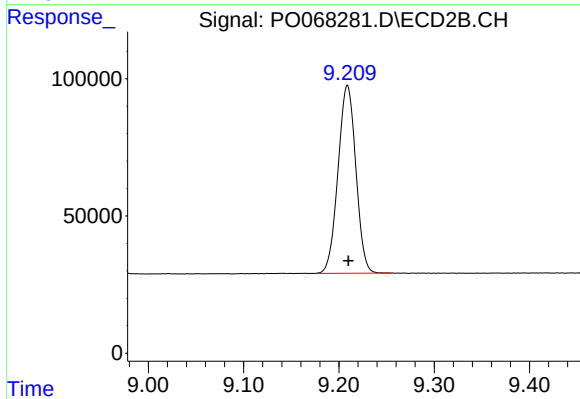

#2 Decachlorobiphenyl

R.T.: 9.209 min
Delta R.T.: -0.001 min
Response: 889392
Conc: 23.10 ng/ml

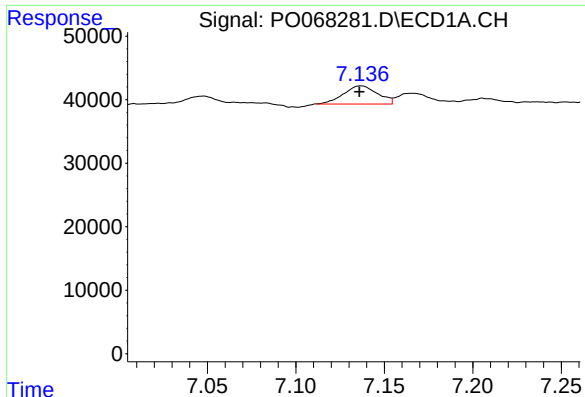


#26 AR-1254-1

R.T.: 7.136 min
Delta R.T.: 0.000 min
Response: 38510
Conc: 32.38 ng/ml m

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2020


Manual Integrations
APPROVED

Sohil
5/12/2020 2:53:39 PM

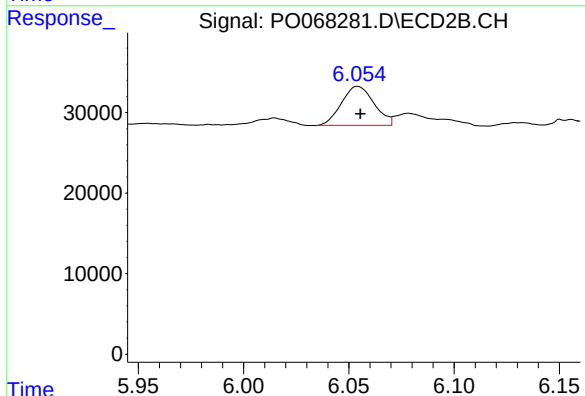


#26 AR-1254-1

R.T.: 6.054 min
Delta R.T.: -0.002 min
Response: 52541
Conc: 25.93 ng/ml m

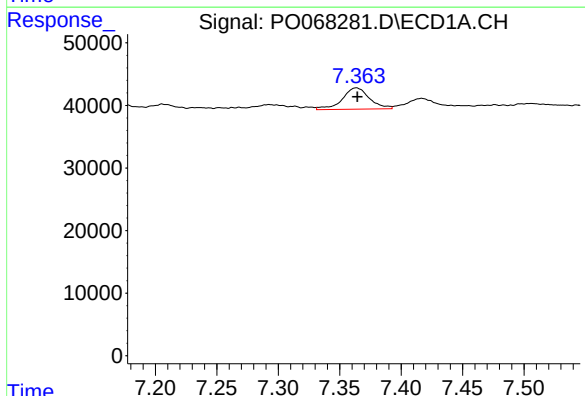


#27 AR-1254-2

R.T.: 7.363 min
Delta R.T.: -0.001 min
Response: 52363
Conc: 28.36 ng/ml

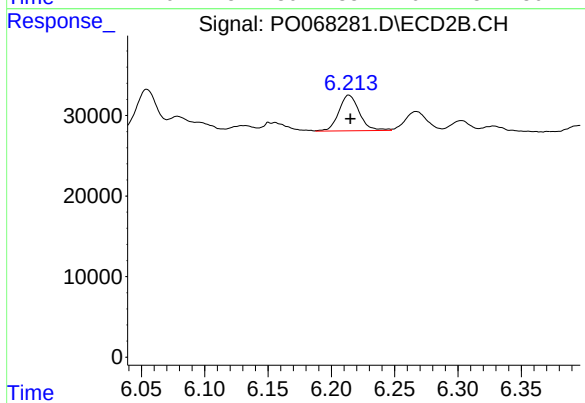

#27 AR-1254-2

R.T.: 6.213 min
Delta R.T.: -0.002 min
Response: 50084
Conc: 27.95 ng/ml m

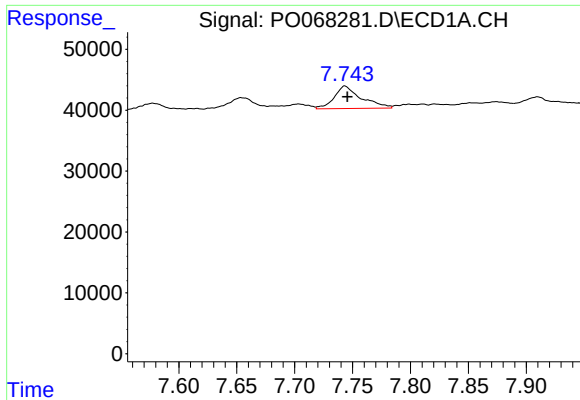


#28 AR-1254-3

R.T.: 7.744 min
Delta R.T.: -0.002 min
Response: 59980
Conc: 30.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2020


Manual Integrations
APPROVED

Sohil
5/12/2020 2:53:39 PM

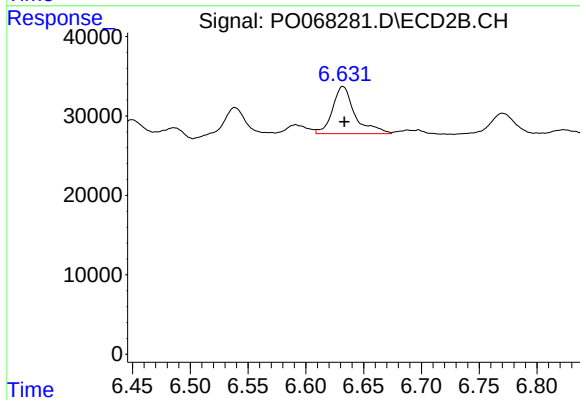


#28 AR-1254-3

R.T.: 6.631 min
Delta R.T.: -0.002 min
Response: 80124
Conc: 27.85 ng/ml m

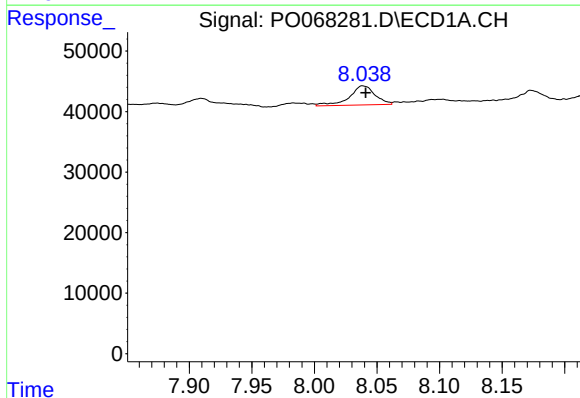


#29 AR-1254-4

R.T.: 8.039 min
Delta R.T.: -0.002 min
Response: 44938
Conc: 28.08 ng/ml

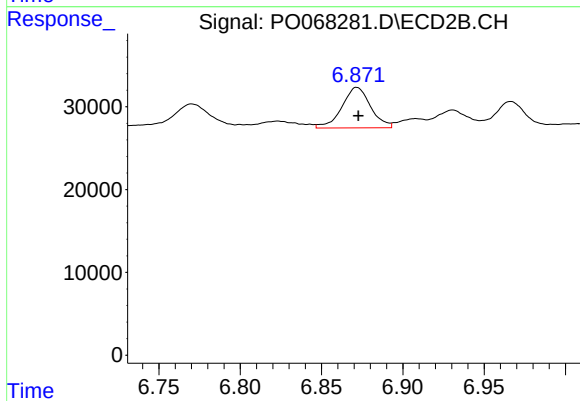

#29 AR-1254-4

R.T.: 6.872 min
Delta R.T.: -0.001 min
Response: 60375
Conc: 31.30 ng/ml

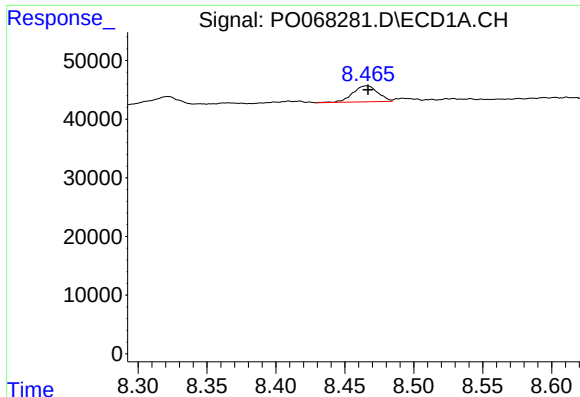


#30 AR-1254-5

R.T.: 8.466 min
Delta R.T.: -0.001 min
Response: 34732
Conc: 21.14 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2020

Manual Integrations
APPROVED

Sohil
5/12/2020 2:53:39 PM

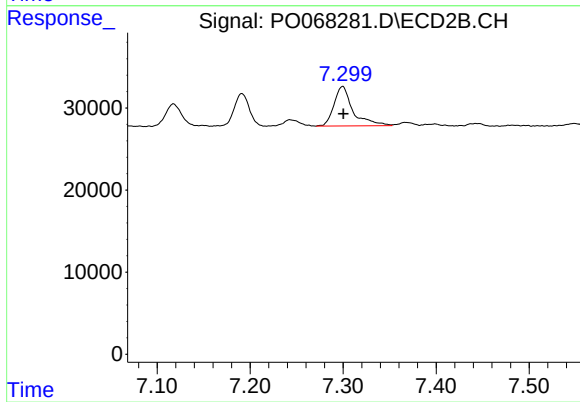

#30 AR-1254-5

R.T.: 7.299 min
Delta R.T.: -0.001 min
Response: 68252
Conc: 25.31 ng/ml