

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051120\
 Data File : P0068285.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 May 2020 15:08
 Operator : DD\AJ
 Sample : L2182-07
 Misc : AR1268 25PPB LOD
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT2-2020

Manual Integrations
 APPROVED

Sohil
 5/12/2020 2:53:42 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 12 00:27:00 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 08 13:29:29 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.918	3.936	452191	552714	16.123	16.107
2)	SA Decachlor...	10.879	9.212	699244	726986	17.572	18.883
Target Compounds							
41)	L9 AR-1268-1	9.398	8.139	133677	200839	28.075m	35.689 #
42)	L9 AR-1268-2	9.495	8.204	123958	162846	27.097	31.832
43)	L9 AR-1268-3	9.715	8.411	115723	140773	29.262	33.203
44)	L9 AR-1268-4	10.147	8.698	42979	65096	24.080	32.165 #
45)	L9 AR-1268-5	10.550	8.974	364272	393995	28.057	29.920

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051120\
Data File : P0068285.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 May 2020 15:08
Operator : DD\AJ
Sample : L2182-07
Misc : AR1268 25PPB LOD
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
LOD-MDL-WATER-01-QT2-2020


Manual Integrations
APPROVED

Sohil
5/12/2020 2:53:42 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 12 00:27:00 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050820.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 08 13:29:29 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

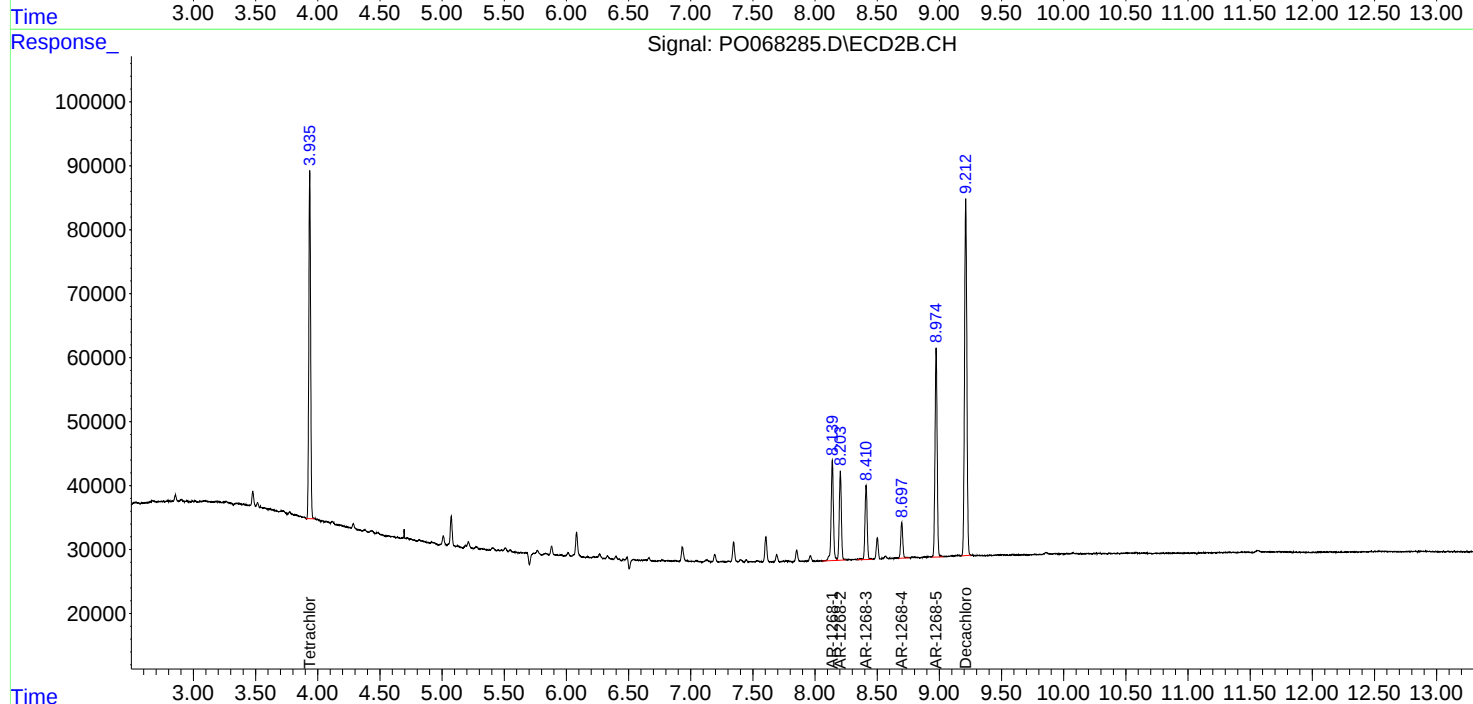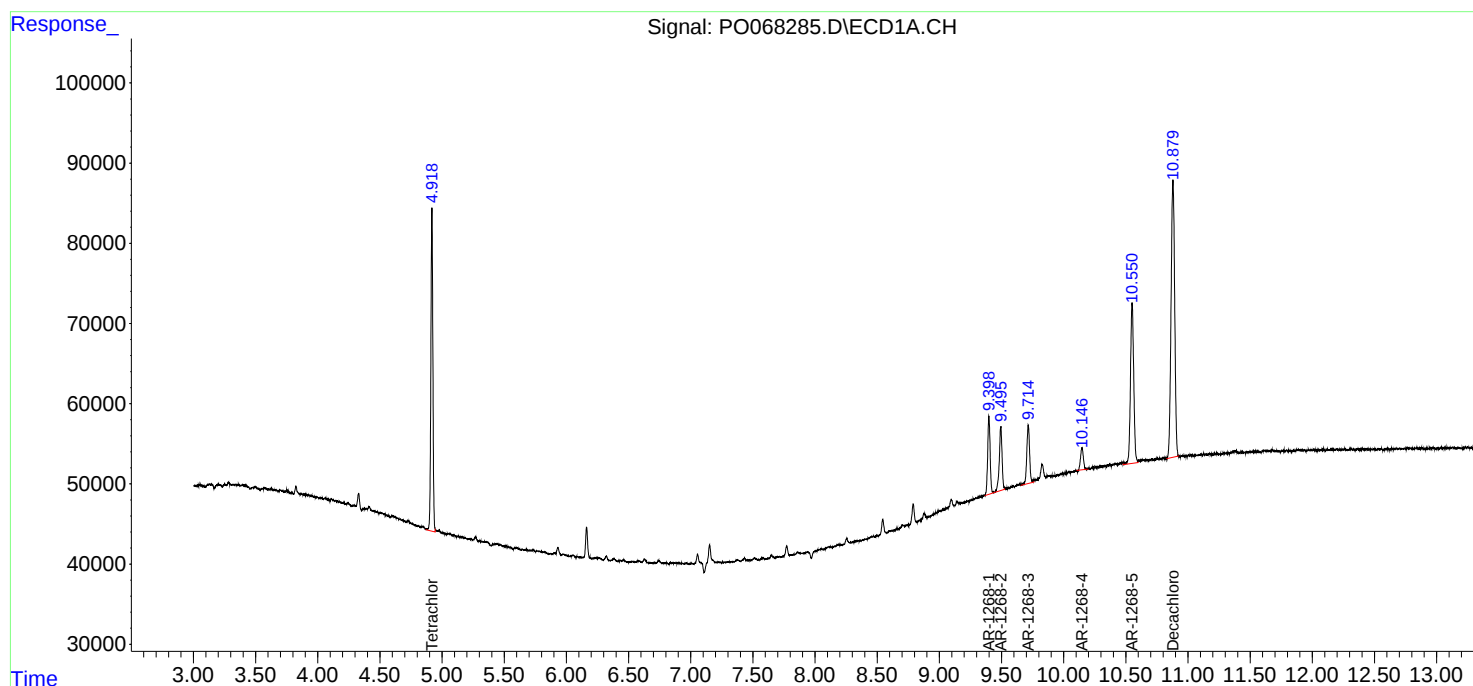

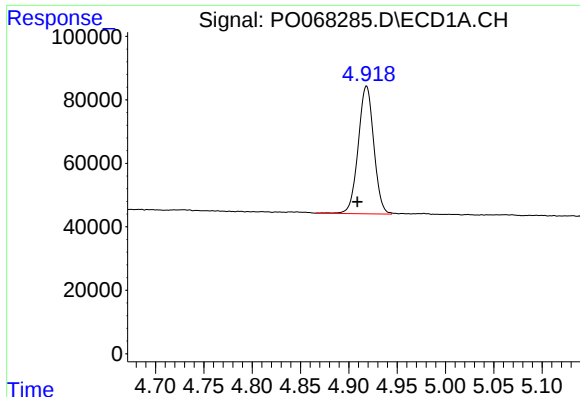


#1 Tetrachloro-m-xylene

R.T.: 4.918 min
Delta R.T.: 0.009 min
Response: 452191
Conc: 16.12 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2020


Manual Integrations
APPROVED

Sohil
5/12/2020 2:53:42 PM

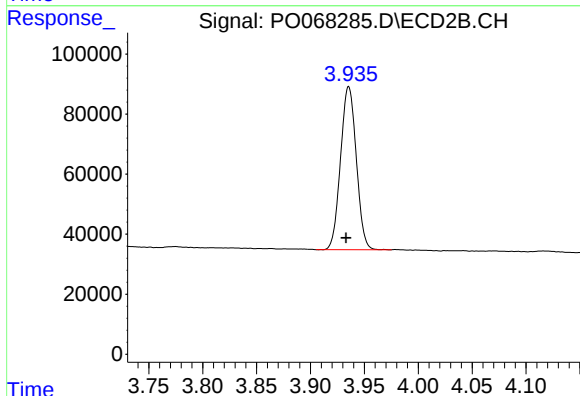


#1 Tetrachloro-m-xylene

R.T.: 3.936 min
Delta R.T.: 0.002 min
Response: 552714
Conc: 16.11 ng/ml

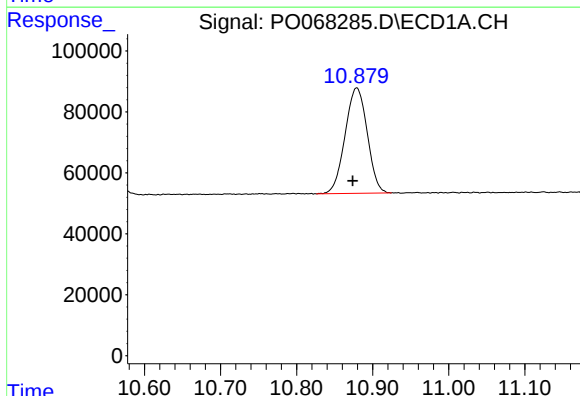


#2 Decachlorobiphenyl

R.T.: 10.879 min
Delta R.T.: 0.005 min
Response: 699244
Conc: 17.57 ng/ml

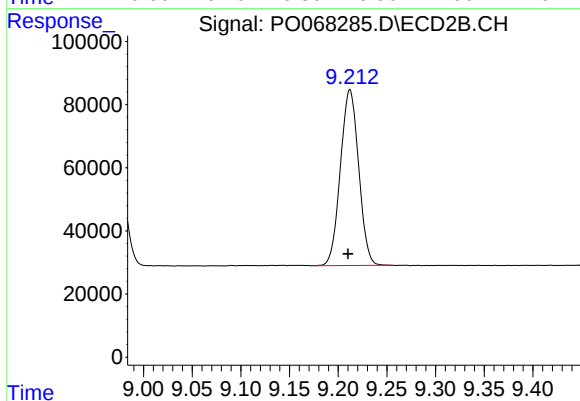

#2 Decachlorobiphenyl

R.T.: 9.212 min
Delta R.T.: 0.002 min
Response: 726986
Conc: 18.88 ng/ml

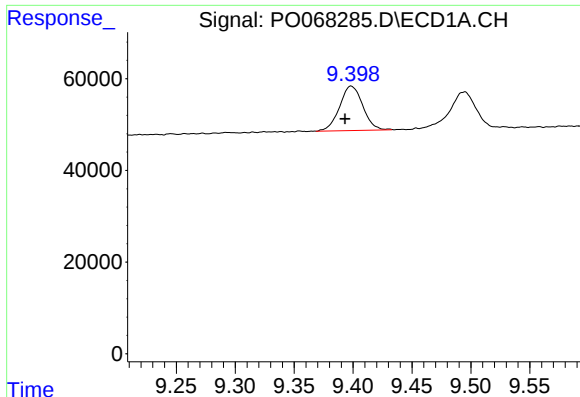


#41 AR-1268-1

R.T.: 9.398 min
Delta R.T.: 0.005 min
Response: 133677
Conc: 28.08 ng/ml m

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2020


Manual Integrations
APPROVED

Sohil
5/12/2020 2:53:42 PM

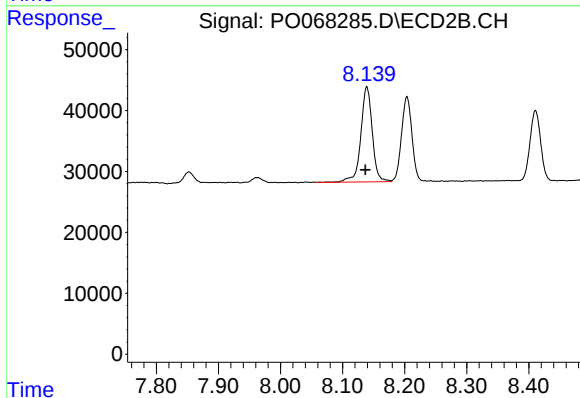


#41 AR-1268-1

R.T.: 8.139 min
Delta R.T.: 0.002 min
Response: 200839
Conc: 35.69 ng/ml

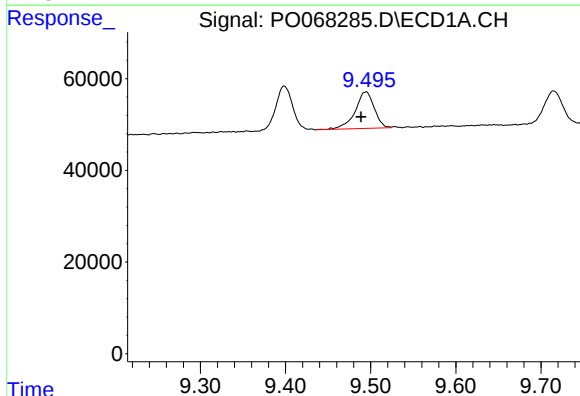


#42 AR-1268-2

R.T.: 9.495 min
Delta R.T.: 0.006 min
Response: 123958
Conc: 27.10 ng/ml

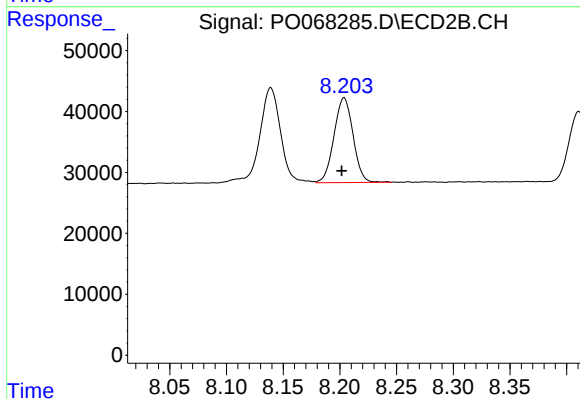

#42 AR-1268-2

R.T.: 8.204 min
Delta R.T.: 0.002 min
Response: 162846
Conc: 31.83 ng/ml

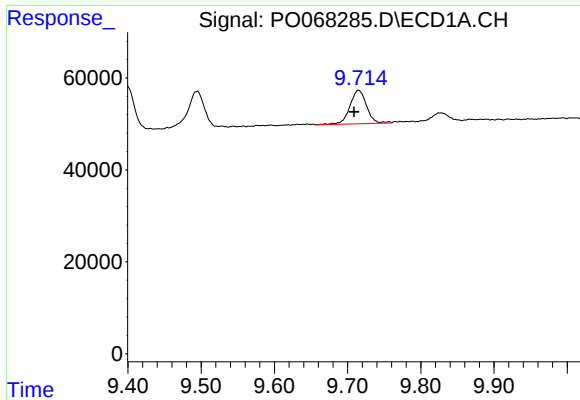


#43 AR-1268-3

R.T.: 9.715 min
Delta R.T.: 0.006 min
Response: 115723
Conc: 29.26 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2020


Manual Integrations
APPROVED

Sohil
5/12/2020 2:53:42 PM

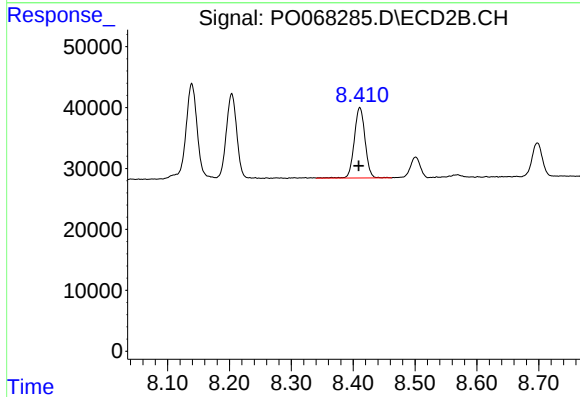


#43 AR-1268-3

R.T.: 8.411 min
Delta R.T.: 0.002 min
Response: 140773
Conc: 33.20 ng/ml

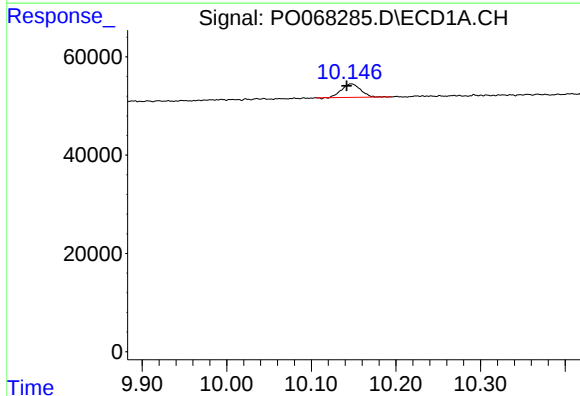


#44 AR-1268-4

R.T.: 10.147 min
Delta R.T.: 0.005 min
Response: 42979
Conc: 24.08 ng/ml

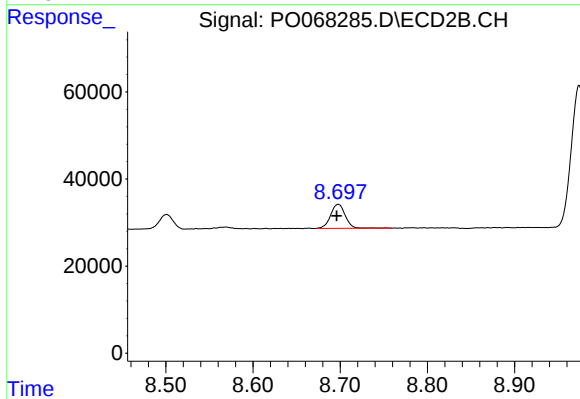

#44 AR-1268-4

R.T.: 8.698 min
Delta R.T.: 0.002 min
Response: 65096
Conc: 32.17 ng/ml

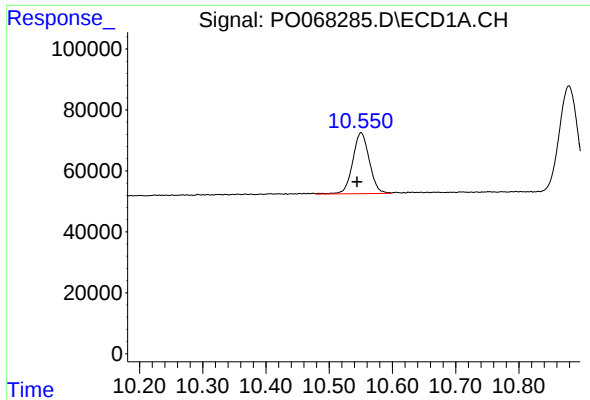


#45 AR-1268-5

R.T.: 10.550 min
Delta R.T.: 0.006 min
Response: 364272
Conc: 28.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2020

Manual Integrations
APPROVED

Sohil
5/12/2020 2:53:42 PM

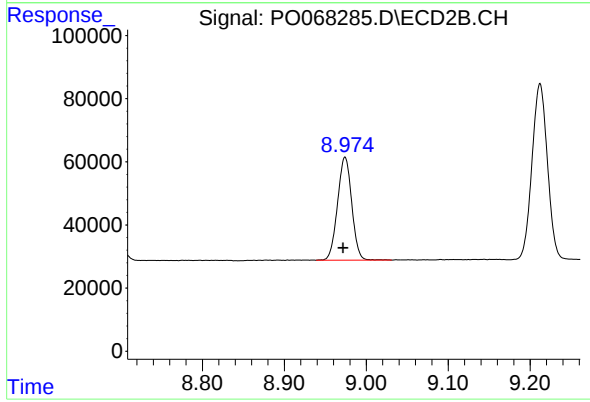

#45 AR-1268-5

R.T.: 8.974 min
Delta R.T.: 0.002 min
Response: 393995
Conc: 29.92 ng/ml