

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051121\
 Data File : P0077679.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 May 2021 14:23
 Operator : DD\AJ
 Sample : PB136261BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB136261BL

Manual Integrations
 APPROVED

Ankita
 5/13/2021 10:46:24 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 11 22:53:47 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue May 11 15:14:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.368	3.647	1424057	353549	20.514m	21.027
2) SA Decachlor...	9.995	8.850	1120421	413243	21.324	23.432

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051121\
Data File : P0077679.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 May 2021 14:23
Operator : DD\AJ
Sample : PB136261BL
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PB136261BL


Manual Integrations
APPROVED

Ankita
5/13/2021 10:46:24 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 11 22:53:47 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue May 11 15:14:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

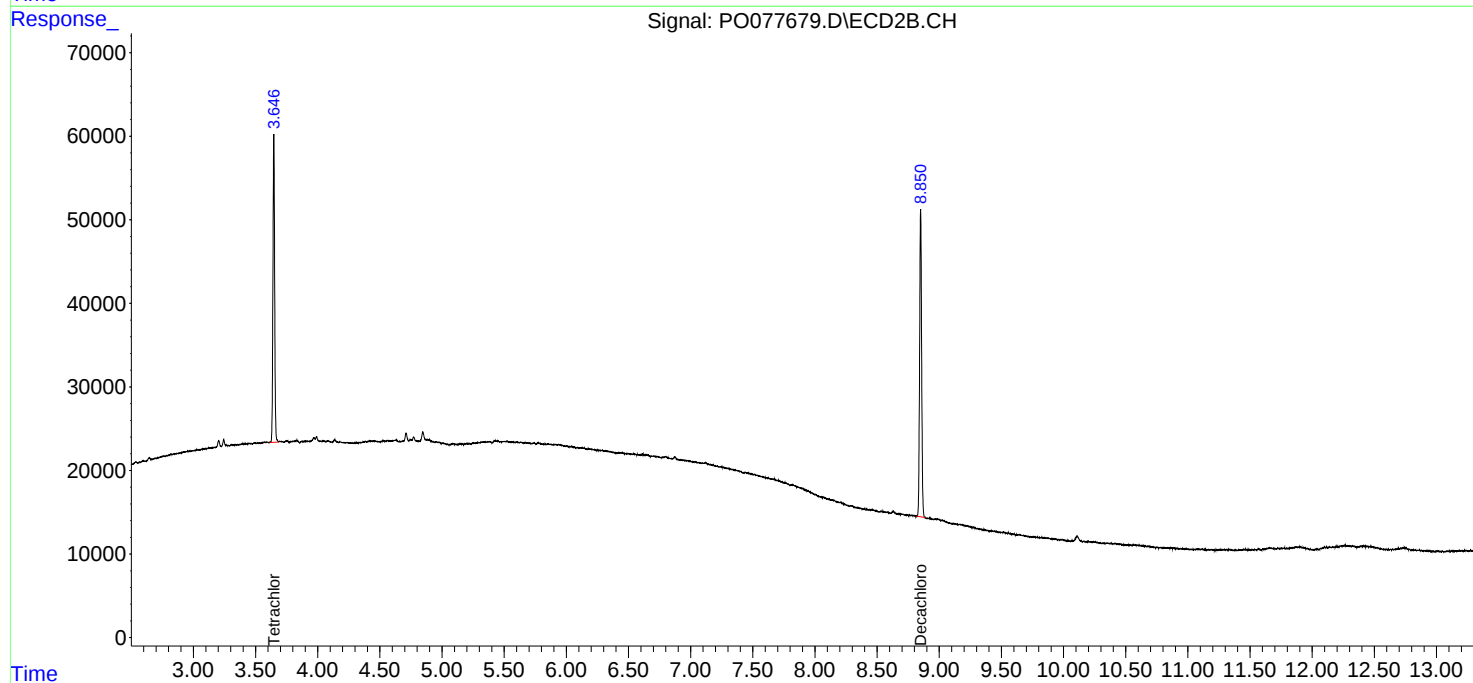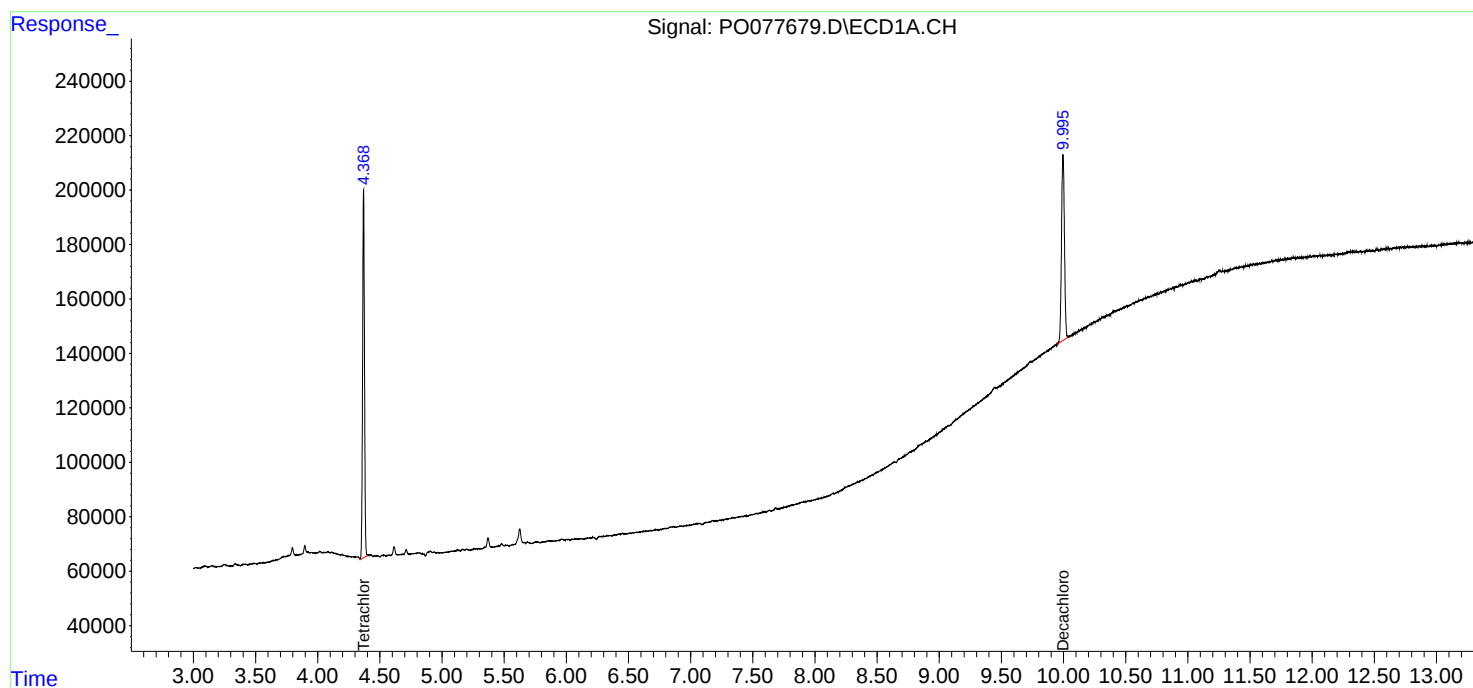

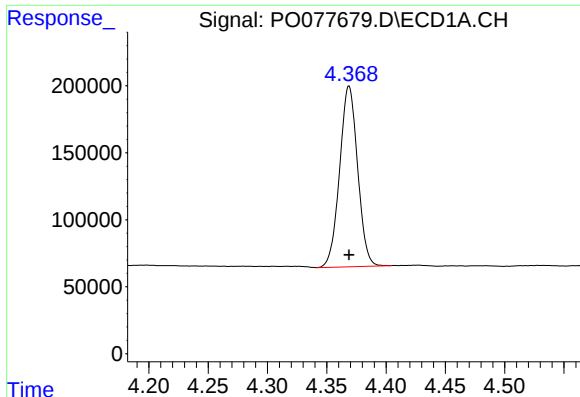


#1 Tetrachloro-m-xylene

R.T.: 4.368 min
Delta R.T.: 0.000 min
Response: 1424057
Conc: 20.51 ng/ml m

Instrument :
ECD_O
ClientSampleId :
PB136261BL


Manual Integrations
APPROVED

Ankita
5/13/2021 10:46:24 AM

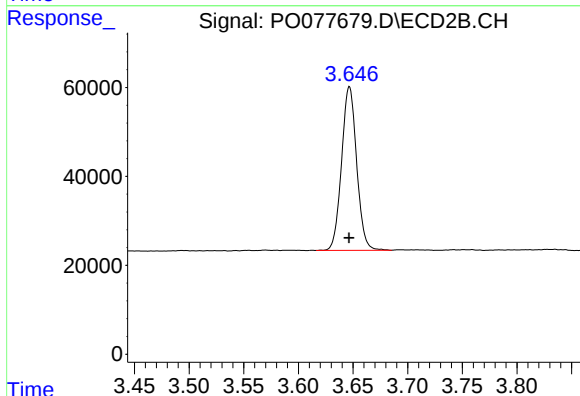


#1 Tetrachloro-m-xylene

R.T.: 3.647 min
Delta R.T.: 0.000 min
Response: 353549
Conc: 21.03 ng/ml

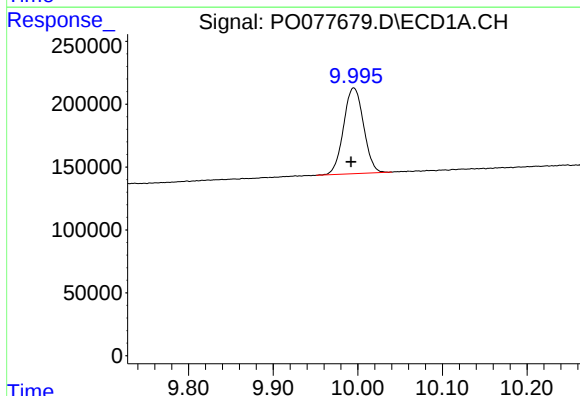

#2 Decachlorobiphenyl

R.T.: 9.995 min
Delta R.T.: 0.003 min
Response: 1120421
Conc: 21.32 ng/ml

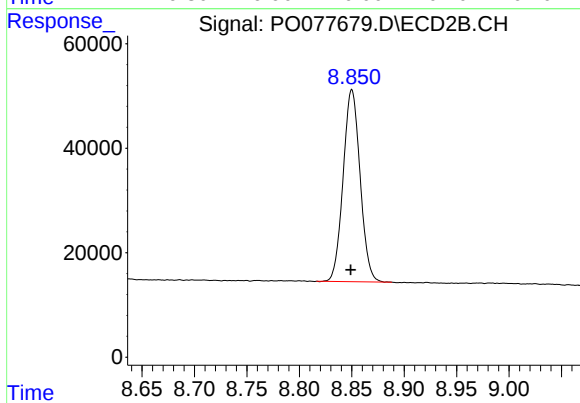

#2 Decachlorobiphenyl

R.T.: 8.850 min
Delta R.T.: 0.001 min
Response: 413243
Conc: 23.43 ng/ml